

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
 Data File : FF010113.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2022 11:10
 Operator : AJ\MA
 Sample : N1962-02 5X
 Misc :
 ALS Vial : 85 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 20 22:28:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.696	520374	3.470 ug/ml
Target Compounds			
7) N-EICOSANE	12.546f	142324	0.820 ug/ml
10) N-TETRACOSANE	14.880	399271	2.364 ug/ml
12) N-OCTACOSANE	16.879	131298	0.820 ug/ml
13) N-TRIACONTANE	17.761	200187	1.303 ug/ml
14) N-DOTRIACONTANE	18.603	259742	1.779 ug/ml
15) N-TETRATRIACONTANE	19.410	246805	1.802 ug/ml
16) N-HEXATRIACONTANE	20.158	512340	4.120 ug/ml
18) N-TETRACONTANE	21.809	1036583	10.102 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010113.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2022 11:10
Operator : AJ\MA
Sample : N1962-02 5X
Misc :
ALS Vial : 85 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 20 22:28:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

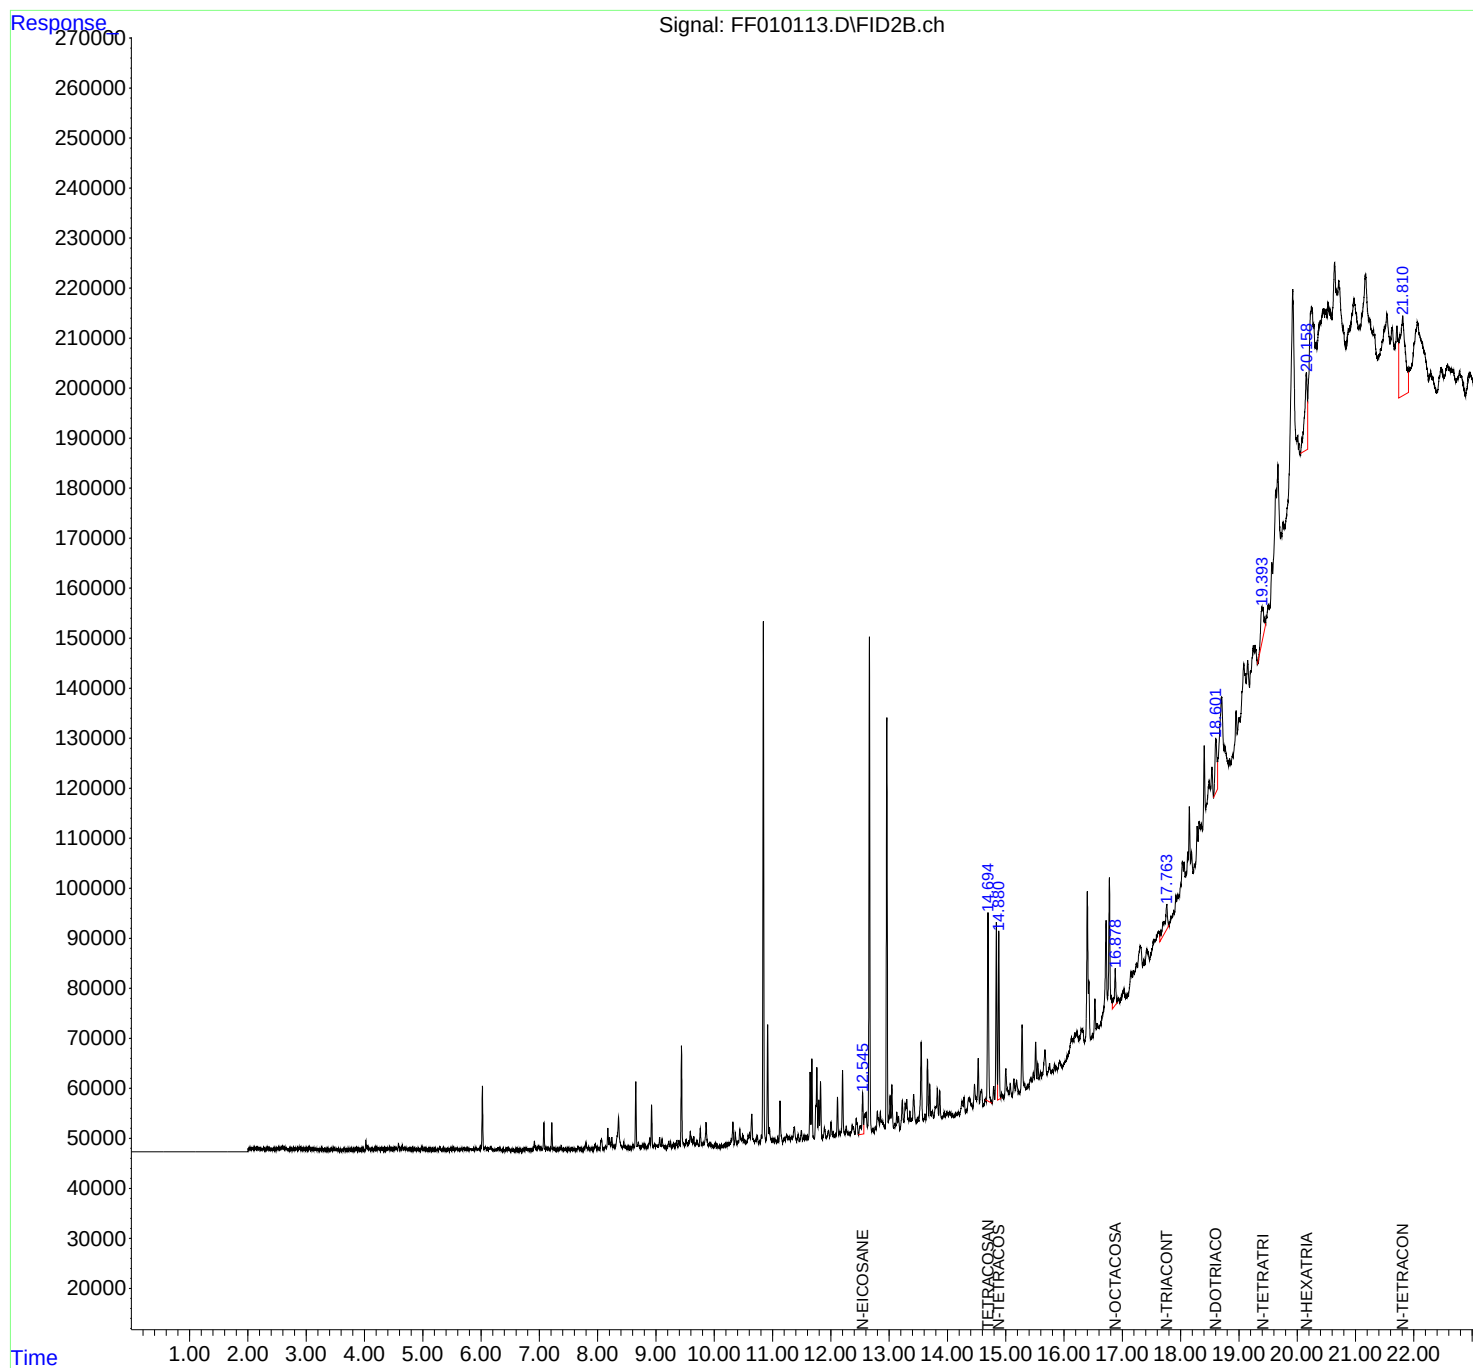


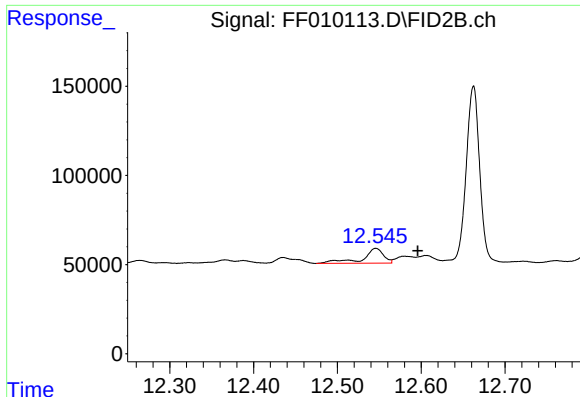

#7 N-EICOSANE


R.T.: 12.546 min
Delta R.T.: -0.050 min
Response: 142324
Conc: 0.82 ug/ml

Instrument :
FID_F
ClientSampleId :

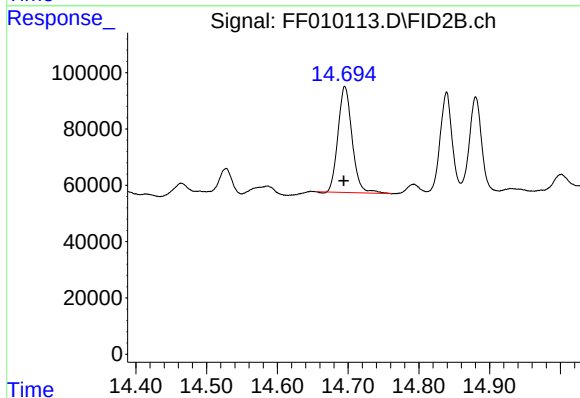


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.696 min
Delta R.T.: 0.002 min
Response: 520374
Conc: 3.47 ug/ml

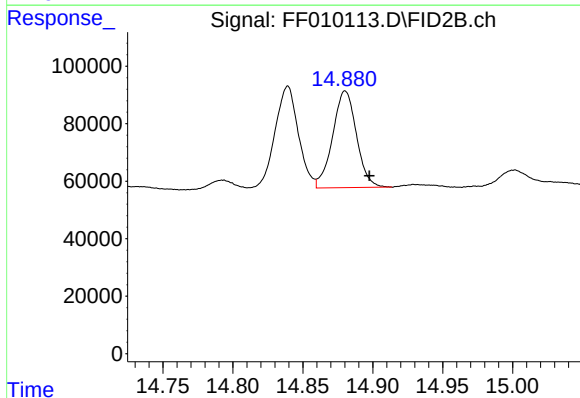


#10 N-TETRACOSANE

R.T.: 14.880 min
Delta R.T.: -0.017 min
Response: 399271
Conc: 2.36 ug/ml

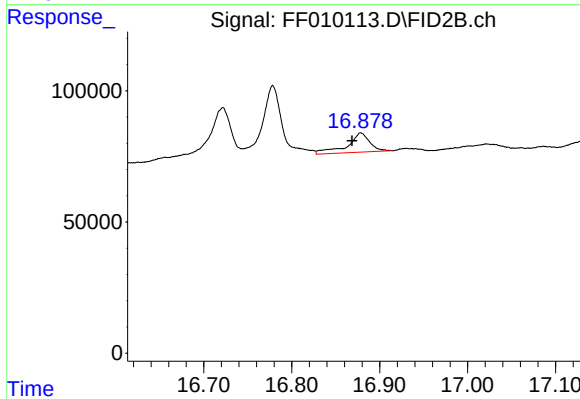

#12 N-OCTACOSANE


R.T.: 16.879 min
Delta R.T.: 0.010 min
Response: 131298
Conc: 0.82 ug/ml

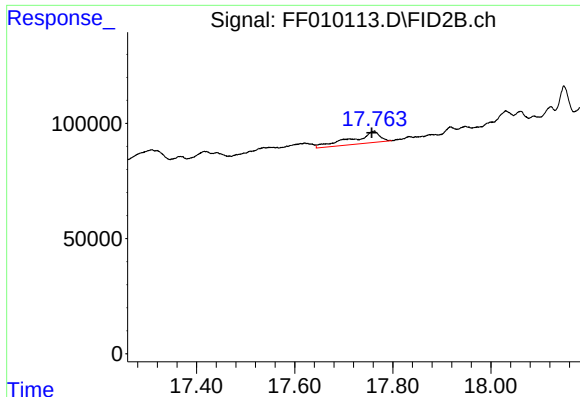

#13 N-TRIACONTANE


R.T.: 17.761 min
Delta R.T.: 0.004 min
Response: 200187
Conc: 1.30 ug/ml

Instrument :
FID_F
ClientSampleId :

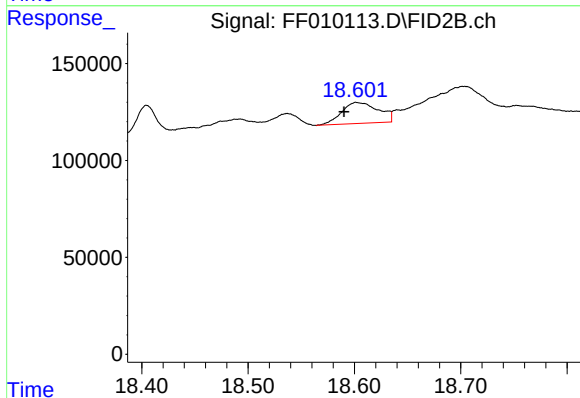


#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: 0.013 min
Response: 259742
Conc: 1.78 ug/ml

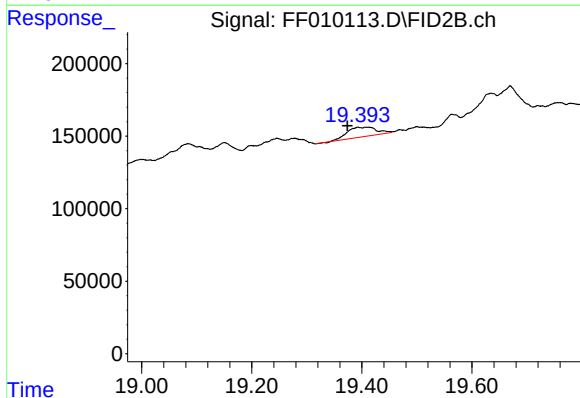


#15 N-TETRATRIACONTANE

R.T.: 19.410 min
Delta R.T.: 0.036 min
Response: 246805
Conc: 1.80 ug/ml

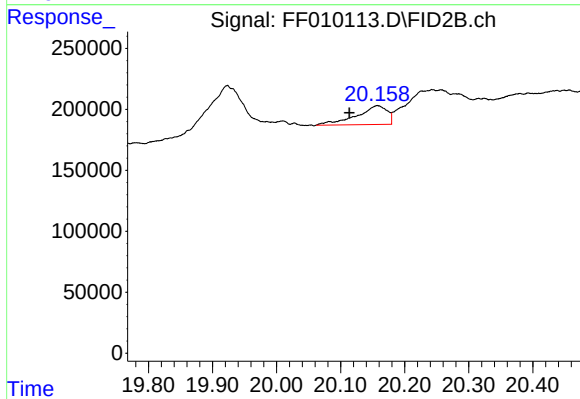

#16 N-HEXATRIACONTANE

R.T.: 20.158 min
Delta R.T.: 0.044 min
Response: 512340
Conc: 4.12 ug/ml

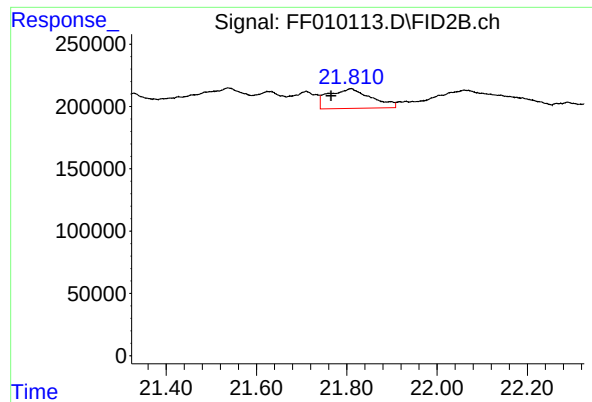

#18 N-TETRACONTANE

R.T.: 21.809 min
Delta R.T.: 0.044 min
Response: 1036583
Conc: 10.10 ug/ml

Instrument :

FID_F

ClientSampleId :