

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
 Data File : FF010116.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2022 12:40
 Operator : AJ\MA
 Sample : N1962-07 5X
 Misc :
 ALS Vial : 88 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 20 22:28:39 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.695	374228	2.495 ug/ml
Target Compounds			
5) N-HEXADECANE	9.858	125416	0.720 ug/ml
7) N-EICOSANE	12.544f	184620	1.063 ug/ml
8) N-DOCOSANE	13.795	119562	0.699 ug/ml
10) N-TETRACOSANE	14.880	912766	5.404 ug/ml
12) N-OCTACOSANE	16.878	230099	1.438 ug/ml
13) N-TRIACONTANE	17.760	177358	1.155 ug/ml
15) N-TETRATRIACONTANE	19.379	20010	0.146 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031822\
Data File : FF010116.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2022 12:40
Operator : AJ\MA
Sample : N1962-07 5X
Misc :
ALS Vial : 88 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 20 22:28:39 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

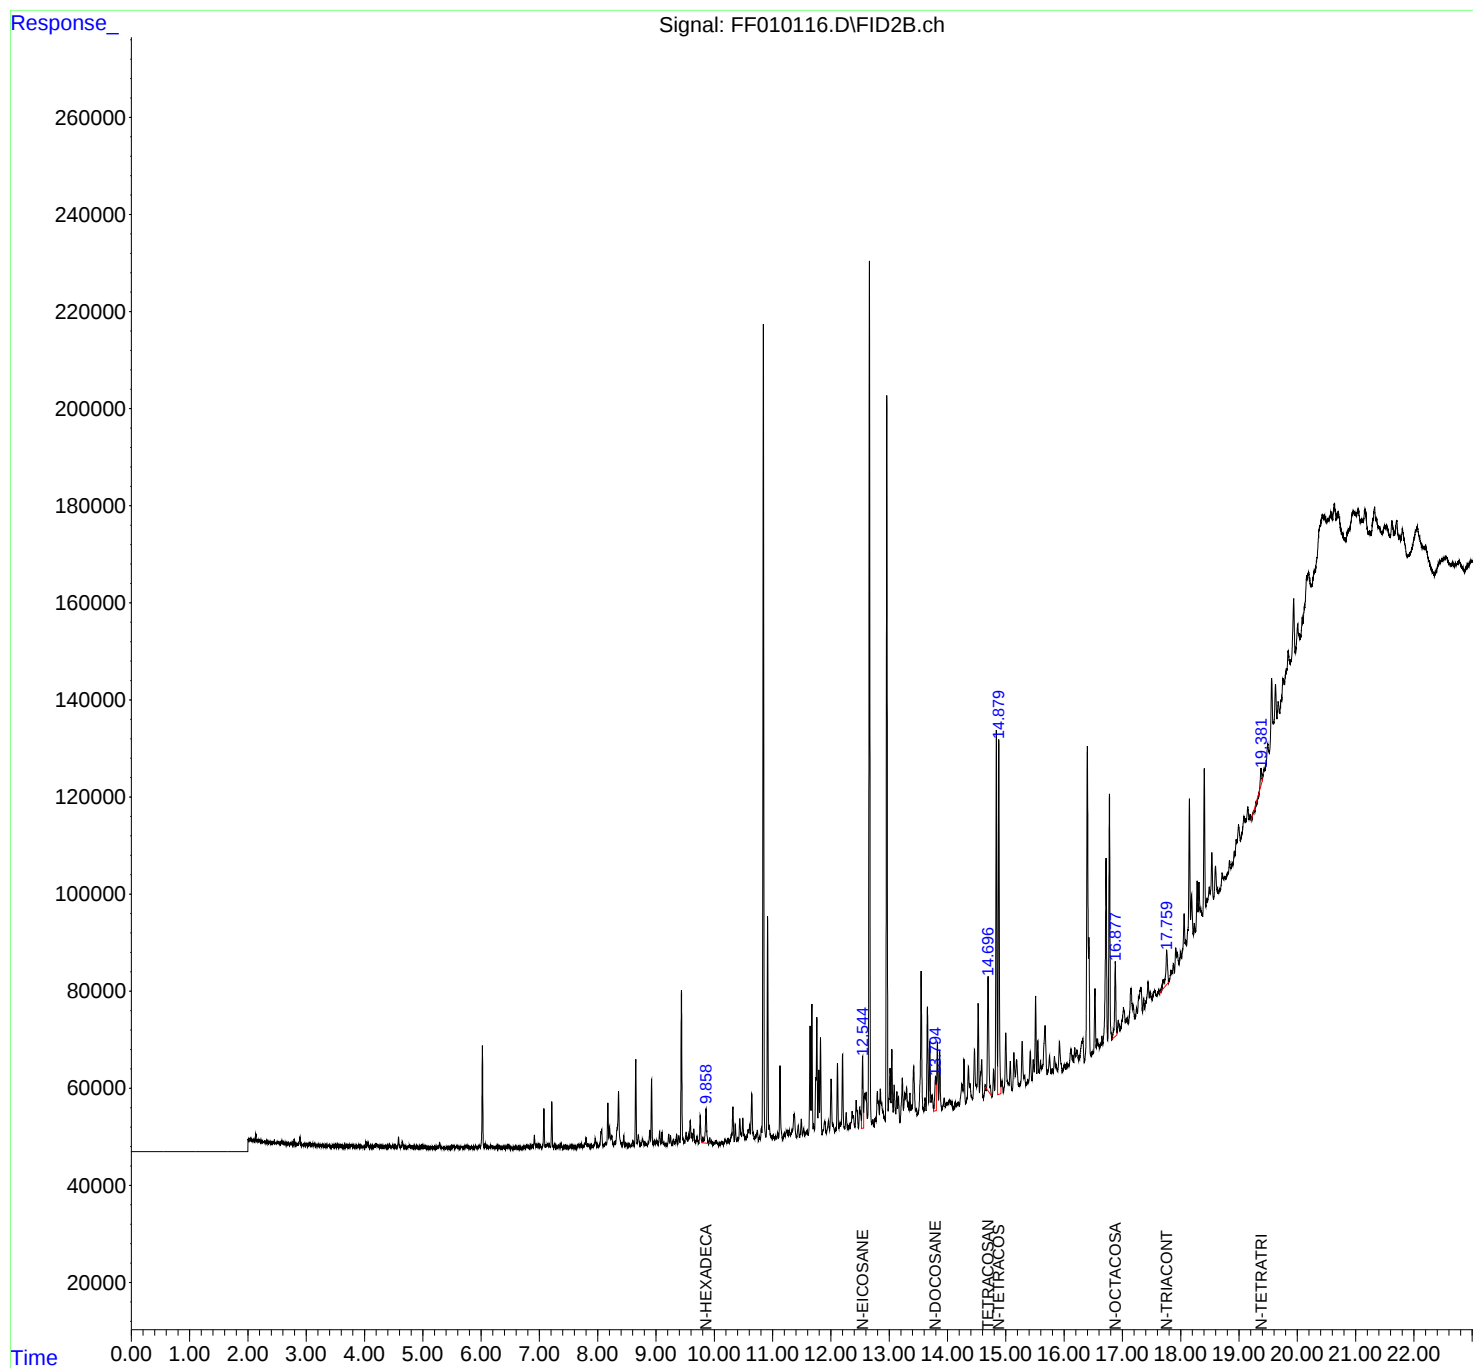


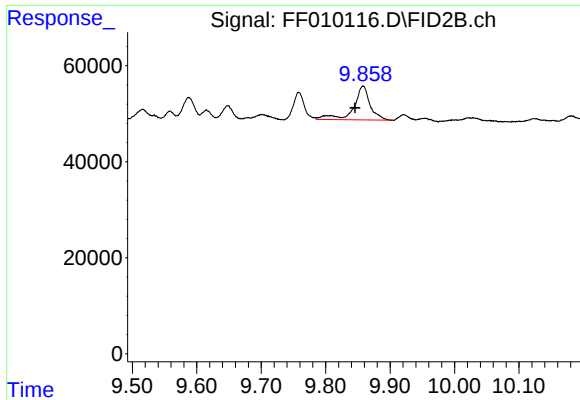

#5 N-HEXADECANE


R.T.: 9.858 min
Delta R.T.: 0.012 min
Response: 125416
Conc: 0.72 ug/ml

Instrument :
FID_F
ClientSampleId :

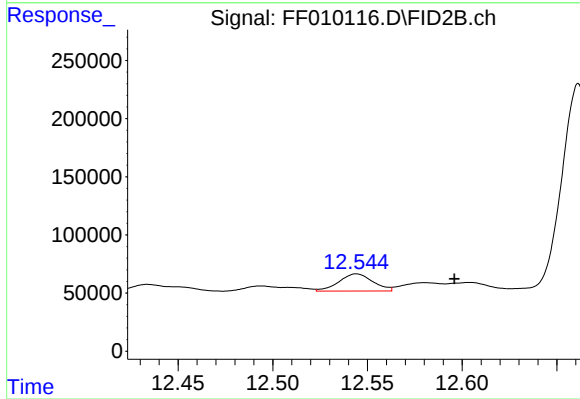


#7 N-EICOSANE

R.T.: 12.544 min
Delta R.T.: -0.052 min
Response: 184620
Conc: 1.06 ug/ml

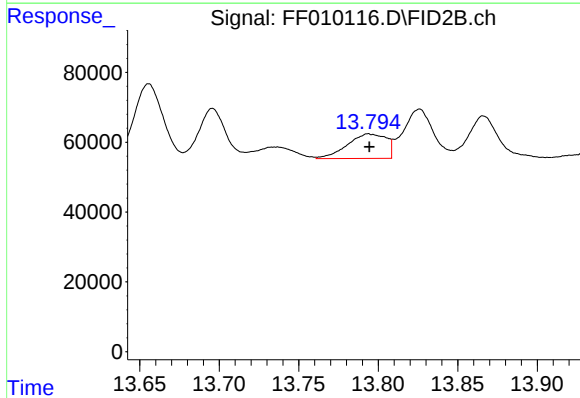


#8 N-DOCOSANE

R.T.: 13.795 min
Delta R.T.: 0.000 min
Response: 119562
Conc: 0.70 ug/ml

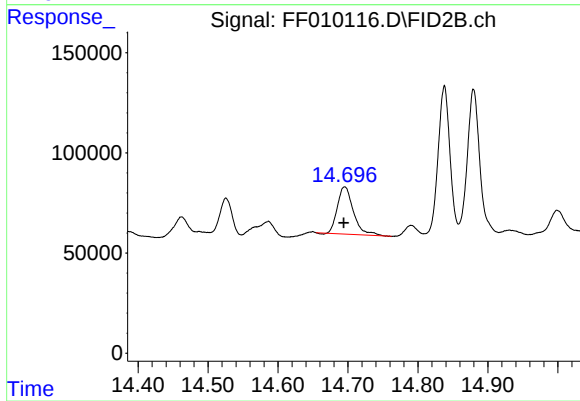

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.695 min
Delta R.T.: 0.001 min
Response: 374228
Conc: 2.50 ug/ml

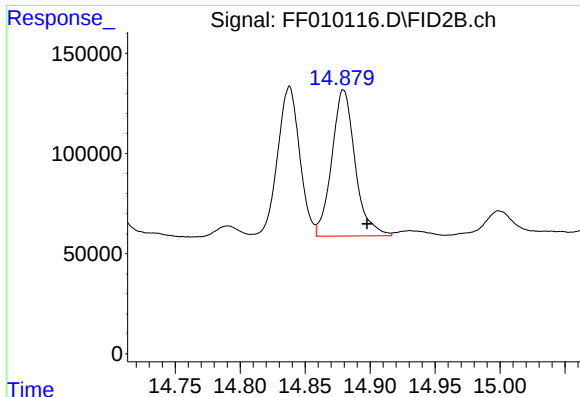

#10 N-TETRACOSANE


R.T.: 14.880 min
Delta R.T.: -0.018 min
Response: 912766
Conc: 5.40 ug/ml

Instrument :
FID_F
ClientSampleId :

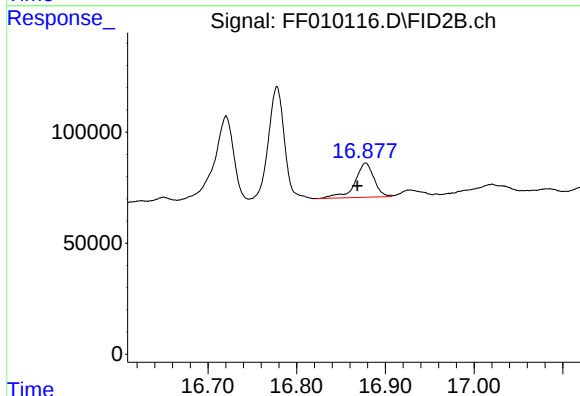


#12 N-OCTACOSANE

R.T.: 16.878 min
Delta R.T.: 0.009 min
Response: 230099
Conc: 1.44 ug/ml

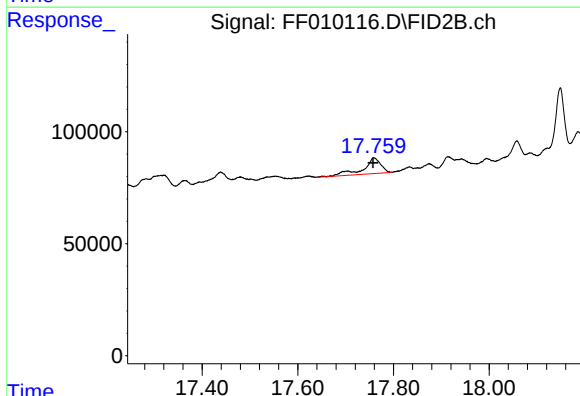

#13 N-TRIACONTANE

R.T.: 17.760 min
Delta R.T.: 0.002 min
Response: 177358
Conc: 1.15 ug/ml

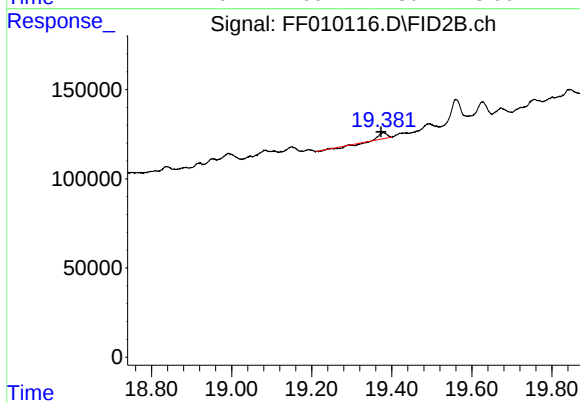

#15 N-TETRATRIACONTANE

R.T.: 19.379 min
Delta R.T.: 0.006 min
Response: 20010
Conc: 0.15 ug/ml