

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003886.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 10:33
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 22:36:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.582	2369915	17.022 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.650	104200	0.708 ug/ml
14)	N-DOTRIACONTANE	18.489	178032	1.252 ug/ml
16)	N-HEXATRIACONTANE	20.053	530744	4.068 ug/ml
18)	N-TETRACONTANE	21.653	407694	3.277 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003886.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 10:33
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 19 22:36:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

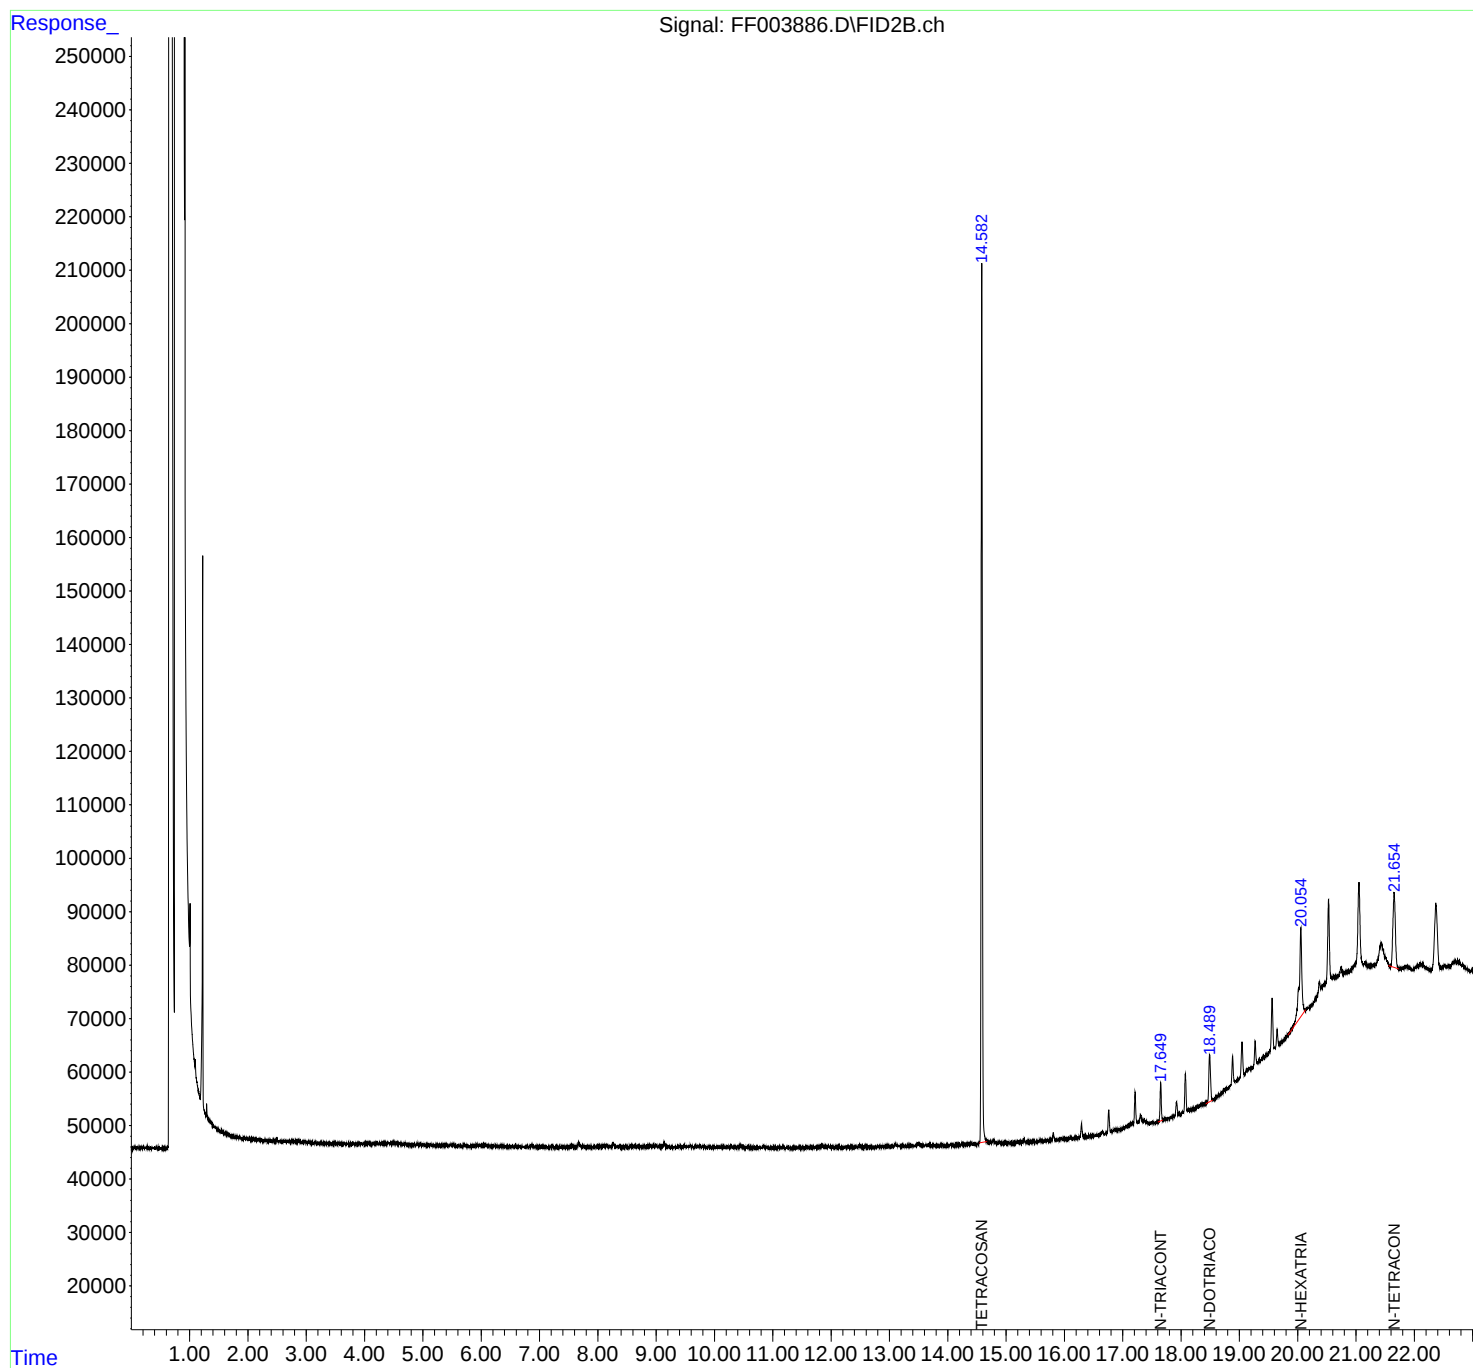


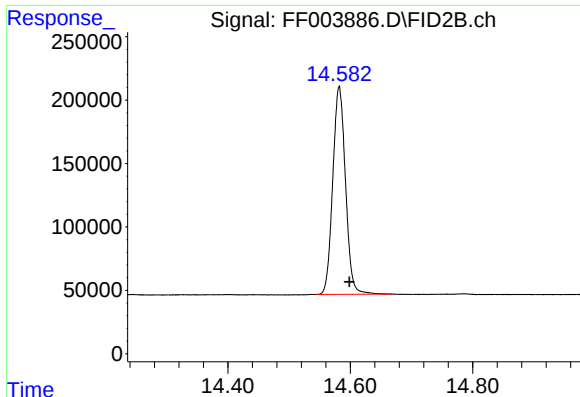

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.582 min
Delta R.T.: -0.016 min
Response: 2369915
Conc: 17.02 ug/ml

Instrument :
FID_F
ClientSampleId :

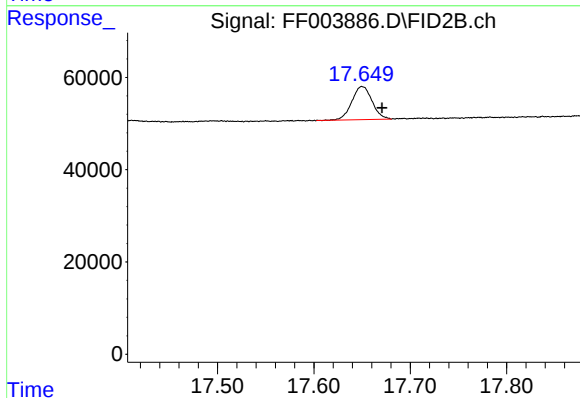


#13 N-TRIACONTANE

R.T.: 17.650 min
Delta R.T.: -0.021 min
Response: 104200
Conc: 0.71 ug/ml

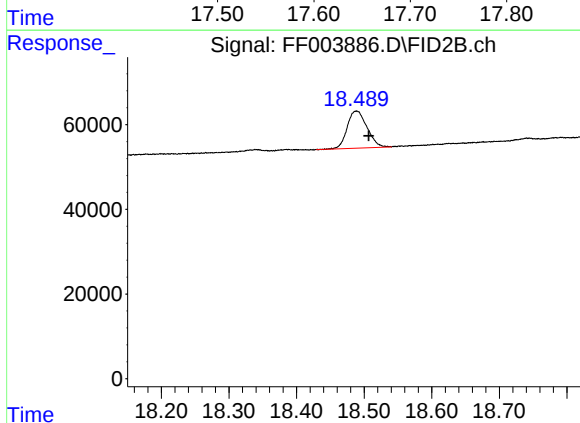


#14 N-DOTRIACONTANE

R.T.: 18.489 min
Delta R.T.: -0.018 min
Response: 178032
Conc: 1.25 ug/ml

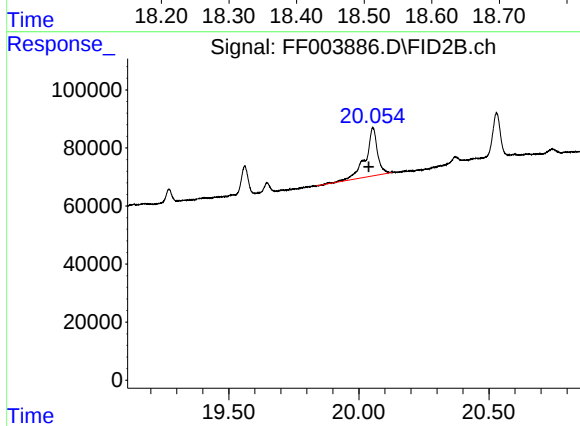

#16 N-HEXATRIACONTANE

R.T.: 20.053 min
Delta R.T.: 0.015 min
Response: 530744
Conc: 4.07 ug/ml

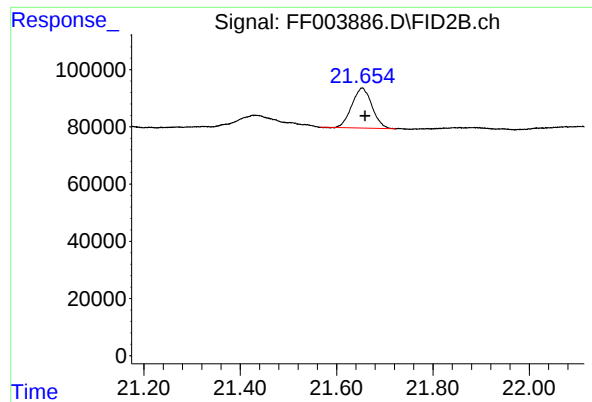

#18 N-TETRACONTANE

R.T.: 21.653 min
Delta R.T.: -0.005 min
Response: 407694
Conc: 3.28 ug/ml

Instrument :
FID_F
ClientSampleId :