

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003889.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 13:13
 Operator : AJ\SJ
 Sample : K1697-11 5X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 22:37:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.580	706239	5.073 ug/ml
Target Compounds			
5) N-HEXADECANE	9.725	102528	0.630 ug/ml
6) N-OCTADECANE	11.248f	159420	0.968 ug/ml
7) N-EICOSANE	12.479	193035	1.180 ug/ml
8) N-DOCOSANE	13.701	212655	1.318 ug/ml
10) N-TETRACOSANE	14.758	1238157	7.826 ug/ml
11) N-HEXACOSANE	15.808	193921	1.256 ug/ml
12) N-OCTACOSANE	16.770	520273	3.443 ug/ml
13) N-TRIACONTANE	17.687	104621	0.711 ug/ml
14) N-DOTRIACONTANE	18.486	343306	2.414 ug/ml
15) N-TETRATRIACONTANE	19.279	605081	4.519 ug/ml
16) N-HEXATRIACONTANE	20.063	925802	7.095 ug/ml
17) N-OCTATRIACONTANE	20.748	145298	1.258 ug/ml
18) N-TETRACONTANE	21.650	330160	2.654 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003889.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 13:13
Operator : AJ\SJ
Sample : K1697-11 5X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 22:37:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

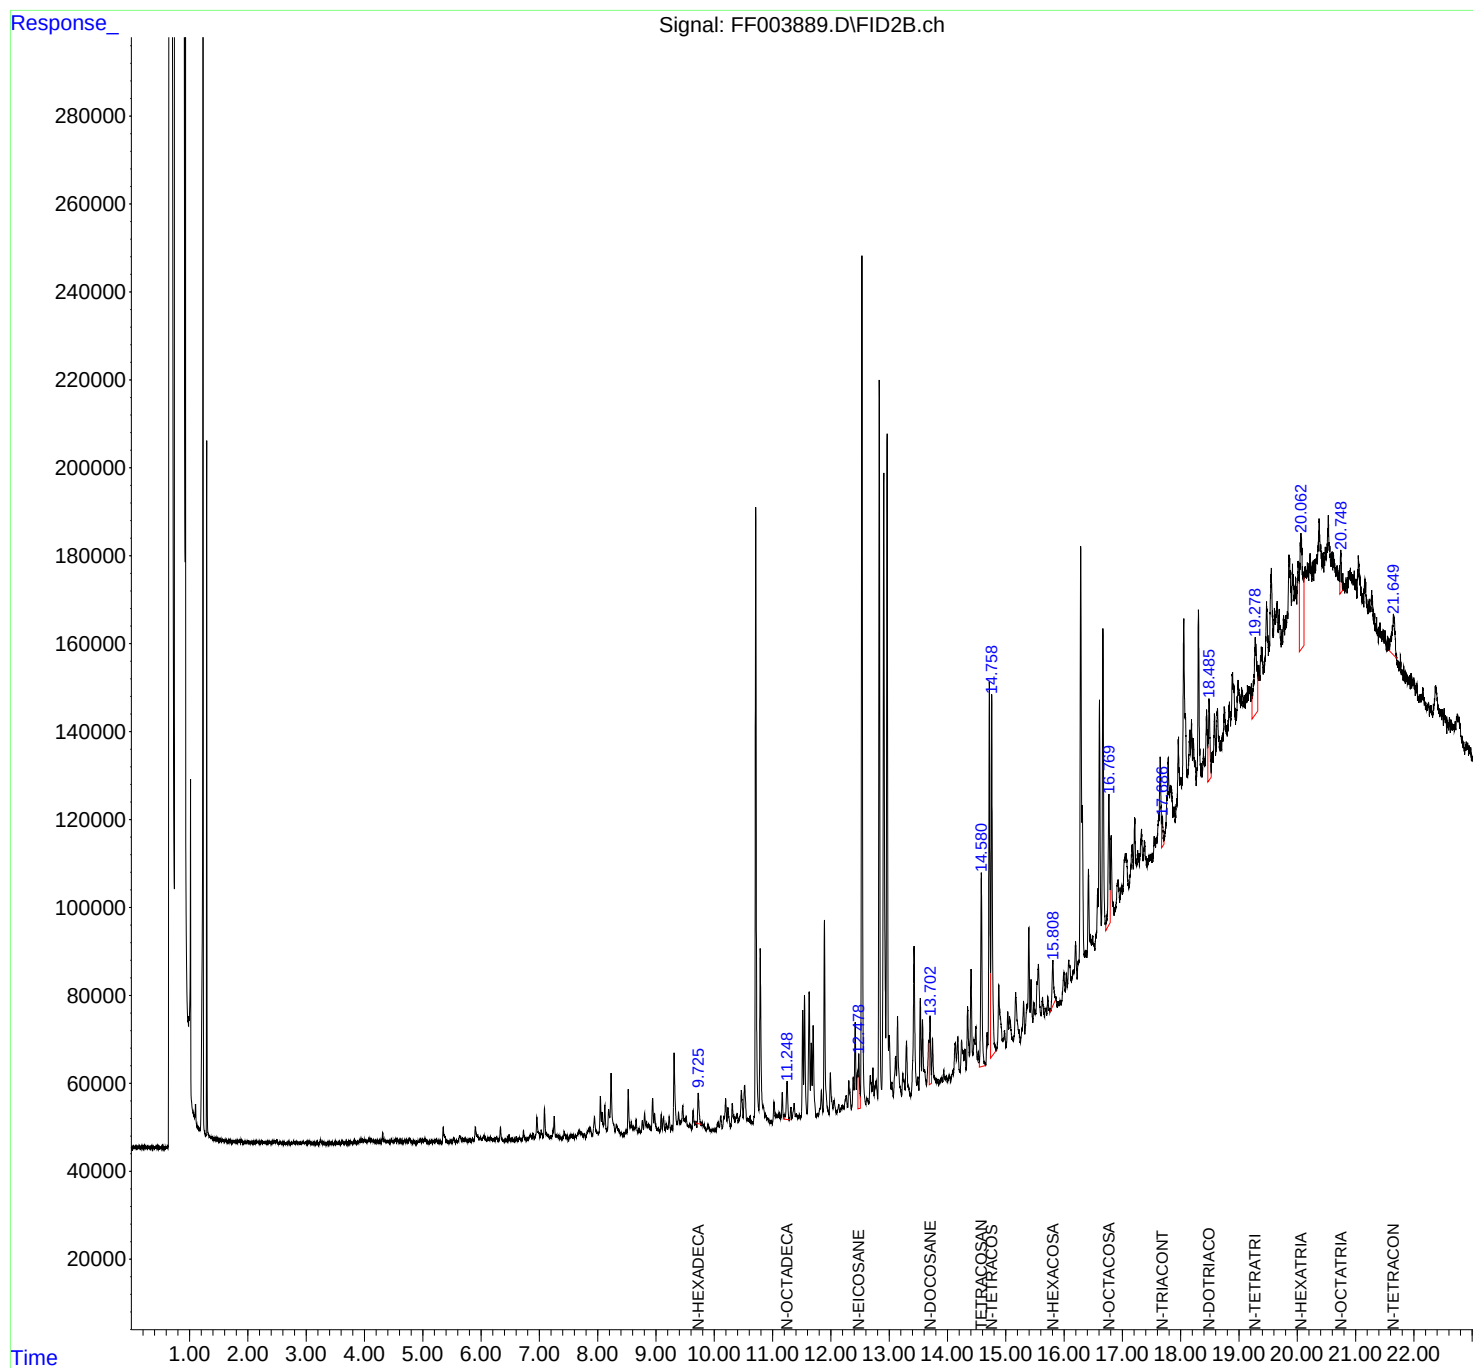


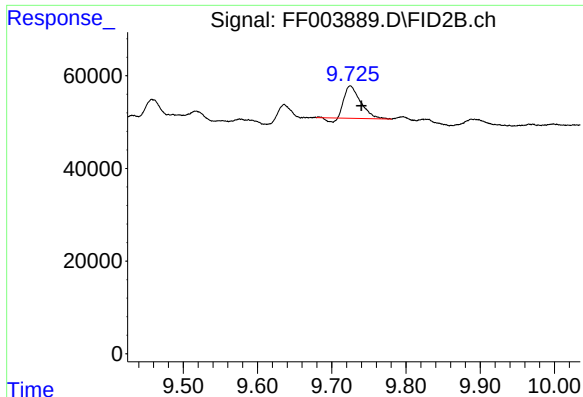

#5 N-HEXADECANE


R.T.: 9.725 min
Delta R.T.: -0.015 min
Response: 102528
Conc: 0.63 ug/ml

Instrument :
FID_F
ClientSampleId :

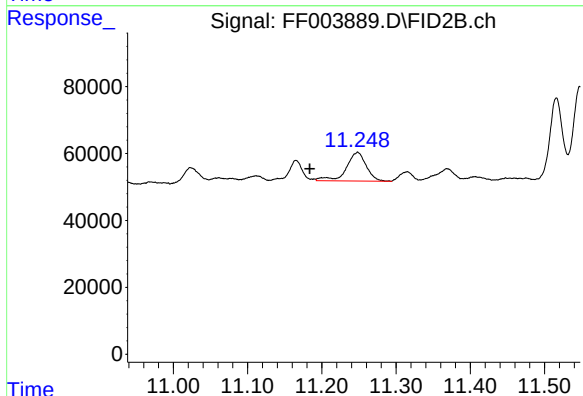


#6 N-OCTADECANE

R.T.: 11.248 min
Delta R.T.: 0.065 min
Response: 159420
Conc: 0.97 ug/ml

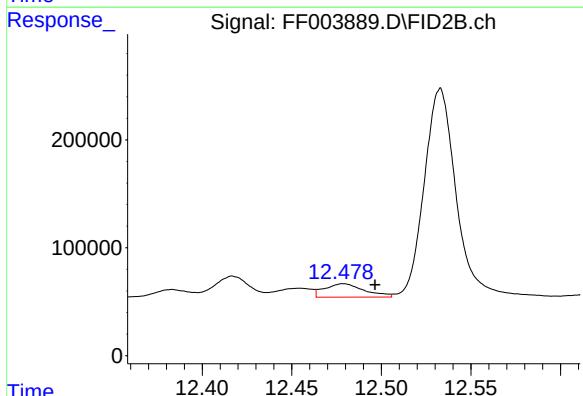


#7 N-EICOSANE

R.T.: 12.479 min
Delta R.T.: -0.018 min
Response: 193035
Conc: 1.18 ug/ml

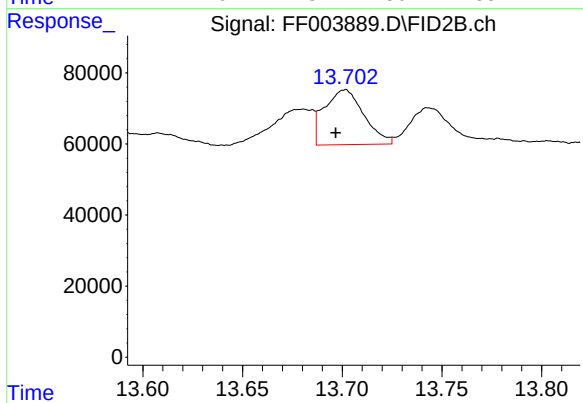

#8 N-DOCOSANE


R.T.: 13.701 min
Delta R.T.: 0.005 min
Response: 212655
Conc: 1.32 ug/ml

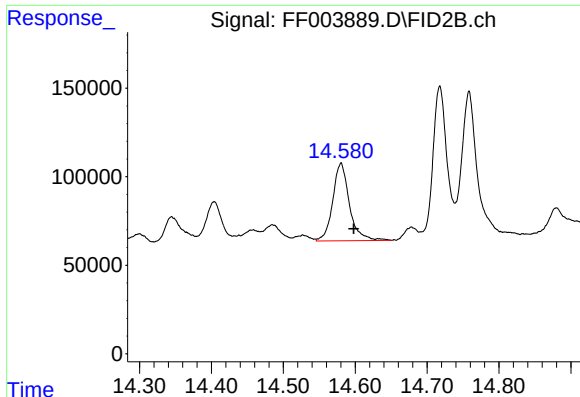

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.580 min
Delta R.T.: -0.018 min
Response: 706239
Conc: 5.07 ug/ml

Instrument :
FID_F
ClientSampleId :

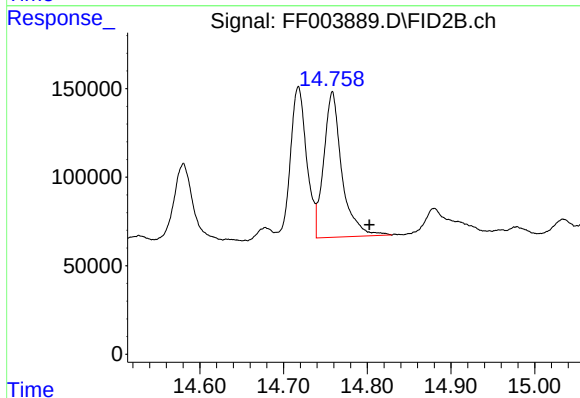


#10 N-TETRACOSANE

R.T.: 14.758 min
Delta R.T.: -0.044 min
Response: 1238157
Conc: 7.83 ug/ml

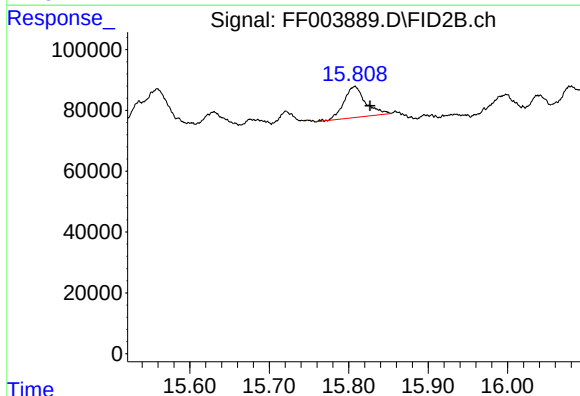


#11 N-HEXACOSANE

R.T.: 15.808 min
Delta R.T.: -0.019 min
Response: 193921
Conc: 1.26 ug/ml

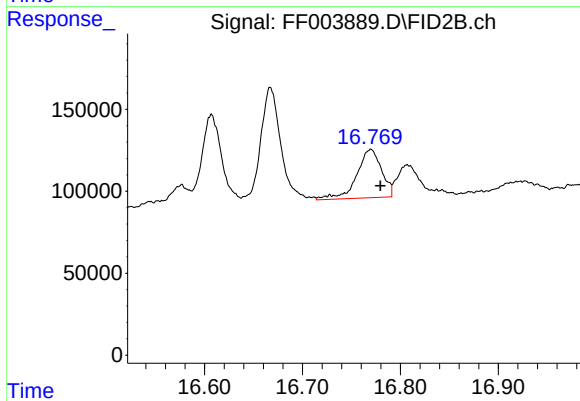

#12 N-OCTACOSANE


R.T.: 16.770 min
Delta R.T.: -0.010 min
Response: 520273
Conc: 3.44 ug/ml

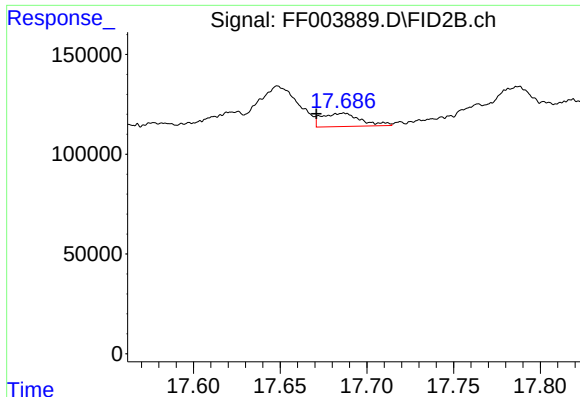

#13 N-TRIACONTANE


R.T.: 17.687 min
Delta R.T.: 0.016 min
Response: 104621
Conc: 0.71 ug/ml

Instrument :
FID_F
ClientSampleId :

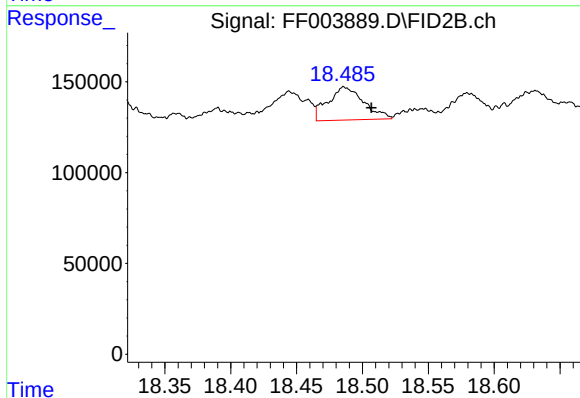


#14 N-DOTRIACONTANE

R.T.: 18.486 min
Delta R.T.: -0.021 min
Response: 343306
Conc: 2.41 ug/ml

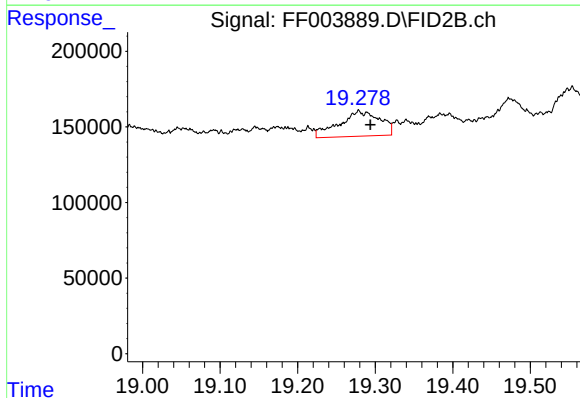


#15 N-TETRATRIACONTANE

R.T.: 19.279 min
Delta R.T.: -0.015 min
Response: 605081
Conc: 4.52 ug/ml

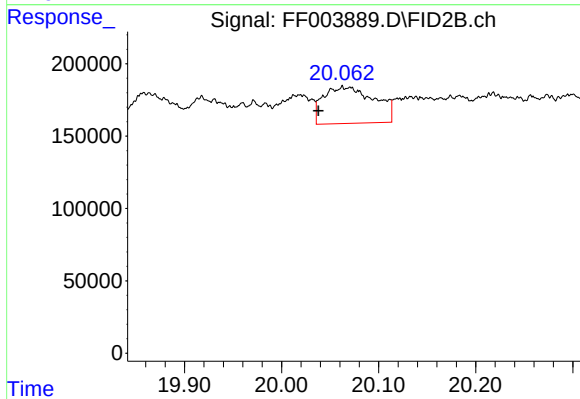

#16 N-HEXATRIACONTANE


R.T.: 20.063 min
Delta R.T.: 0.025 min
Response: 925802
Conc: 7.10 ug/ml

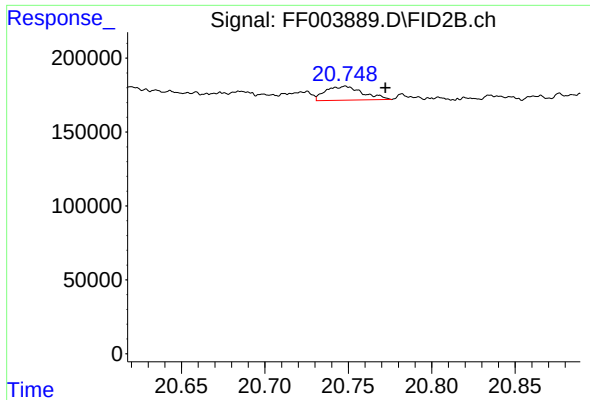

#17 N-OCTATRIACONTANE

R.T.: 20.748 min
Delta R.T.: -0.024 min
Response: 145298
Conc: 1.26 ug/ml

Instrument :
FID_F
ClientSampleId :

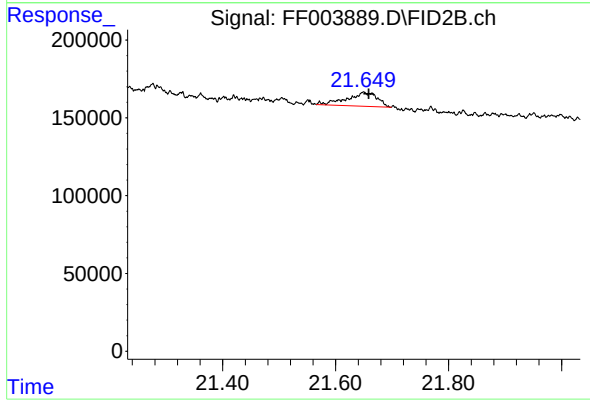

#18 N-TETRACONTANE

R.T.: 21.650 min
Delta R.T.: -0.009 min
Response: 330160
Conc: 2.65 ug/ml