

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003892.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 16:32
 Operator : AJ\SJ
 Sample : K1693-09 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 22:38:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.590	147589	1.060 ug/ml
Target Compounds			
4) N-TETRADECANE	8.132	155109	0.967 ug/ml
5) N-HEXADECANE	9.732	222956	1.369 ug/ml
6) N-OCTADECANE	11.174	176324	1.070 ug/ml
7) N-EICOSANE	12.487	175632	1.074 ug/ml
8) N-DOCOSANE	13.689	57142	0.354 ug/ml
10) N-TETRACOSANE	14.790	243009	1.536 ug/ml
11) N-HEXACOSANE	15.818	426105	2.761 ug/ml
12) N-OCTACOSANE	16.774	349342	2.312 ug/ml
13) N-TRIACONTANE	17.661	577039	3.923 ug/ml
14) N-DOTRIACONTANE	18.499	1103813	7.762 ug/ml
15) N-TETRATRIACONTANE	19.285	835191	6.238 ug/ml
16) N-HEXATRIACONTANE	20.070	4454252	34.137 ug/ml
17) N-OCTATRIACONTANE	20.749	1287624	11.152 ug/ml
18) N-TETRACONTANE	21.654	919461	7.391 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003892.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 16:32
Operator : AJ\SJ
Sample : K1693-09 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 22:38:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

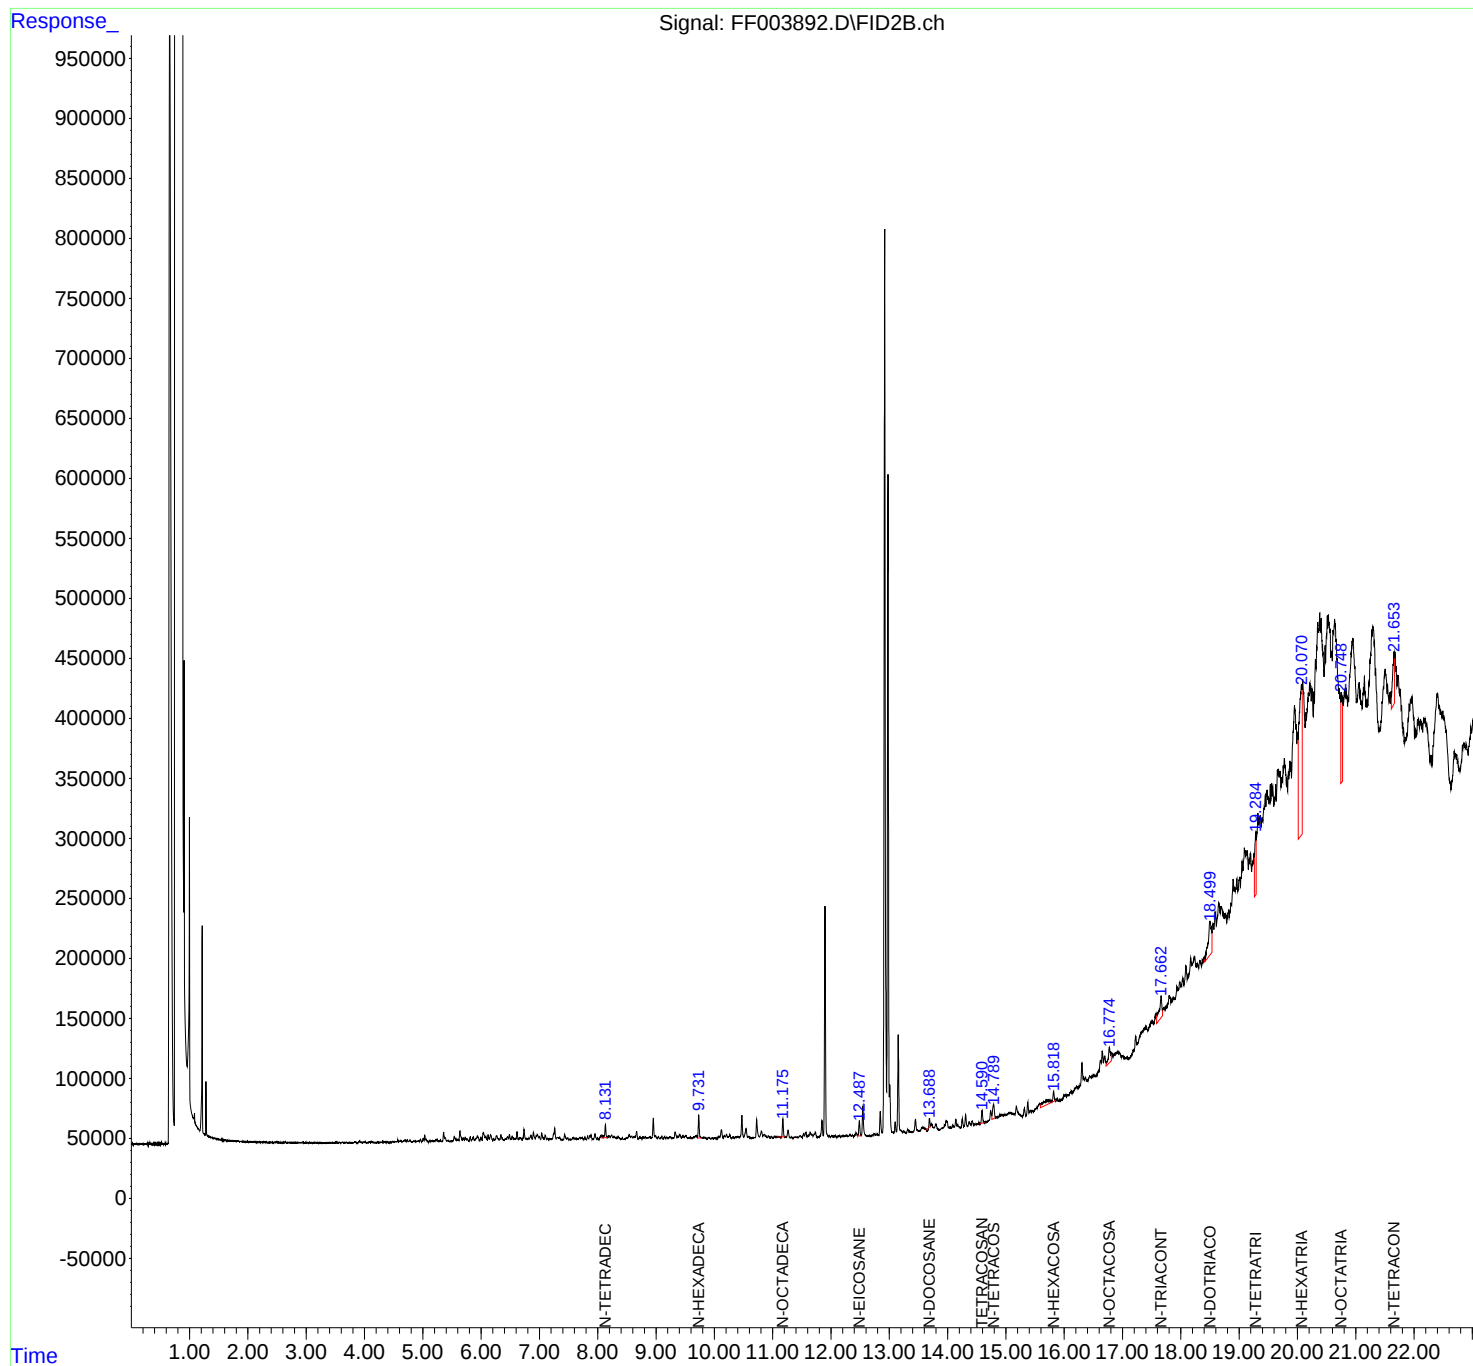


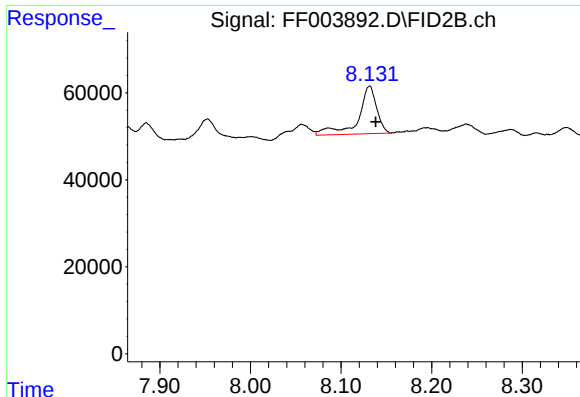

#4 N-TETRADECANE


R.T.: 8.132 min
Delta R.T.: -0.007 min
Response: 155109
Conc: 0.97 ug/ml

Instrument :
FID_F
ClientSampleId :

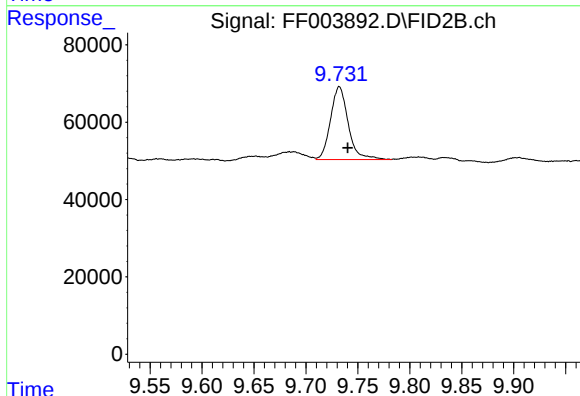


#5 N-HEXADECANE

R.T.: 9.732 min
Delta R.T.: -0.008 min
Response: 222956
Conc: 1.37 ug/ml

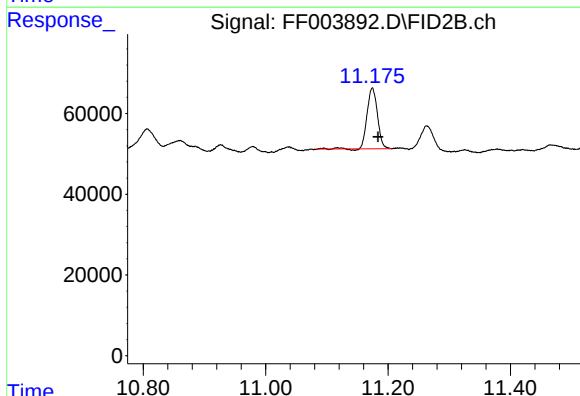


#6 N-OCTADECANE

R.T.: 11.174 min
Delta R.T.: -0.010 min
Response: 176324
Conc: 1.07 ug/ml

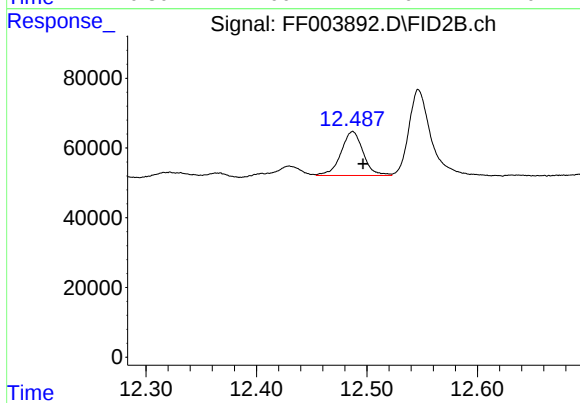

#7 N-EICOSANE


R.T.: 12.487 min
Delta R.T.: -0.009 min
Response: 175632
Conc: 1.07 ug/ml

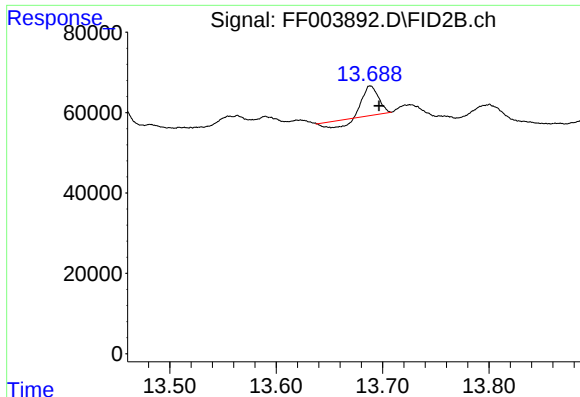

#8 N-DOCOSANE


R.T.: 13.689 min
Delta R.T.: -0.008 min
Response: 57142
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

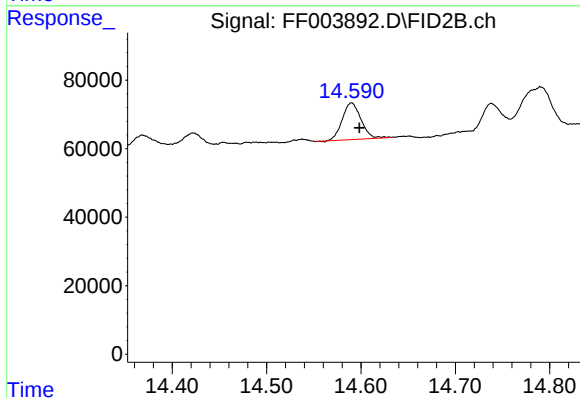


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.590 min
Delta R.T.: -0.008 min
Response: 147589
Conc: 1.06 ug/ml

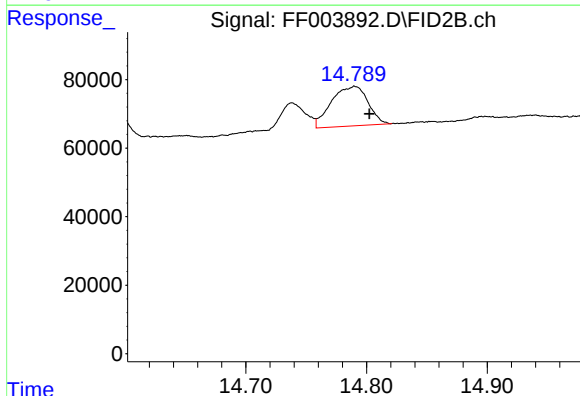


#10 N-TETRACOSANE

R.T.: 14.790 min
Delta R.T.: -0.012 min
Response: 243009
Conc: 1.54 ug/ml

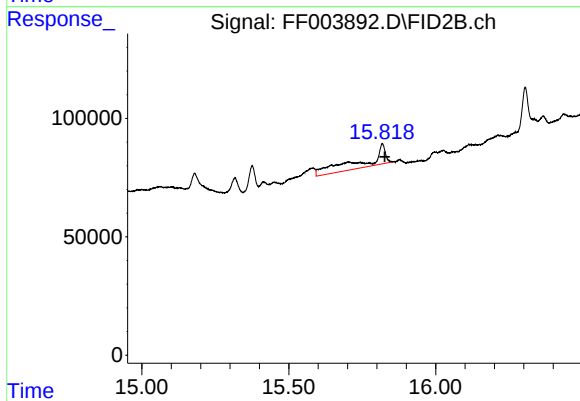

#11 N-HEXACOSANE


R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 426105
Conc: 2.76 ug/ml

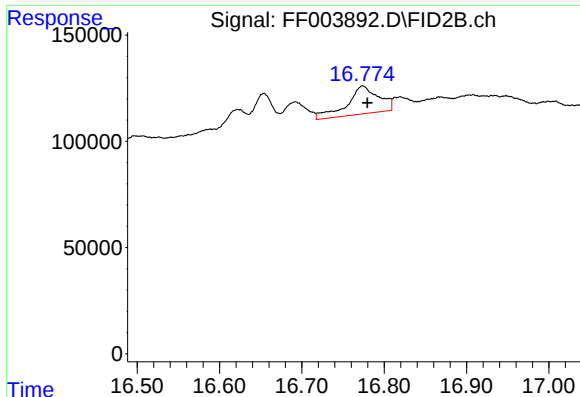

#12 N-OCTACOSANE


R.T.: 16.774 min
Delta R.T.: -0.006 min
Response: 349342
Conc: 2.31 ug/ml

Instrument :
FID_F
ClientSampleId :

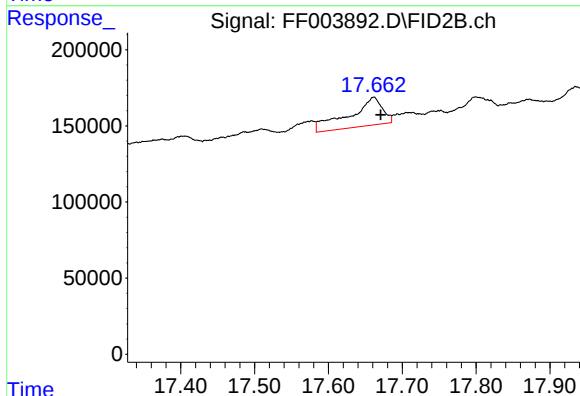


#13 N-TRIACONTANE

R.T.: 17.661 min
Delta R.T.: -0.009 min
Response: 577039
Conc: 3.92 ug/ml

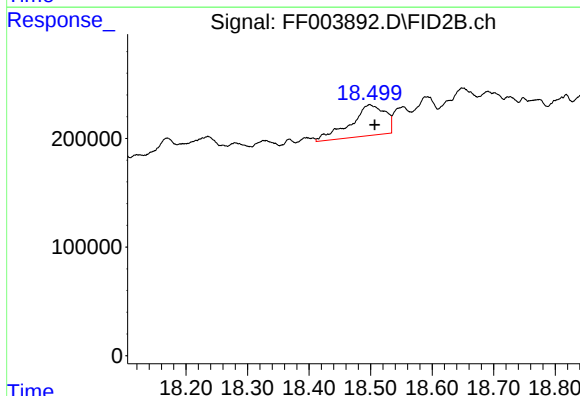


#14 N-DOTRIACONTANE

R.T.: 18.499 min
Delta R.T.: -0.008 min
Response: 1103813
Conc: 7.76 ug/ml

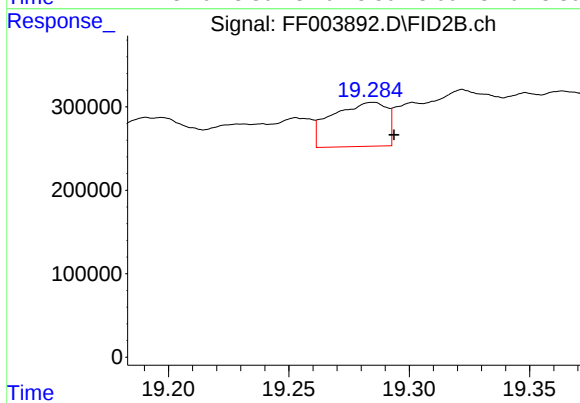

#15 N-TETRATRIACONTANE


R.T.: 19.285 min
Delta R.T.: -0.009 min
Response: 835191
Conc: 6.24 ug/ml

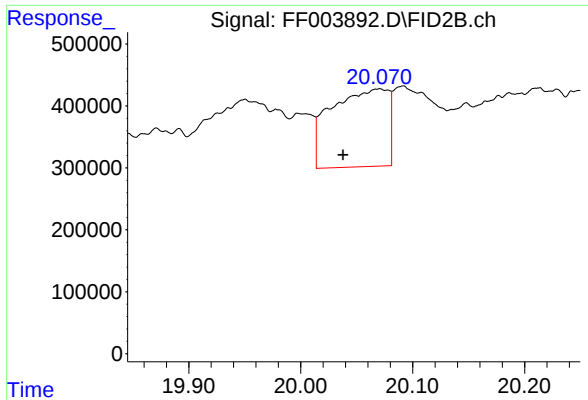

#16 N-HEXATRIACONTANE


R.T.: 20.070 min
Delta R.T.: 0.032 min
Response: 4454252
Conc: 34.14 ug/ml

Instrument :
FID_F
ClientSampleId :

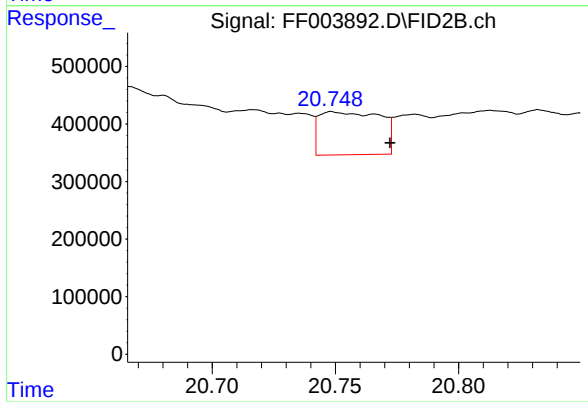

#17 N-OCTATRIACONTANE

R.T.: 20.749 min
Delta R.T.: -0.023 min
Response: 1287624
Conc: 11.15 ug/ml

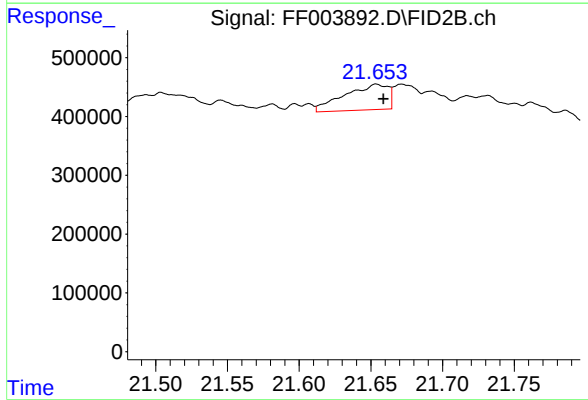

#18 N-TETRACONTANE

R.T.: 21.654 min
Delta R.T.: -0.005 min
Response: 919461
Conc: 7.39 ug/ml