

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003893.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 17:03
 Operator : AJ\SJ
 Sample : K1693-11 10X
 Misc :
 ALS Vial : 59 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 22:38:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	208299	1.496 ug/ml
Target Compounds			
7) N-EICOSANE	12.543	948819	5.800 ug/ml
10) N-TETRACOSANE	14.771	483916	3.058 ug/ml
11) N-HEXACOSANE	15.817	178347	1.156 ug/ml
12) N-OCTACOSANE	16.771	466765	3.089 ug/ml
13) N-TRIACONTANE	17.658	1255879	8.538 ug/ml
14) N-DOTRIACONTANE	18.498	502768	3.535 ug/ml
15) N-TETRATRIACONTANE	19.289	946568	7.069 ug/ml
16) N-HEXATRIACONTANE	20.027	1982496	15.194 ug/ml
17) N-OCTATRIACONTANE	20.780	1158086	10.030 ug/ml
18) N-TETRACONTANE	21.662	1584564	12.737 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003893.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 17:03
Operator : AJ\SJ
Sample : K1693-11 10X
Misc :
ALS Vial : 59 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 22:38:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

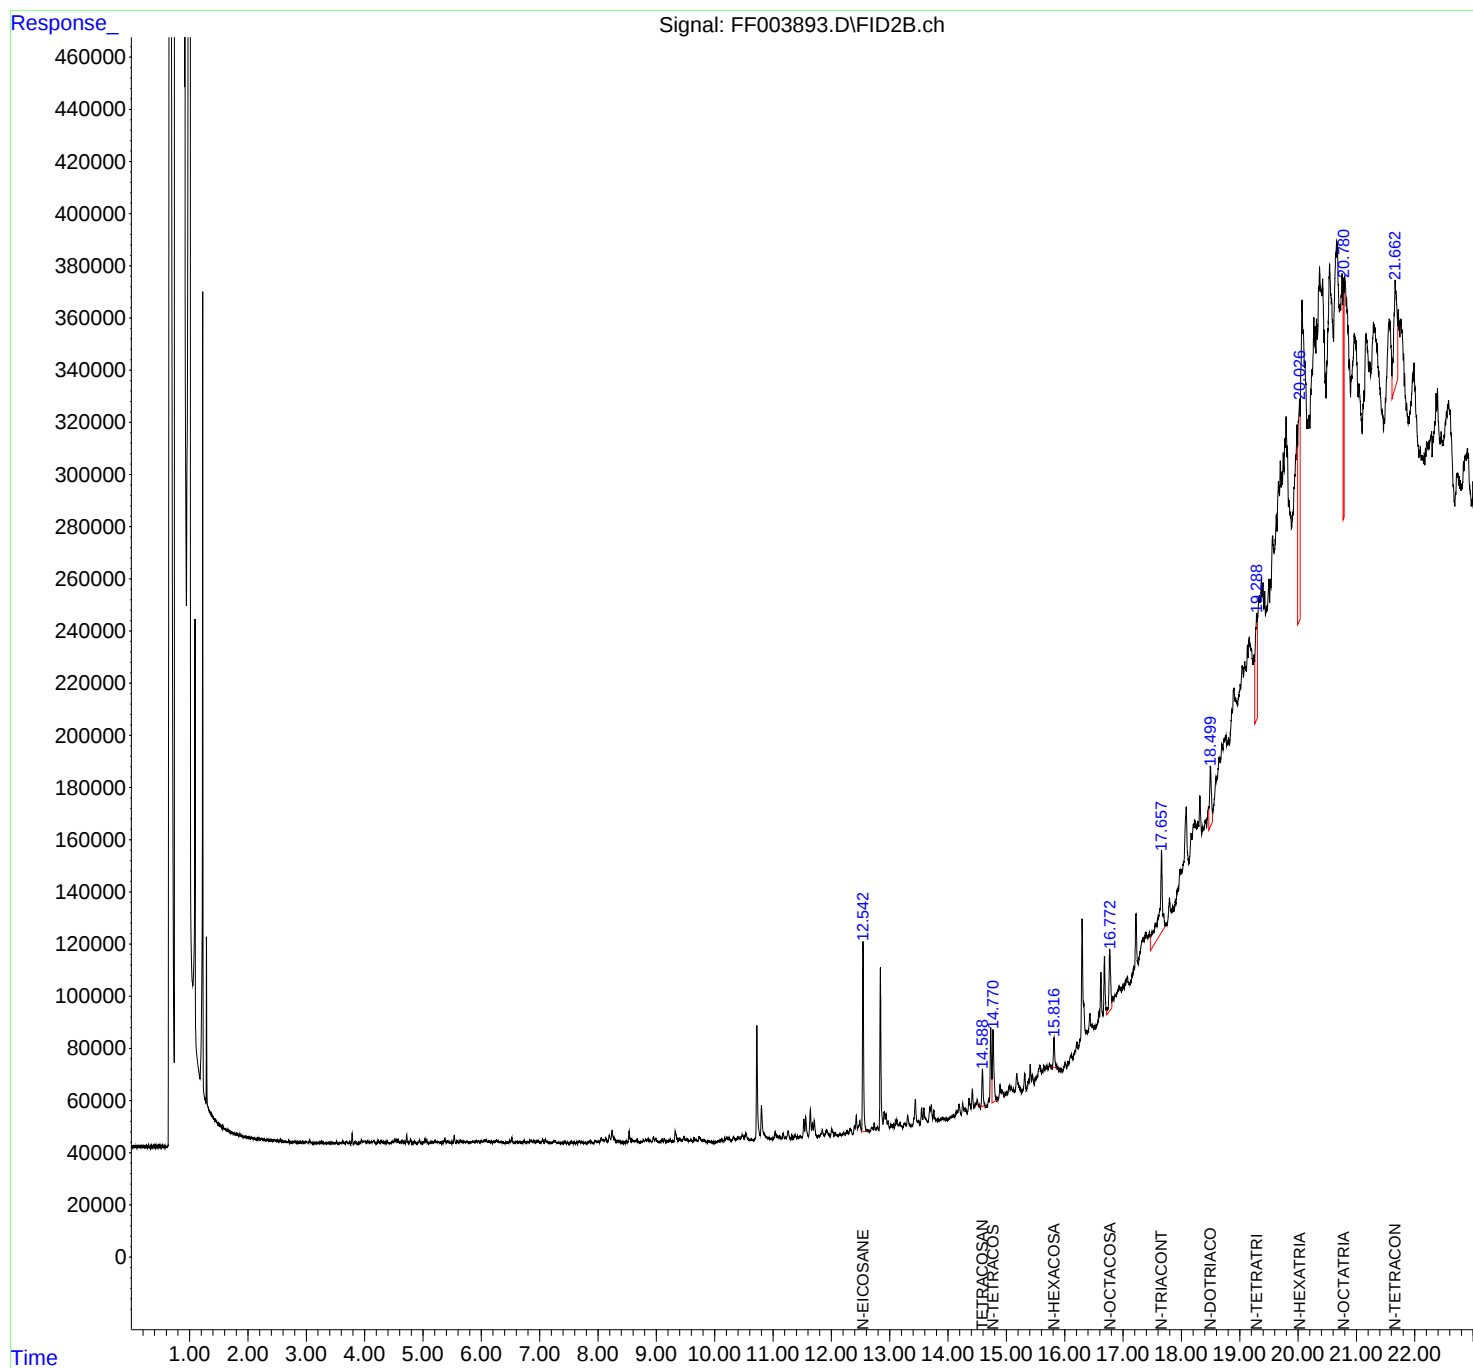


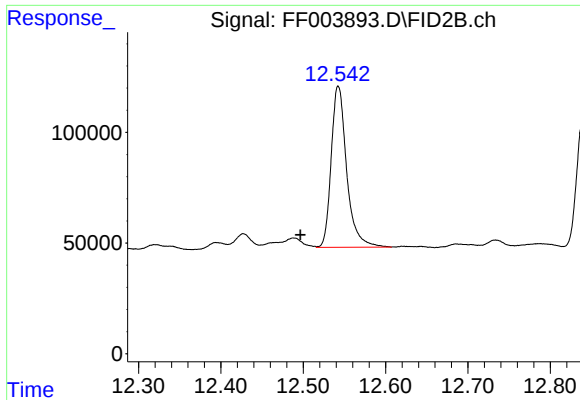

#7 N-EICOSANE


R.T.: 12.543 min
Delta R.T.: 0.046 min
Response: 948819
Conc: 5.80 ug/ml

Instrument :
FID_F
ClientSampleId :

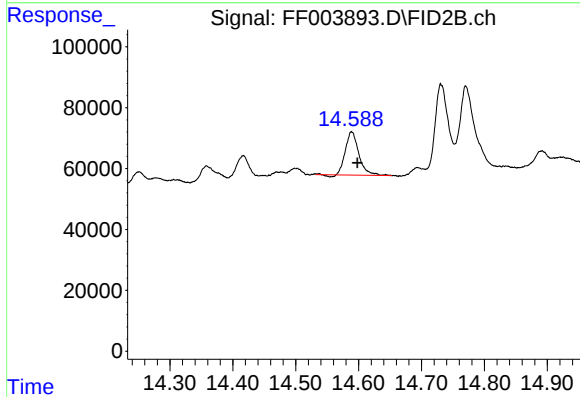


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.589 min
Delta R.T.: -0.009 min
Response: 208299
Conc: 1.50 ug/ml

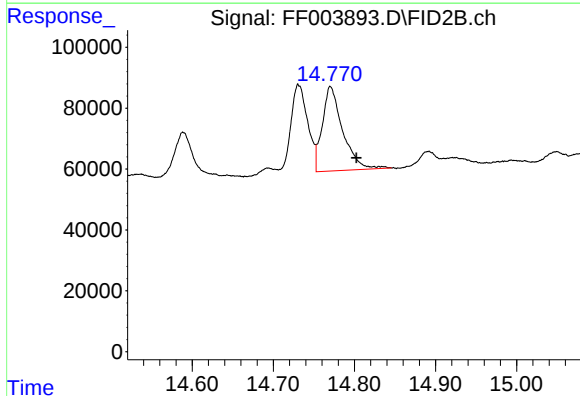


#10 N-TETRACOSANE

R.T.: 14.771 min
Delta R.T.: -0.032 min
Response: 483916
Conc: 3.06 ug/ml

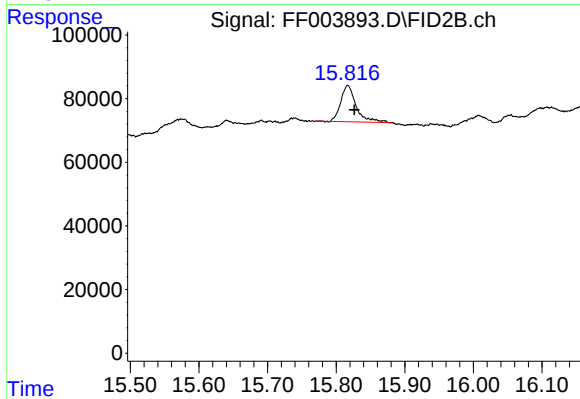

#11 N-HEXACOSANE


R.T.: 15.817 min
Delta R.T.: -0.010 min
Response: 178347
Conc: 1.16 ug/ml

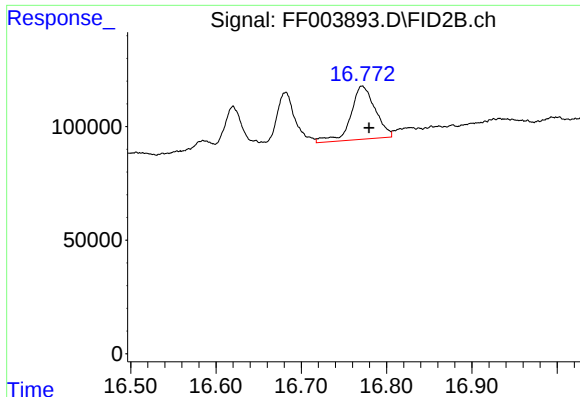

#12 N-OCTACOSANE


R.T.: 16.771 min
Delta R.T.: -0.008 min
Response: 466765
Conc: 3.09 ug/ml

Instrument :
FID_F
ClientSampleId :

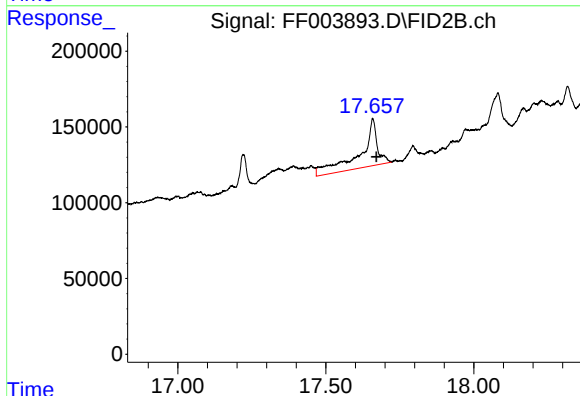


#13 N-TRIACONTANE

R.T.: 17.658 min
Delta R.T.: -0.012 min
Response: 1255879
Conc: 8.54 ug/ml

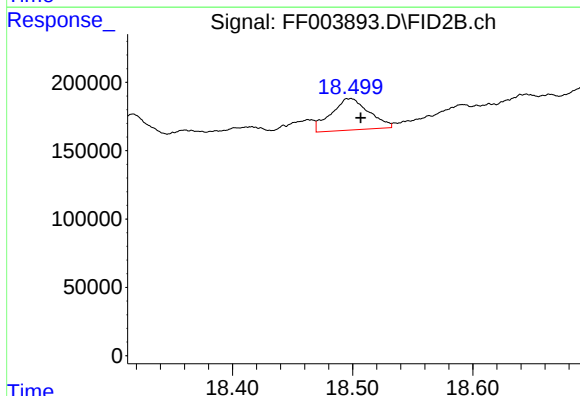


#14 N-DOTRIACONTANE

R.T.: 18.498 min
Delta R.T.: -0.009 min
Response: 502768
Conc: 3.54 ug/ml

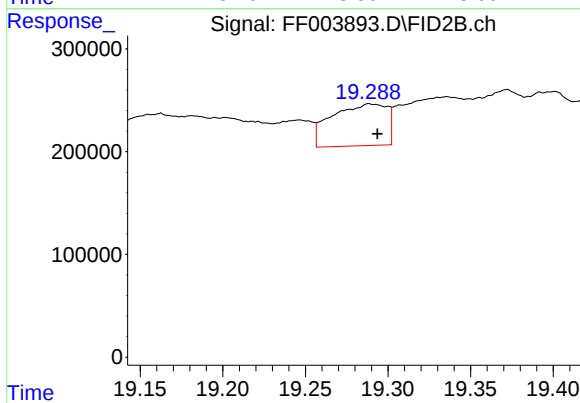

#15 N-TETRATRIACONTANE


R.T.: 19.289 min
Delta R.T.: -0.005 min
Response: 946568
Conc: 7.07 ug/ml

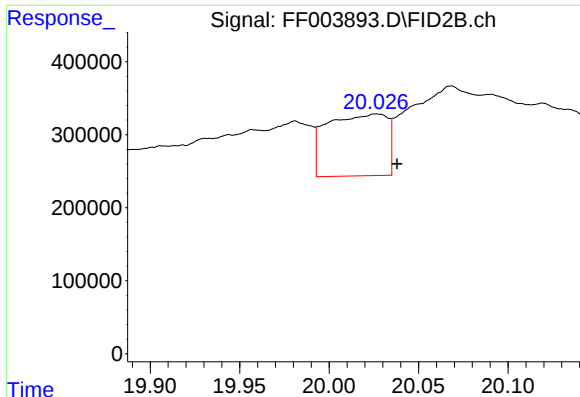

#16 N-HEXATRIACONTANE


R.T.: 20.027 min
Delta R.T.: -0.011 min
Response: 1982496
Conc: 15.19 ug/ml

Instrument :
FID_F
ClientSampleId :

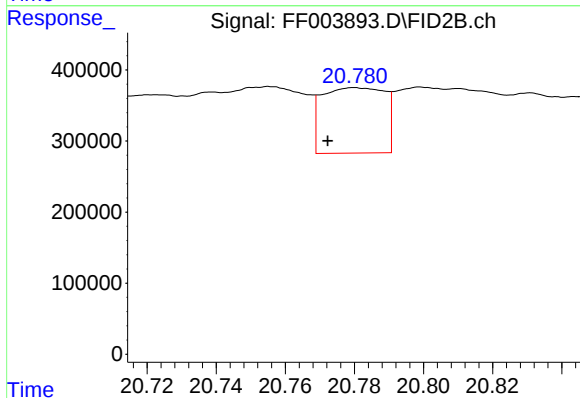

#17 N-OCTATRIACONTANE

R.T.: 20.780 min
Delta R.T.: 0.008 min
Response: 1158086
Conc: 10.03 ug/ml

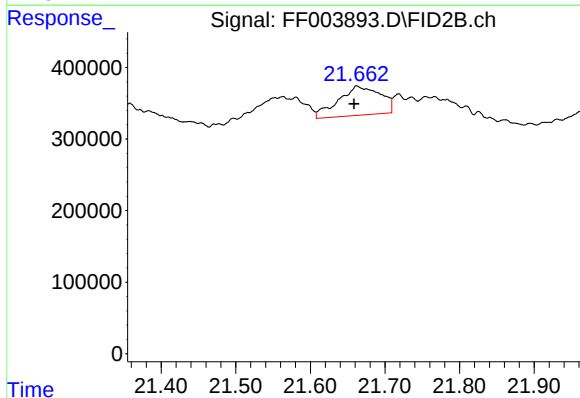

#18 N-TETRACONTANE

R.T.: 21.662 min
Delta R.T.: 0.004 min
Response: 1584564
Conc: 12.74 ug/ml