

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003894.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 17:33
 Operator : AJ\SJ
 Sample : K1956-06
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 22:38:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.588	2117449	15.209 ug/ml
Target Compounds			
4) N-TETRADECANE	8.189f	453495	2.828 ug/ml
10) N-TETRACOSANE	14.791	180406	1.140 ug/ml
11) N-HEXACOSANE	15.816	818455	5.303 ug/ml
12) N-OCTACOSANE	16.770	2027817	13.419 ug/ml
13) N-TRIACONTANE	17.660	2342857	15.927 ug/ml
14) N-DOTRIACONTANE	18.493	1437707	10.110 ug/ml
15) N-TETRATRIACONTANE	19.280	527791	3.942 ug/ml
16) N-HEXATRIACONTANE	20.037	727448	5.575 ug/ml
17) N-OCTATRIACONTANE	20.757	1673317	14.492 ug/ml
18) N-TETRACONTANE	21.674	565562	4.546 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003894.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 17:33
Operator : AJ\SJ
Sample : K1956-06
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampled :

Integration File: autoint1.e
Quant Time: Mar 19 22:38:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

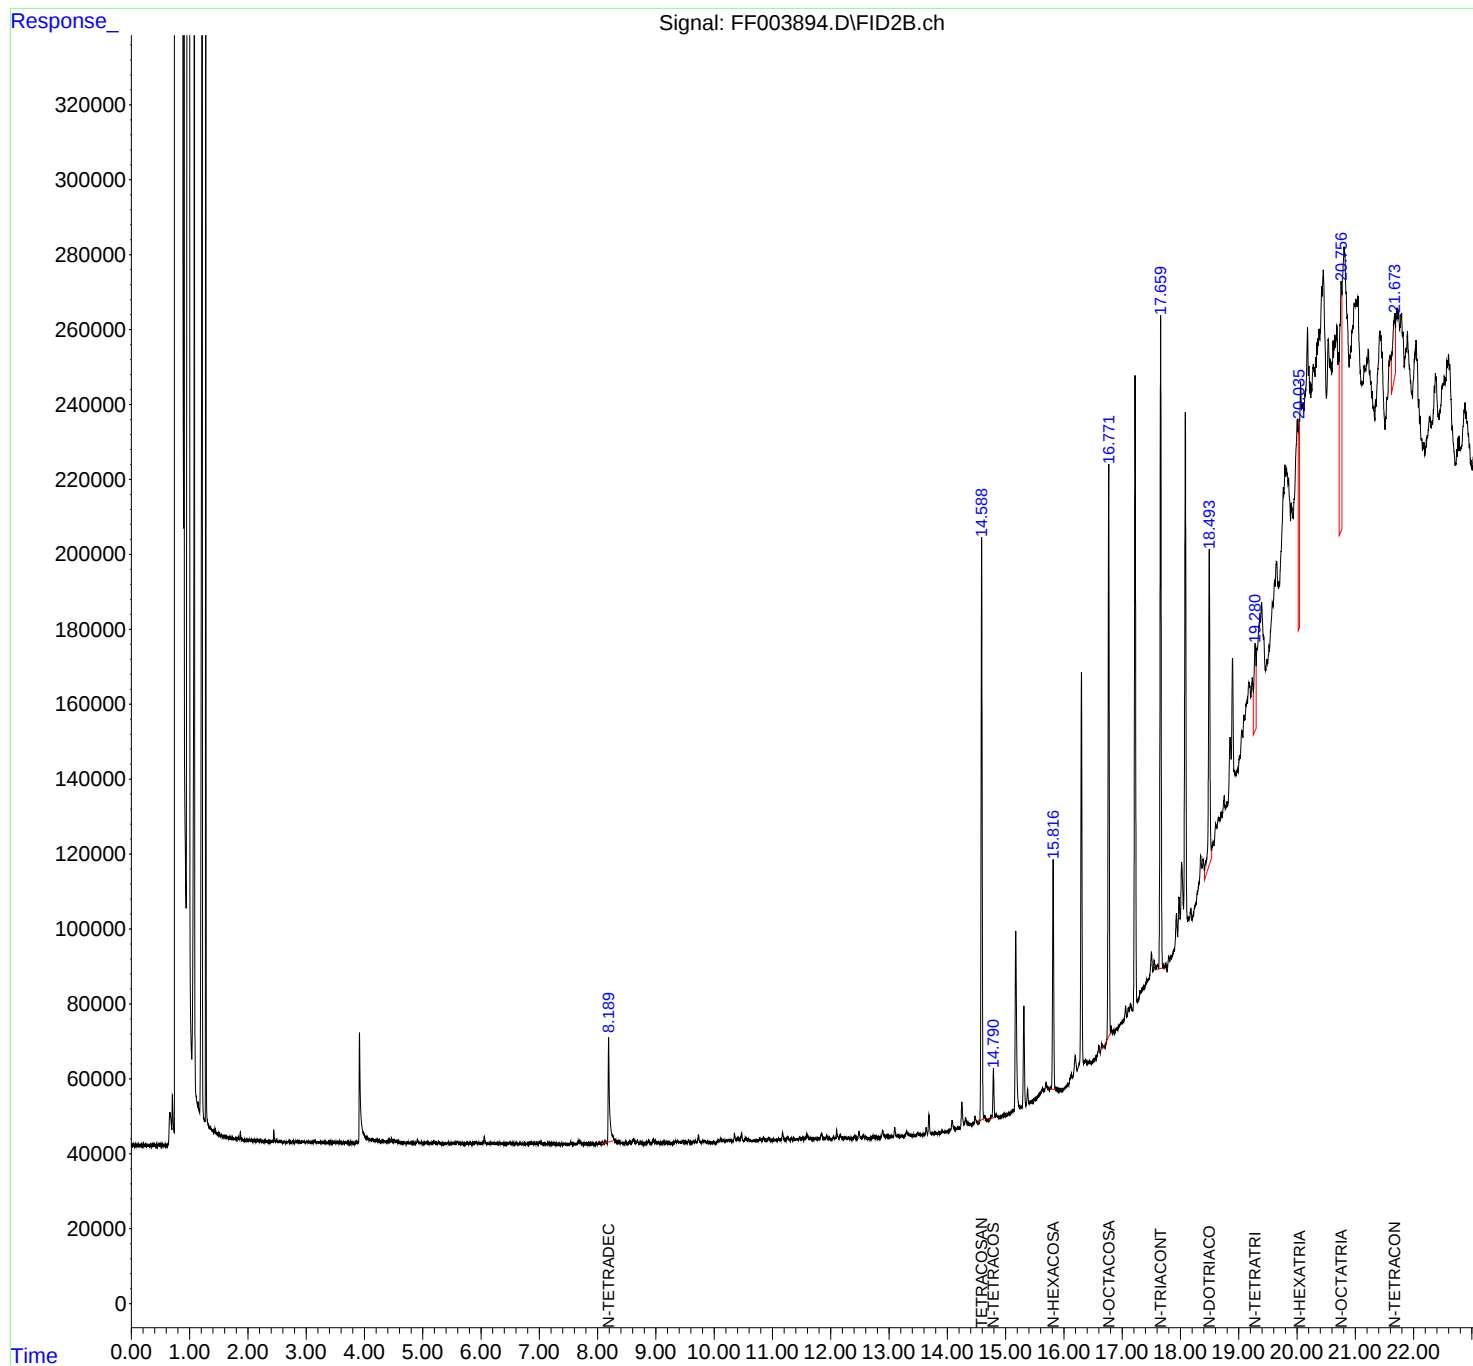


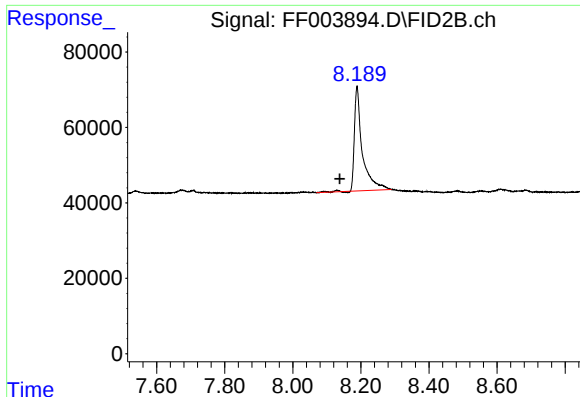

#4 N-TETRADECANE


R.T.: 8.189 min
Delta R.T.: 0.051 min
Response: 453495
Conc: 2.83 ug/ml

Instrument :
FID_F
ClientSampleId :

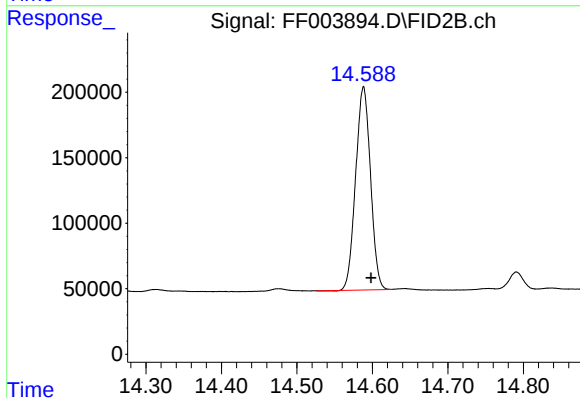


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.588 min
Delta R.T.: -0.010 min
Response: 2117449
Conc: 15.21 ug/ml

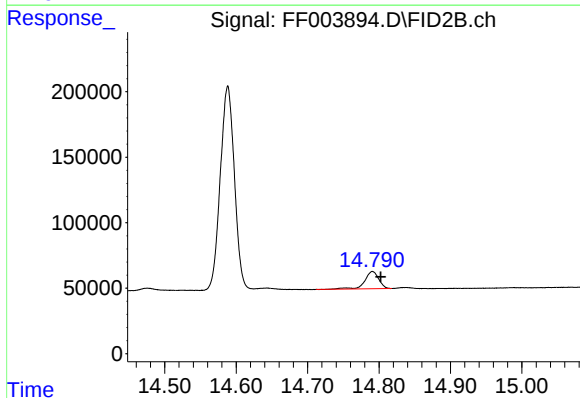


#10 N-TETRACOSANE

R.T.: 14.791 min
Delta R.T.: -0.012 min
Response: 180406
Conc: 1.14 ug/ml

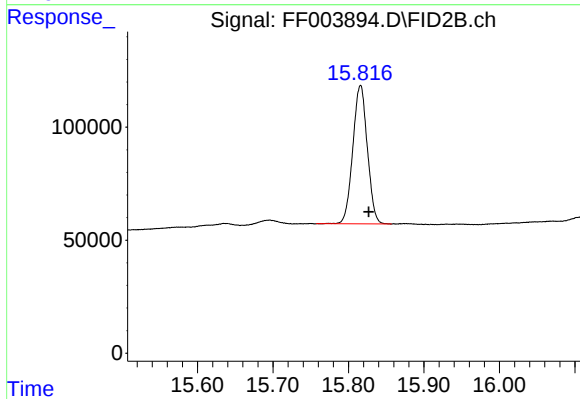

#11 N-HEXACOSANE


R.T.: 15.816 min
Delta R.T.: -0.011 min
Response: 818455
Conc: 5.30 ug/ml

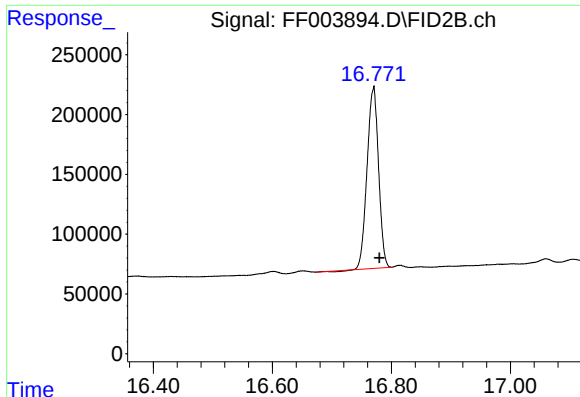

#12 N-OCTACOSANE


R.T.: 16.770 min
Delta R.T.: -0.010 min
Response: 2027817
Conc: 13.42 ug/ml

Instrument :
FID_F
ClientSampleId :

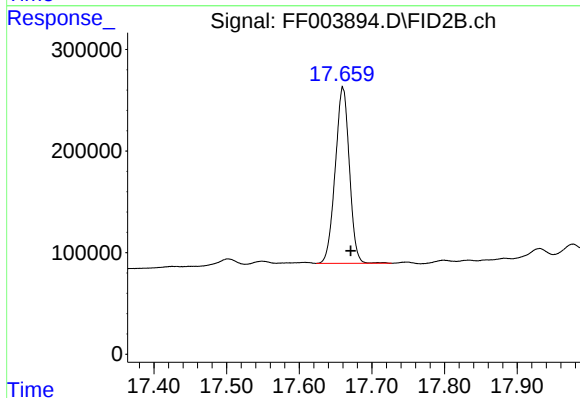


#13 N-TRIACONTANE

R.T.: 17.660 min
Delta R.T.: -0.011 min
Response: 2342857
Conc: 15.93 ug/ml

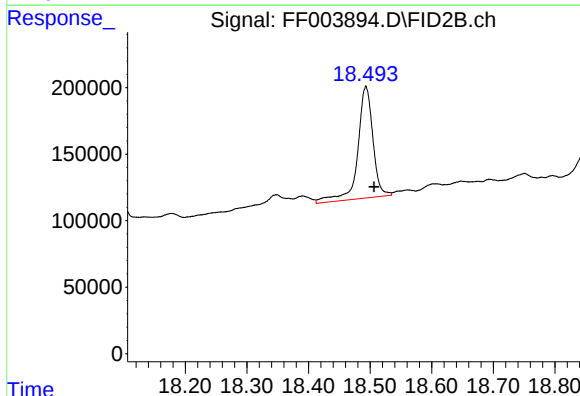


#14 N-DOTRIACONTANE

R.T.: 18.493 min
Delta R.T.: -0.014 min
Response: 1437707
Conc: 10.11 ug/ml

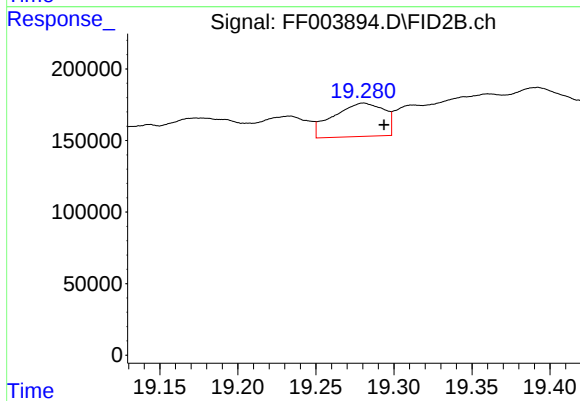

#15 N-TETRATRIACONTANE


R.T.: 19.280 min
Delta R.T.: -0.013 min
Response: 527791
Conc: 3.94 ug/ml

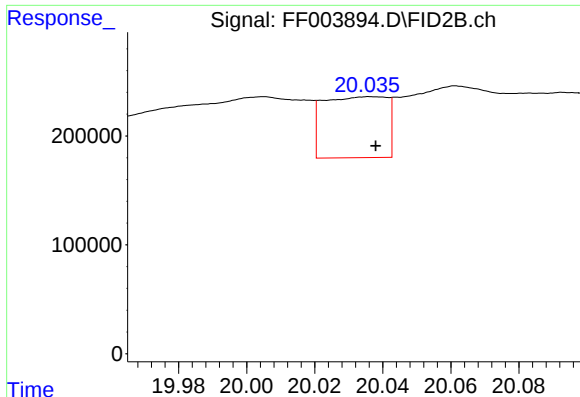

#16 N-HEXATRIACONTANE


R.T.: 20.037 min
Delta R.T.: -0.001 min
Response: 727448
Conc: 5.58 ug/ml

Instrument :
FID_F
ClientSampleId :

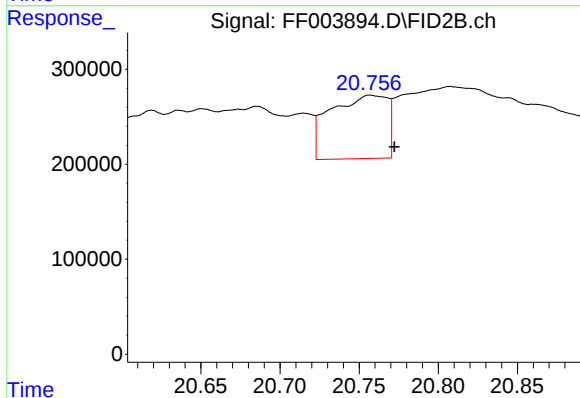

#17 N-OCTATRIACONTANE

R.T.: 20.757 min
Delta R.T.: -0.015 min
Response: 1673317
Conc: 14.49 ug/ml

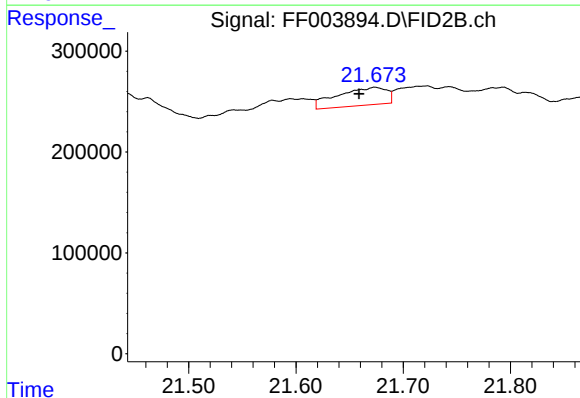

#18 N-TETRACONTANE

R.T.: 21.674 min
Delta R.T.: 0.015 min
Response: 565562
Conc: 4.55 ug/ml