

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003897.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 19:04
 Operator : AJ\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 22:39:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	2090793	15.017 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.656	138885	0.944 ug/ml
14) N-DOTRIACONTANE	18.492	219214	1.541 ug/ml
15) N-TETRATRIACONTANE	19.278	69289	0.517 ug/ml
16) N-HEXATRIACONTANE	20.055	96885	0.743 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003897.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 19:04
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 22:39:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

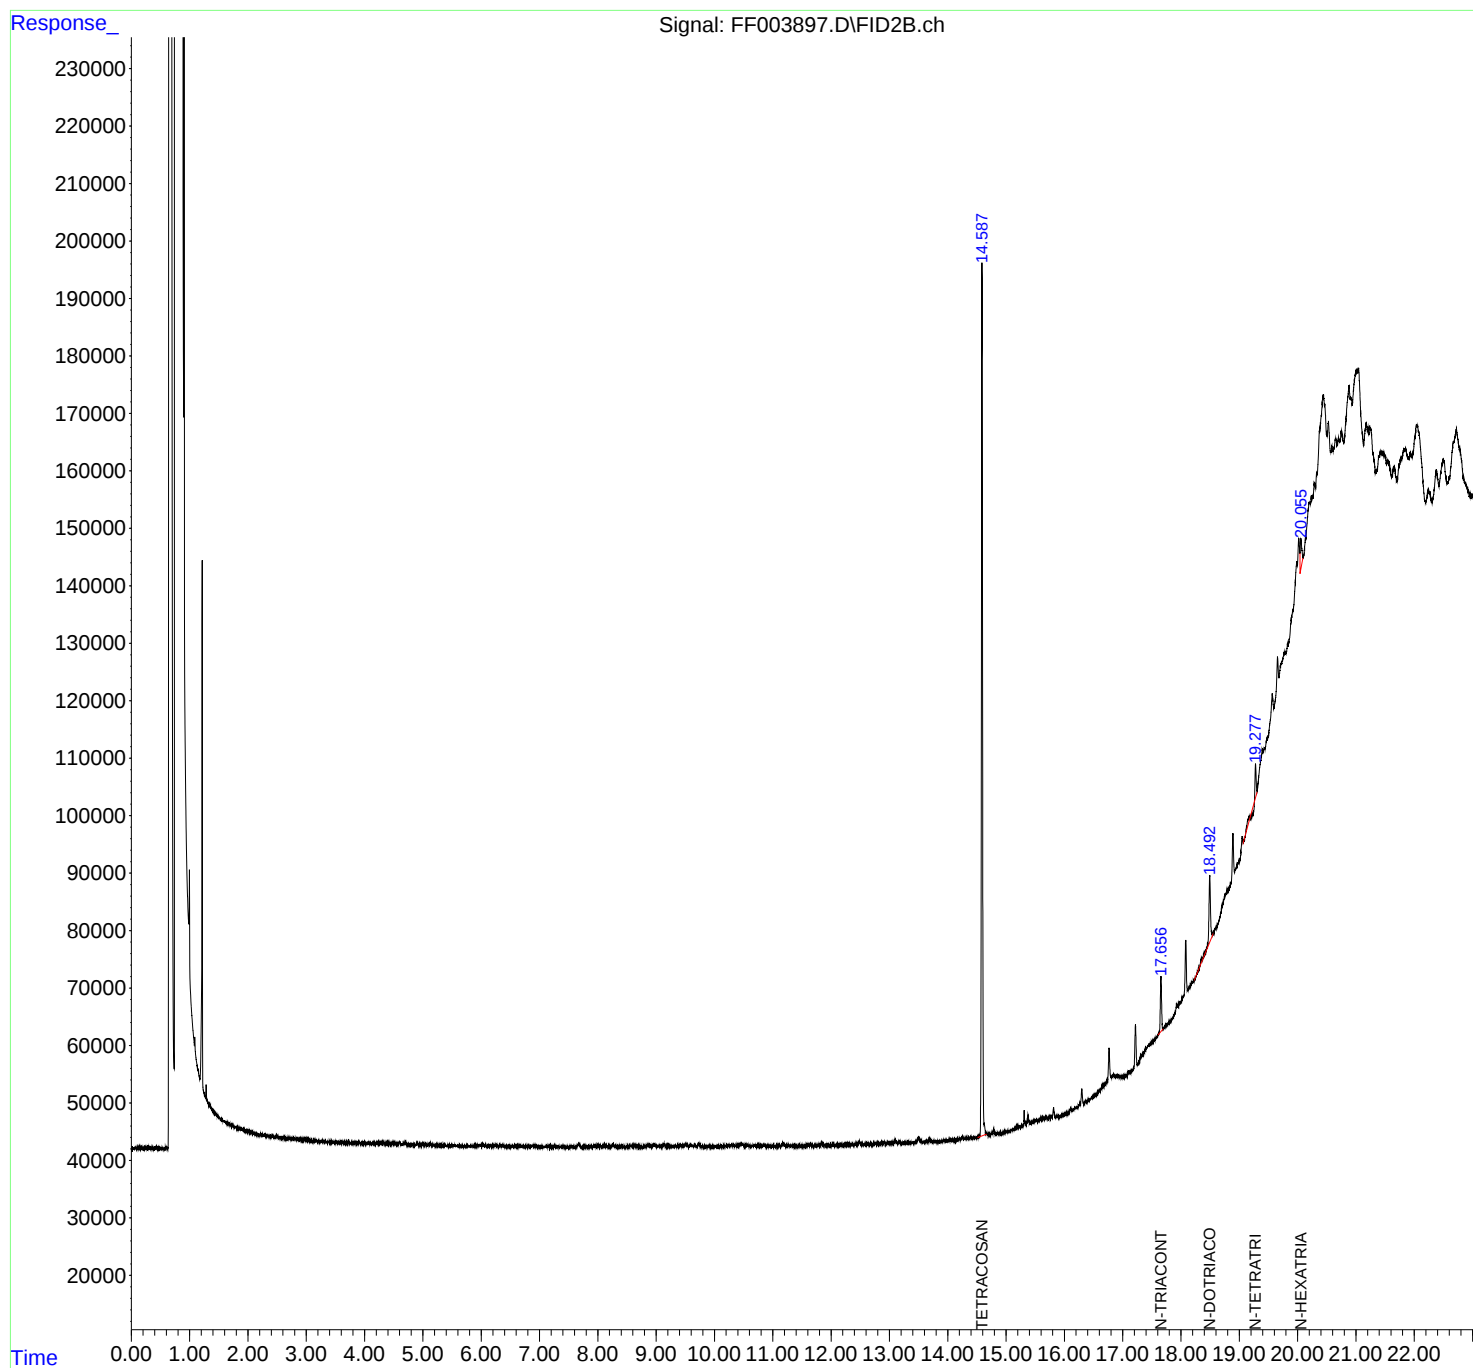


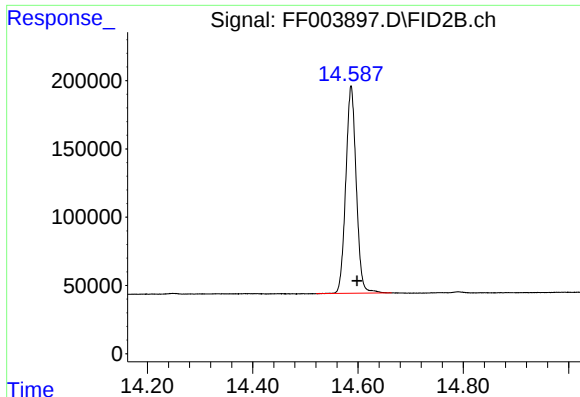

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.587 min
Delta R.T.: -0.011 min
Response: 2090793
Conc: 15.02 ug/ml

Instrument :
FID_F
ClientSampleId :

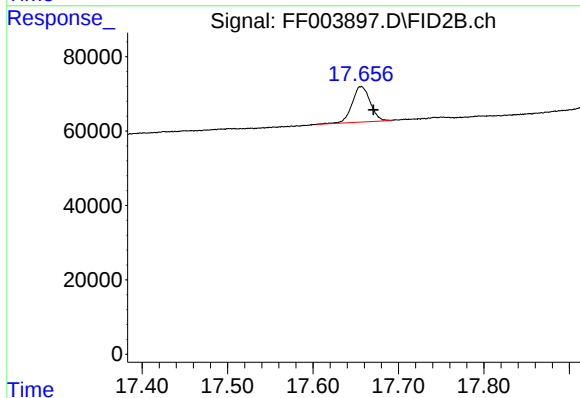


#13 N-TRIACONTANE

R.T.: 17.656 min
Delta R.T.: -0.015 min
Response: 138885
Conc: 0.94 ug/ml

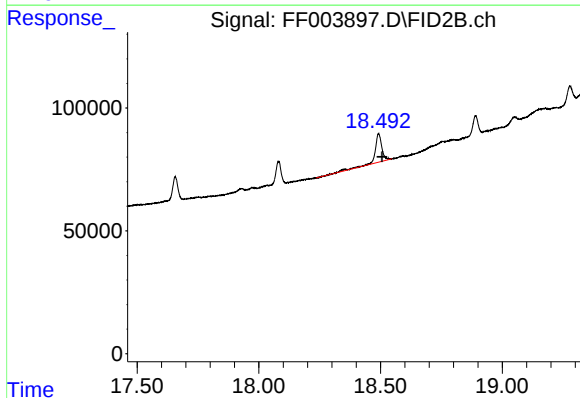


#14 N-DOTRIACONTANE

R.T.: 18.492 min
Delta R.T.: -0.015 min
Response: 219214
Conc: 1.54 ug/ml

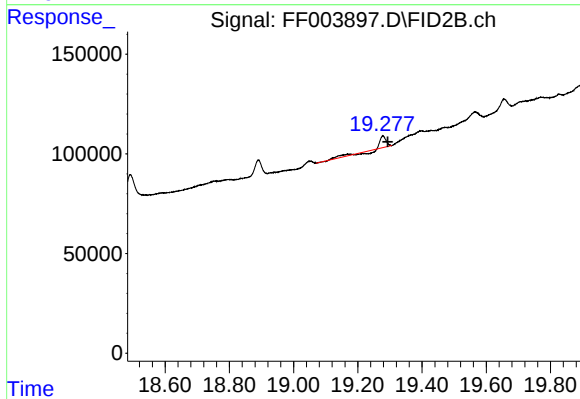

#15 N-TETRATRIACONTANE

R.T.: 19.278 min
Delta R.T.: -0.016 min
Response: 69289
Conc: 0.52 ug/ml

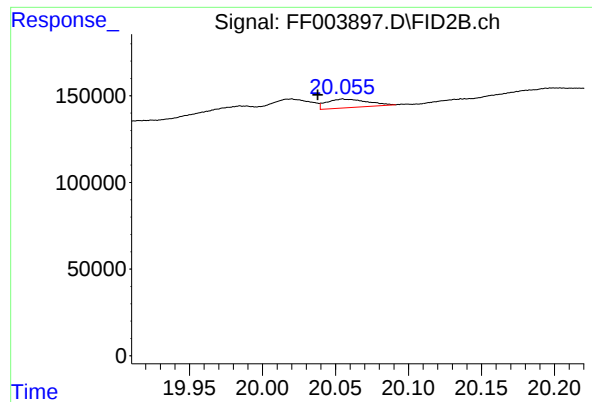

#16 N-HEXATRIACONTANE

R.T.: 20.055 min
Delta R.T.: 0.017 min
Response: 96885
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :