

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003895.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 18:03
 Operator : AJ\SJ
 Sample : K1956-06MS
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 TP-8-AMS

Integration File: autoint1.e
 Quant Time: Mar 19 22:39:12 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.588	2100451	15.086 ug/ml
Target Compounds				
2)	N-DECANE	4.316	2751296	17.886 ug/ml
3)	N-DODECANE	6.338	2768820	17.742 ug/ml
4)	N-TETRADECANE	8.130	2746596	17.130 ug/ml
5)	N-HEXADECANE	9.731	2710594	16.643 ug/ml
6)	N-OCTADECANE	11.174	2664490	16.172 ug/ml
7)	N-EICOSANE	12.485	2583126	15.790 ug/ml
8)	N-DOCOSANE	13.686	2545394	15.772 ug/ml
10)	N-TETRACOSANE	14.792	2507716	15.849 ug/ml
11)	N-HEXACOSANE	15.817	2537588	16.441 ug/ml
12)	N-OCTACOSANE	16.770	2695503	17.838 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003895.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 18:03
Operator : AJ\SJ
Sample : K1956-06MS
Misc :
ALS Vial : 61 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
TP-8-AMS

Integration File: autoint1.e
Quant Time: Mar 19 22:39:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

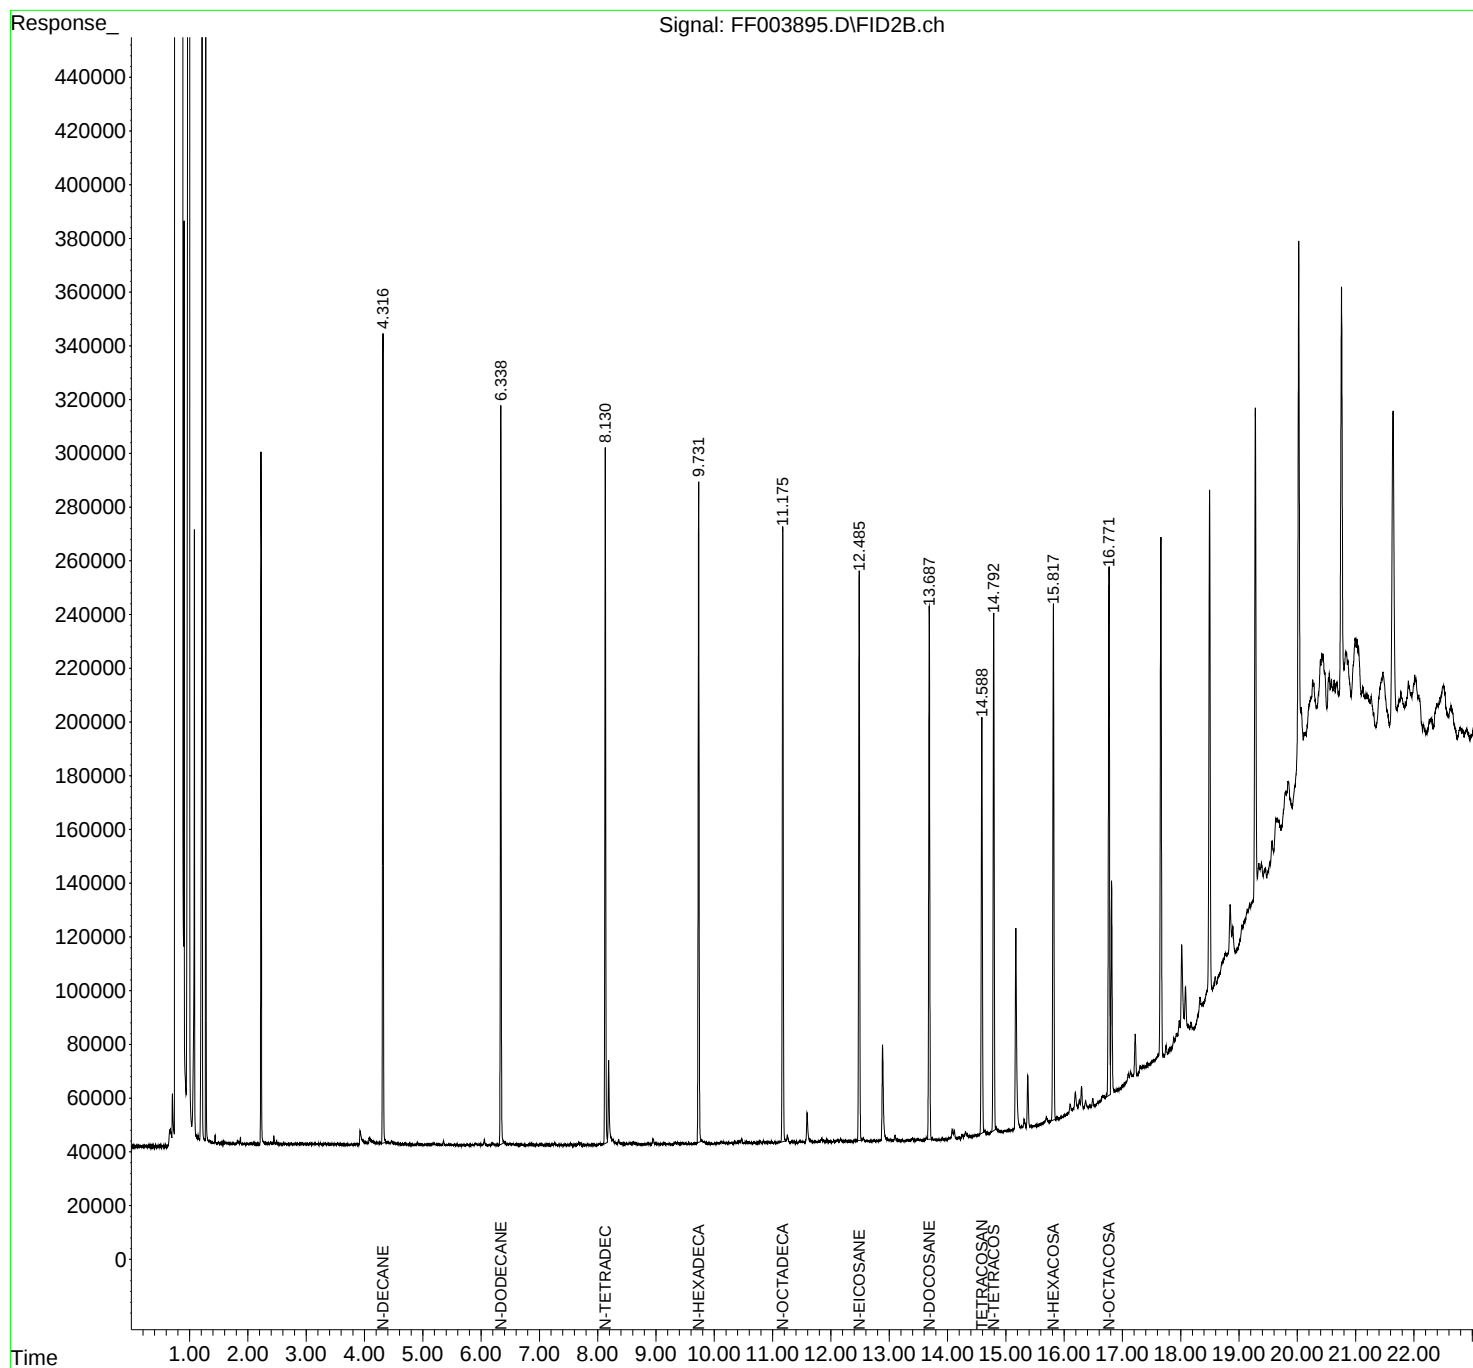


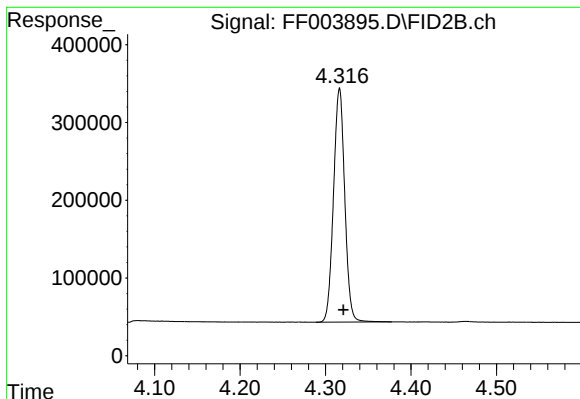

#2 N-DECANE


R.T.: 4.316 min
Delta R.T.: -0.004 min
Response: 2751296
Conc: 17.89 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-8-AMS

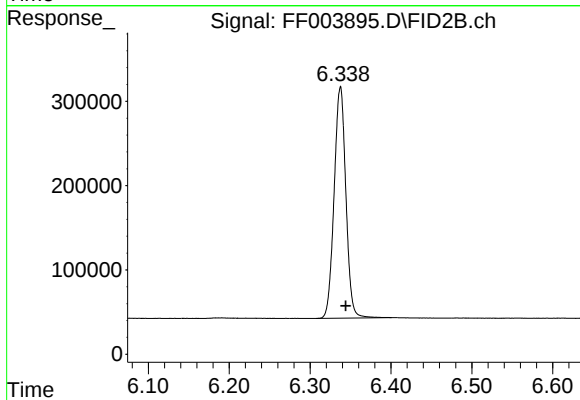


#3 N-DODECANE

R.T.: 6.338 min
Delta R.T.: -0.007 min
Response: 2768820
Conc: 17.74 ug/ml

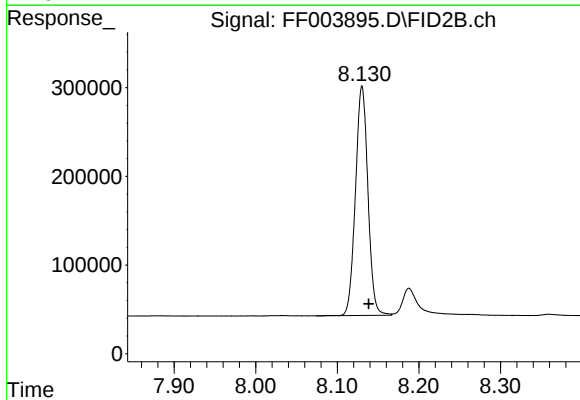


#4 N-TETRADECANE

R.T.: 8.130 min
Delta R.T.: -0.008 min
Response: 2746596
Conc: 17.13 ug/ml

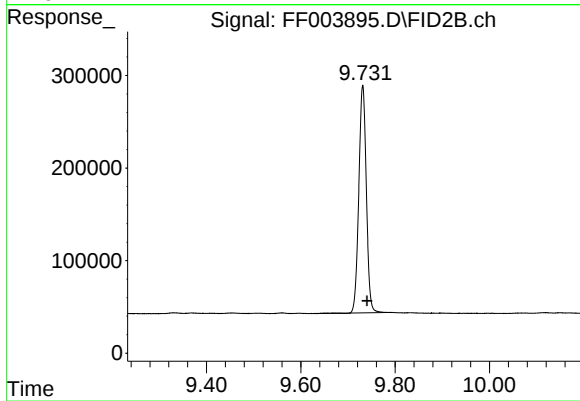

#5 N-HEXADECANE


R.T.: 9.731 min
Delta R.T.: -0.009 min
Response: 2710594
Conc: 16.64 ug/ml

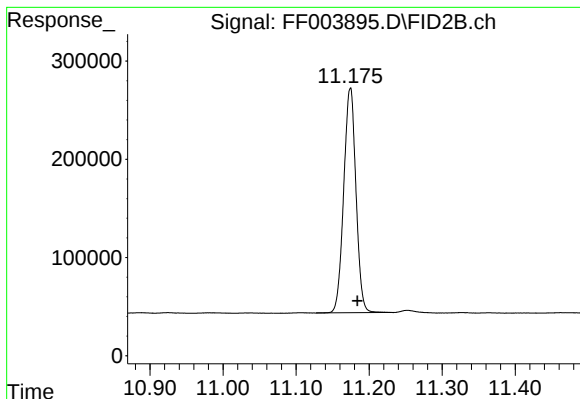

#6 N-OCTADECANE


R.T.: 11.174 min
Delta R.T.: -0.009 min
Response: 2664490
Conc: 16.17 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-8-AMS

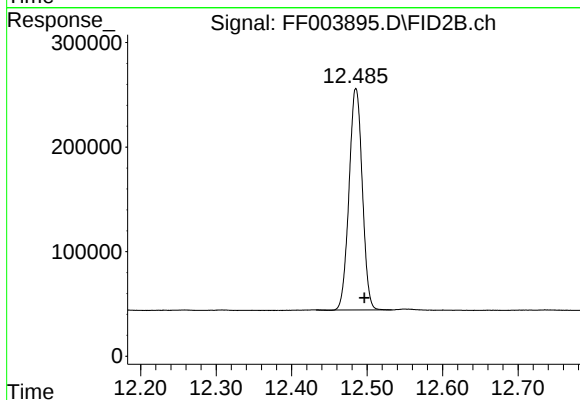


#7 N-EICOSANE

R.T.: 12.485 min
Delta R.T.: -0.011 min
Response: 2583126
Conc: 15.79 ug/ml

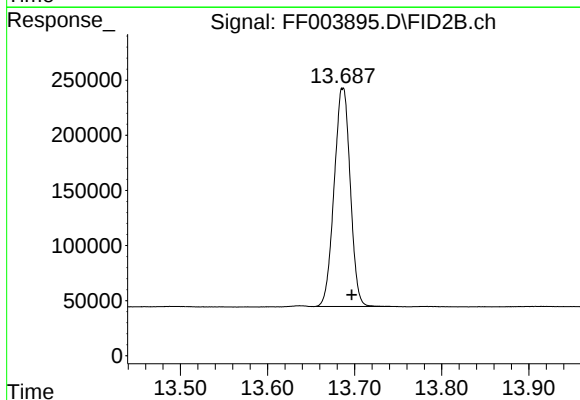


#8 N-DOCOSANE

R.T.: 13.686 min
Delta R.T.: -0.010 min
Response: 2545394
Conc: 15.77 ug/ml

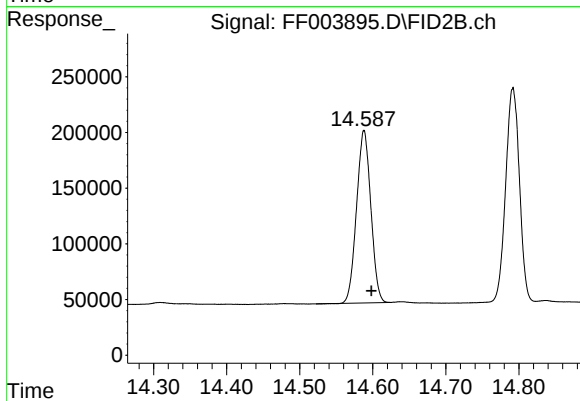

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.588 min
Delta R.T.: -0.010 min
Response: 2100451
Conc: 15.09 ug/ml

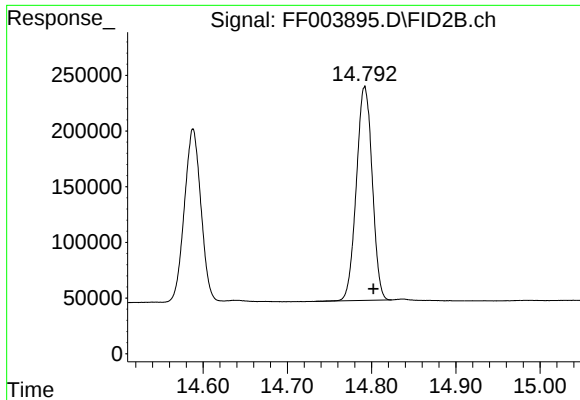

#10 N-TETRACOSANE


R.T.: 14.792 min
Delta R.T.: -0.011 min
Response: 2507716
Conc: 15.85 ug/ml

Instrument :
FID_F
ClientSampleId :
TP-8-AMS

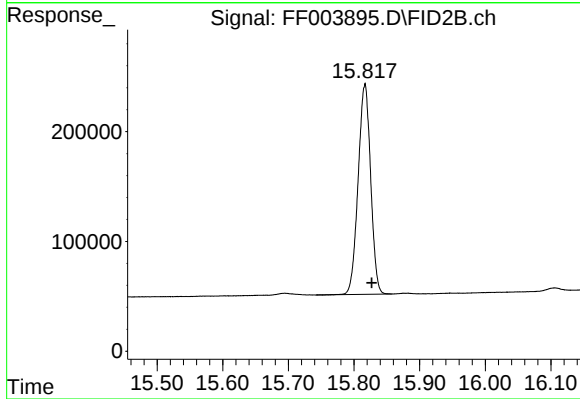

#11 N-HEXACOSANE

R.T.: 15.817 min
Delta R.T.: -0.010 min
Response: 2537588
Conc: 16.44 ug/ml

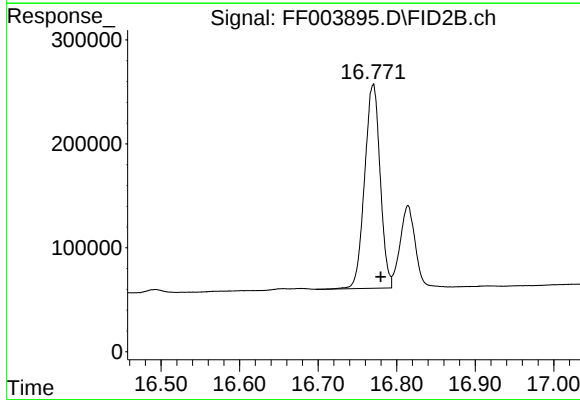

#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.010 min
Response: 2695503
Conc: 17.84 ug/ml