

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
 Data File : FF003898.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2019 19:35
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 19 22:39:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	5960960	42.814 ug/ml
Target Compounds			
2) N-DECANE	4.316	8066906	52.444 ug/ml
3) N-DODECANE	6.339	7969146	51.063 ug/ml
4) N-TETRADECANE	8.132	7778533	48.514 ug/ml
5) N-HEXADECANE	9.733	7549855	46.355 ug/ml
6) N-OCTADECANE	11.176	7329180	44.485 ug/ml
7) N-EICOSANE	12.487	7065405	43.189 ug/ml
8) N-DOCOSANE	13.688	6871941	42.580 ug/ml
10) N-TETRACOSANE	14.794	6765355	42.759 ug/ml
11) N-HEXACOSANE	15.818	6751146	43.741 ug/ml
12) N-OCTACOSANE	16.770	6854095	45.357 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031919\
Data File : FF003898.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2019 19:35
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 19 22:39:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

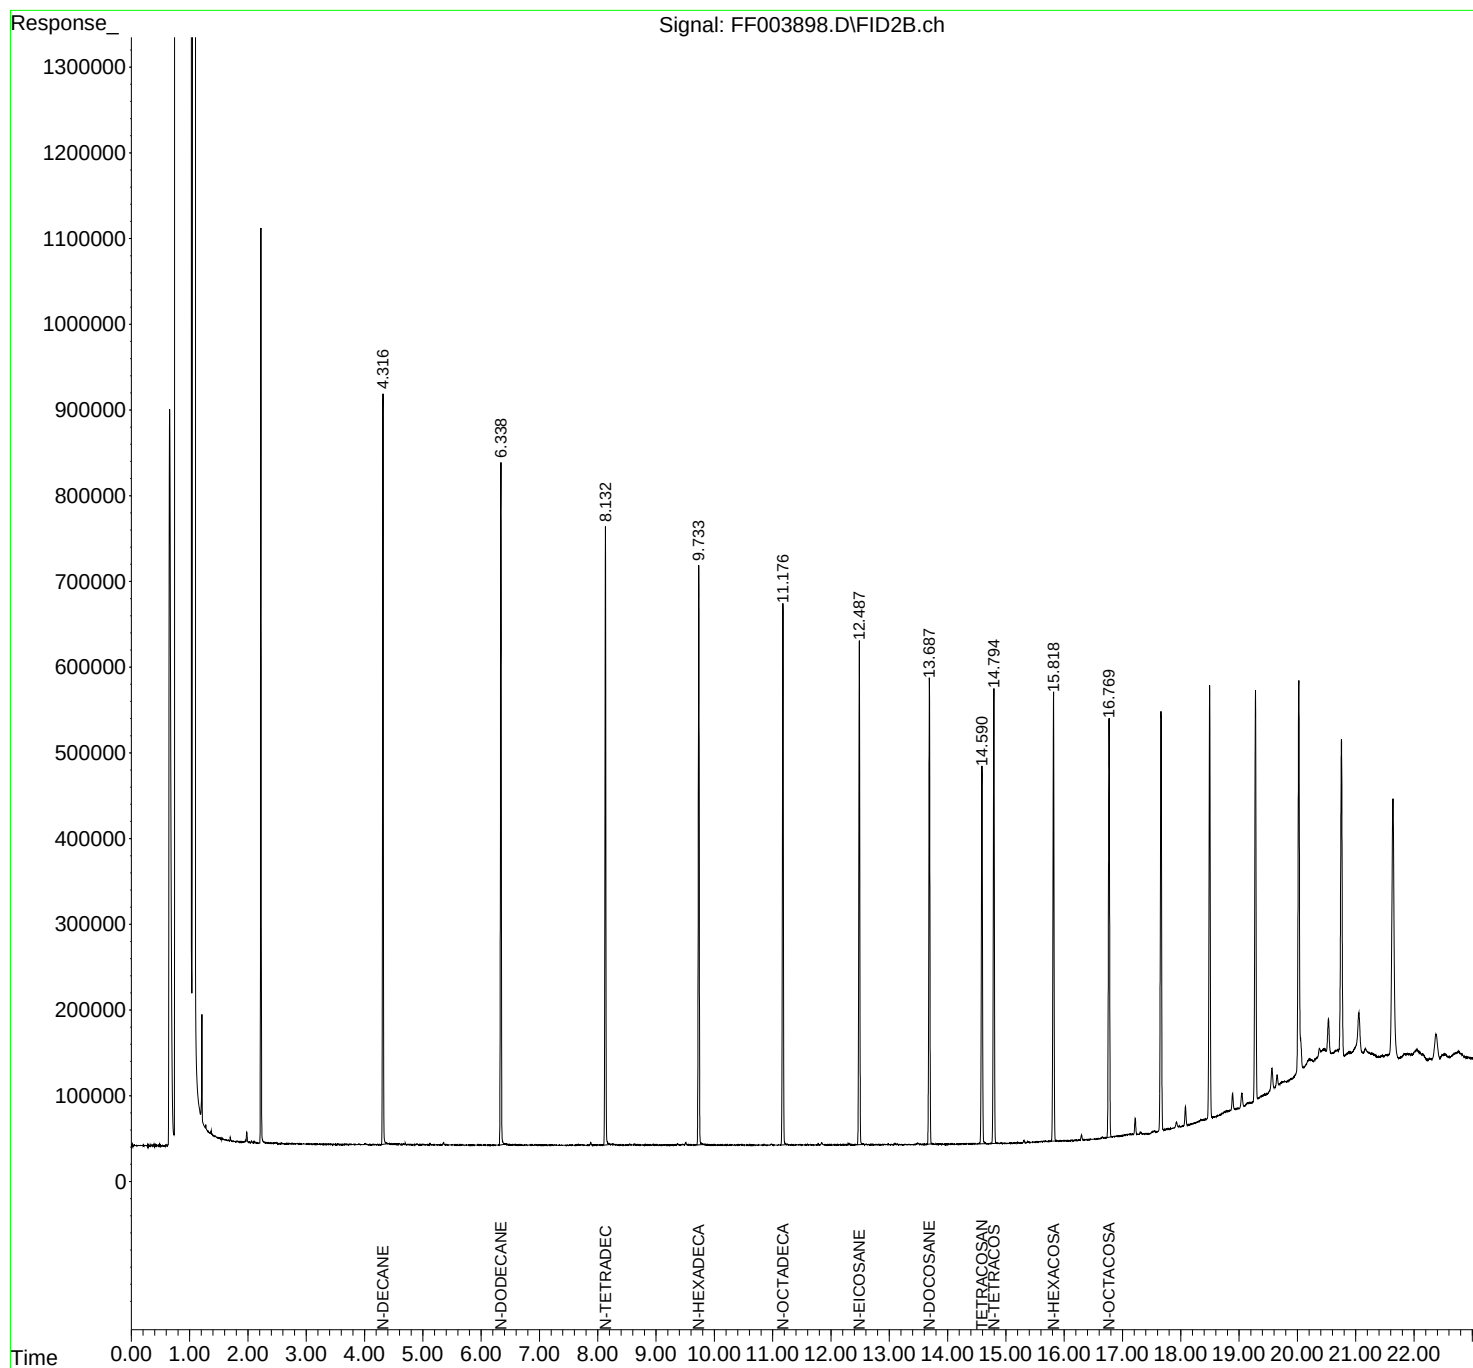


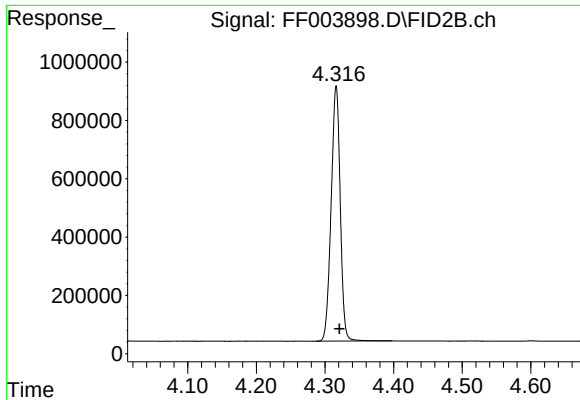

#2 N-DECANE


R.T.: 4.316 min
Delta R.T.: -0.004 min
Response: 8066906
Conc: 52.44 ug/ml

Instrument :
FID_F
ClientSampleId :

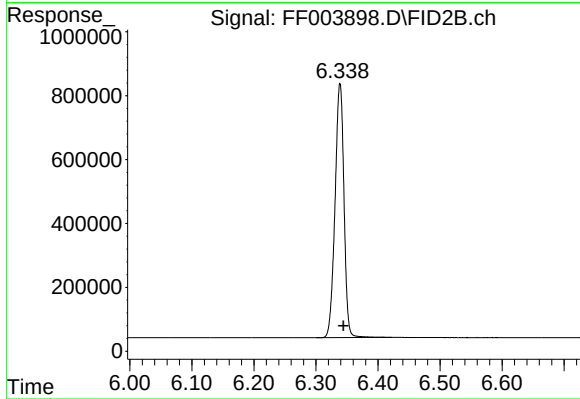


#3 N-DODECANE

R.T.: 6.339 min
Delta R.T.: -0.005 min
Response: 7969146
Conc: 51.06 ug/ml

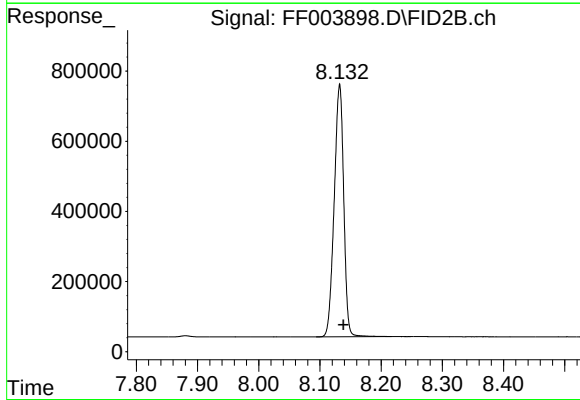


#4 N-TETRADECANE

R.T.: 8.132 min
Delta R.T.: -0.006 min
Response: 7778533
Conc: 48.51 ug/ml

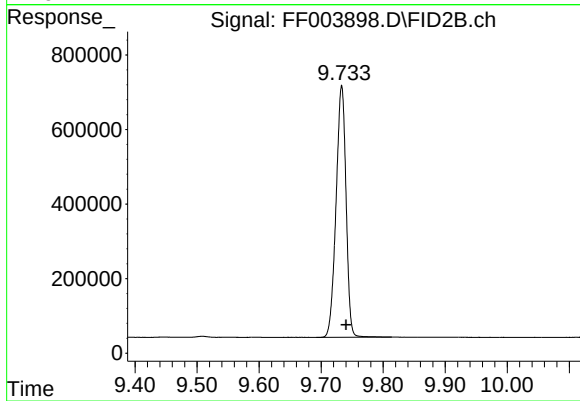

#5 N-HEXADECANE


R.T.: 9.733 min
Delta R.T.: -0.007 min
Response: 7549855
Conc: 46.35 ug/ml

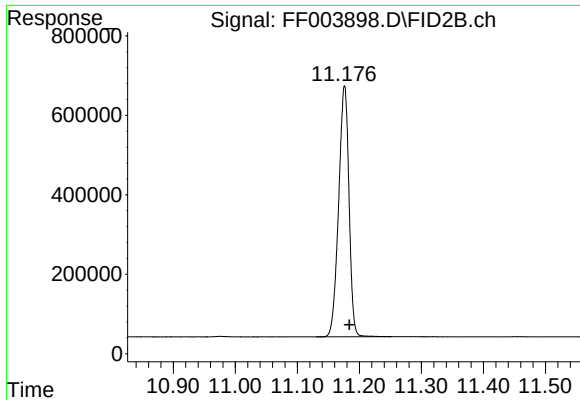

#6 N-OCTADECANE


R.T.: 11.176 min
Delta R.T.: -0.008 min
Response: 7329180
Conc: 44.49 ug/ml

Instrument :
FID_F
ClientSampleId :

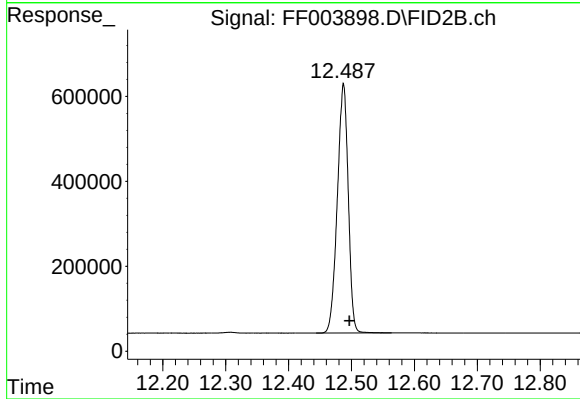


#7 N-EICOSANE

R.T.: 12.487 min
Delta R.T.: -0.009 min
Response: 7065405
Conc: 43.19 ug/ml

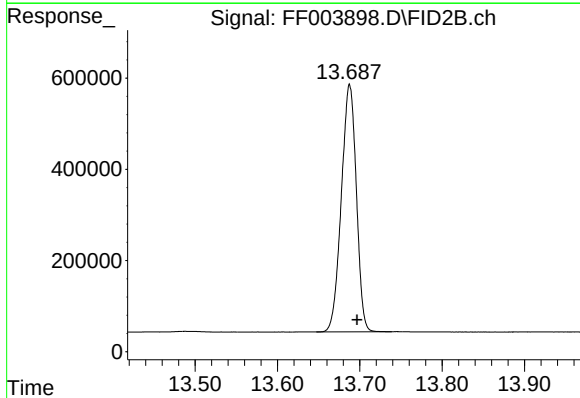


#8 N-DOCOSANE

R.T.: 13.688 min
Delta R.T.: -0.009 min
Response: 6871941
Conc: 42.58 ug/ml

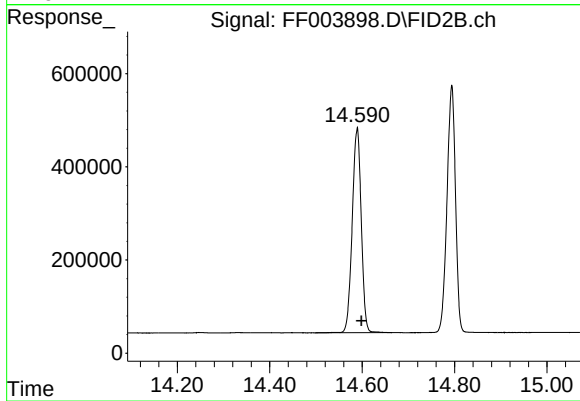

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.589 min
Delta R.T.: -0.009 min
Response: 5960960
Conc: 42.81 ug/ml

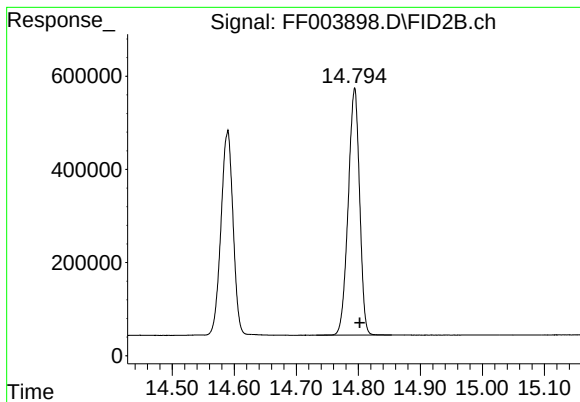

#10 N-TETRACOSANE


R.T.: 14.794 min
Delta R.T.: -0.008 min
Response: 6765355
Conc: 42.76 ug/ml

Instrument :
FID_F
ClientSampleId :

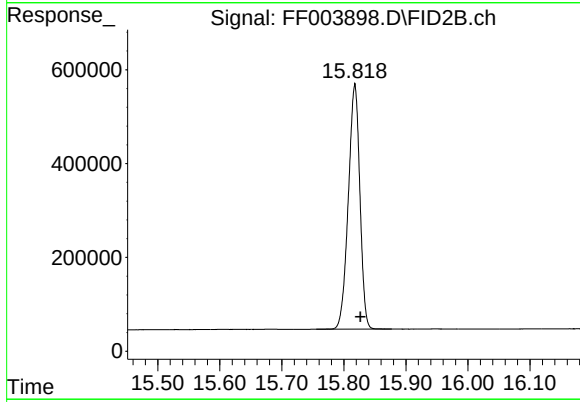

#11 N-HEXACOSANE

R.T.: 15.818 min
Delta R.T.: -0.009 min
Response: 6751146
Conc: 43.74 ug/ml

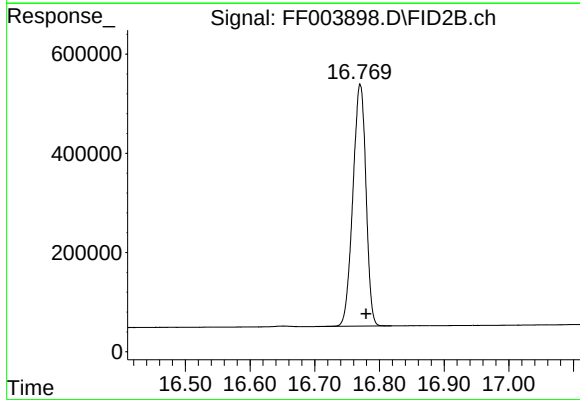

#12 N-OCTACOSANE

R.T.: 16.770 min
Delta R.T.: -0.009 min
Response: 6854095
Conc: 45.36 ug/ml