

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031920\
 Data File : FF006623.D
 Signal(s) : FID2B.ch
 Acq On : 19 Mar 2020 17:44
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 20 01:39:26 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

	Compound	R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.593	2254424	17.517 ug/ml
Target Compounds				
14)	N-DOTRIACONTANE	18.468	118175	0.877 ug/ml
15)	N-TETRATRIACONTANE	19.249	106733	0.945 ug/ml
16)	N-HEXATRIACONTANE	20.015	186488	2.031 ug/ml
17)	N-OCTATRIACONTANE	20.703	87526	1.268 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031920\
Data File : FF006623.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2020 17:44
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 01:39:26 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

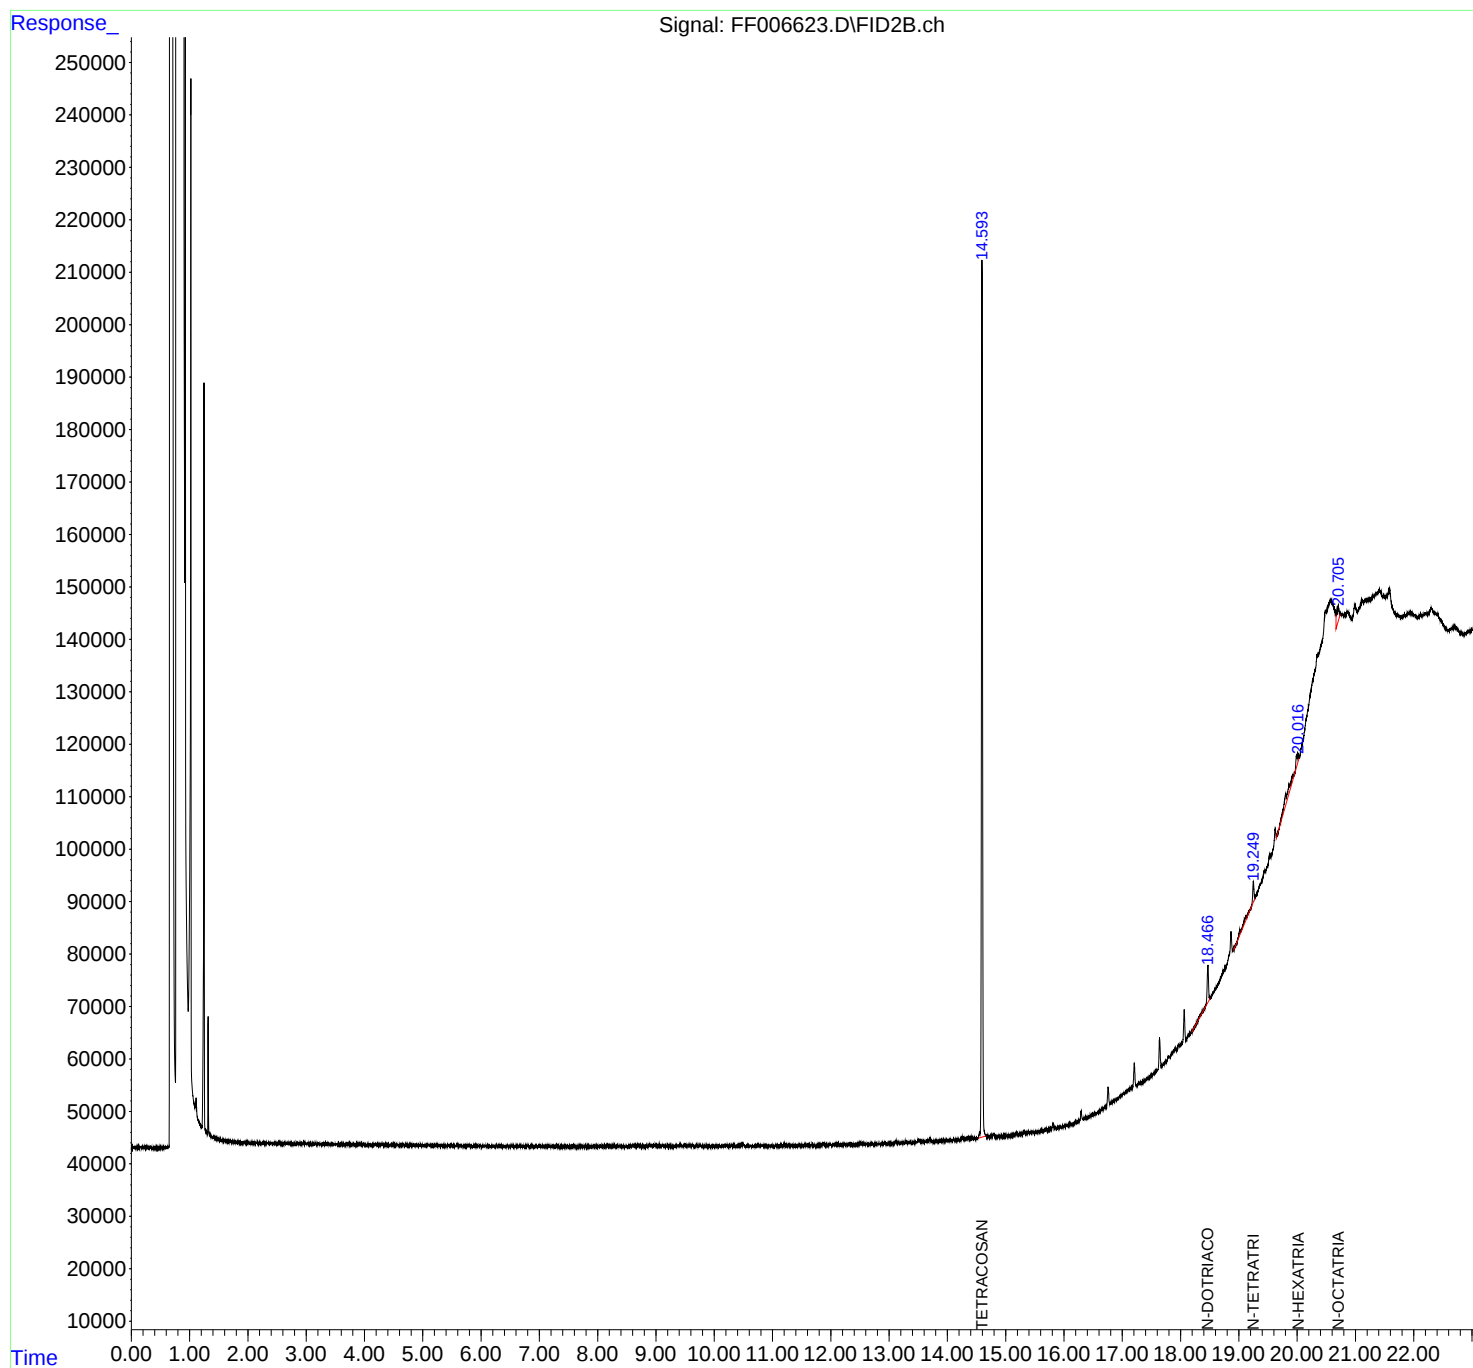

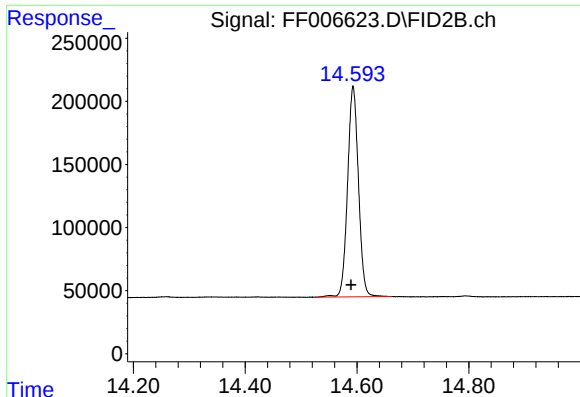


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.593 min
Delta R.T.: 0.003 min
Response: 2254424
Conc: 17.52 ug/ml

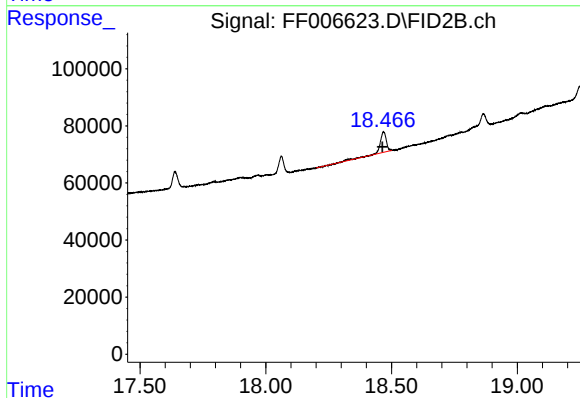


#14 N-DOTRIACONTANE

R.T.: 18.468 min
Delta R.T.: 0.004 min
Response: 118175
Conc: 0.88 ug/ml

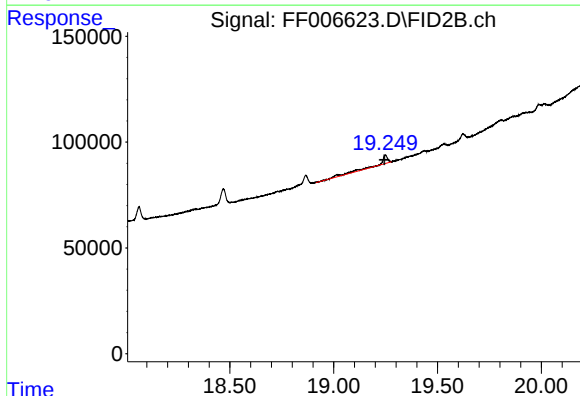


#15 N-TETRATRIACONTANE

R.T.: 19.249 min
Delta R.T.: 0.005 min
Response: 106733
Conc: 0.95 ug/ml

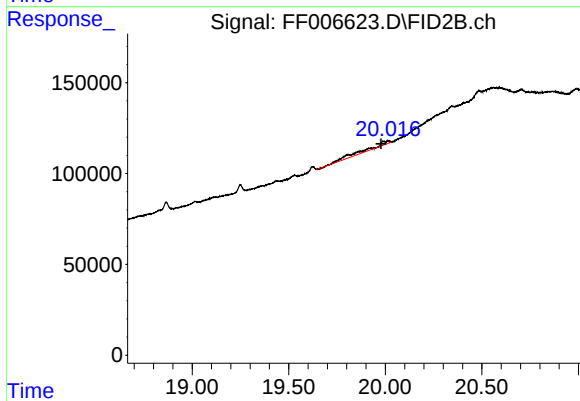

#16 N-HEXATRIACONTANE

R.T.: 20.015 min
Delta R.T.: 0.036 min
Response: 186488
Conc: 2.03 ug/ml

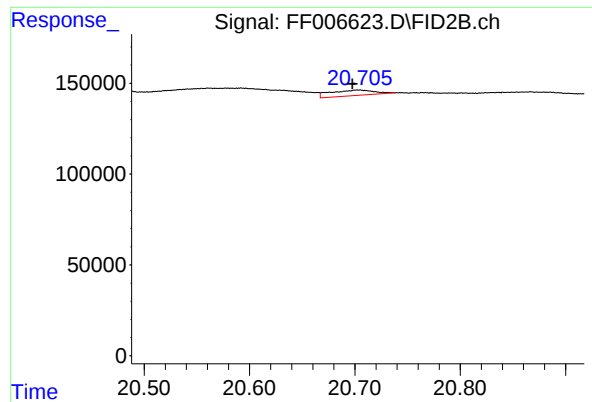

#17 N-OCTATRIACONTANE

R.T.: 20.703 min
Delta R.T.: 0.006 min
Response: 87526
Conc: 1.27 ug/ml