

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031920\
Data File : FF006618.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2020 15:12
Operator : DD\AJ
Sample : L1978-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 01:38:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.596	1876803	14.583 ug/ml

Target Compounds


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF031920\
Data File : FF006618.D
Signal(s) : FID2B.ch
Acq On : 19 Mar 2020 15:12
Operator : DD\AJ
Sample : L1978-03
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 01:38:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

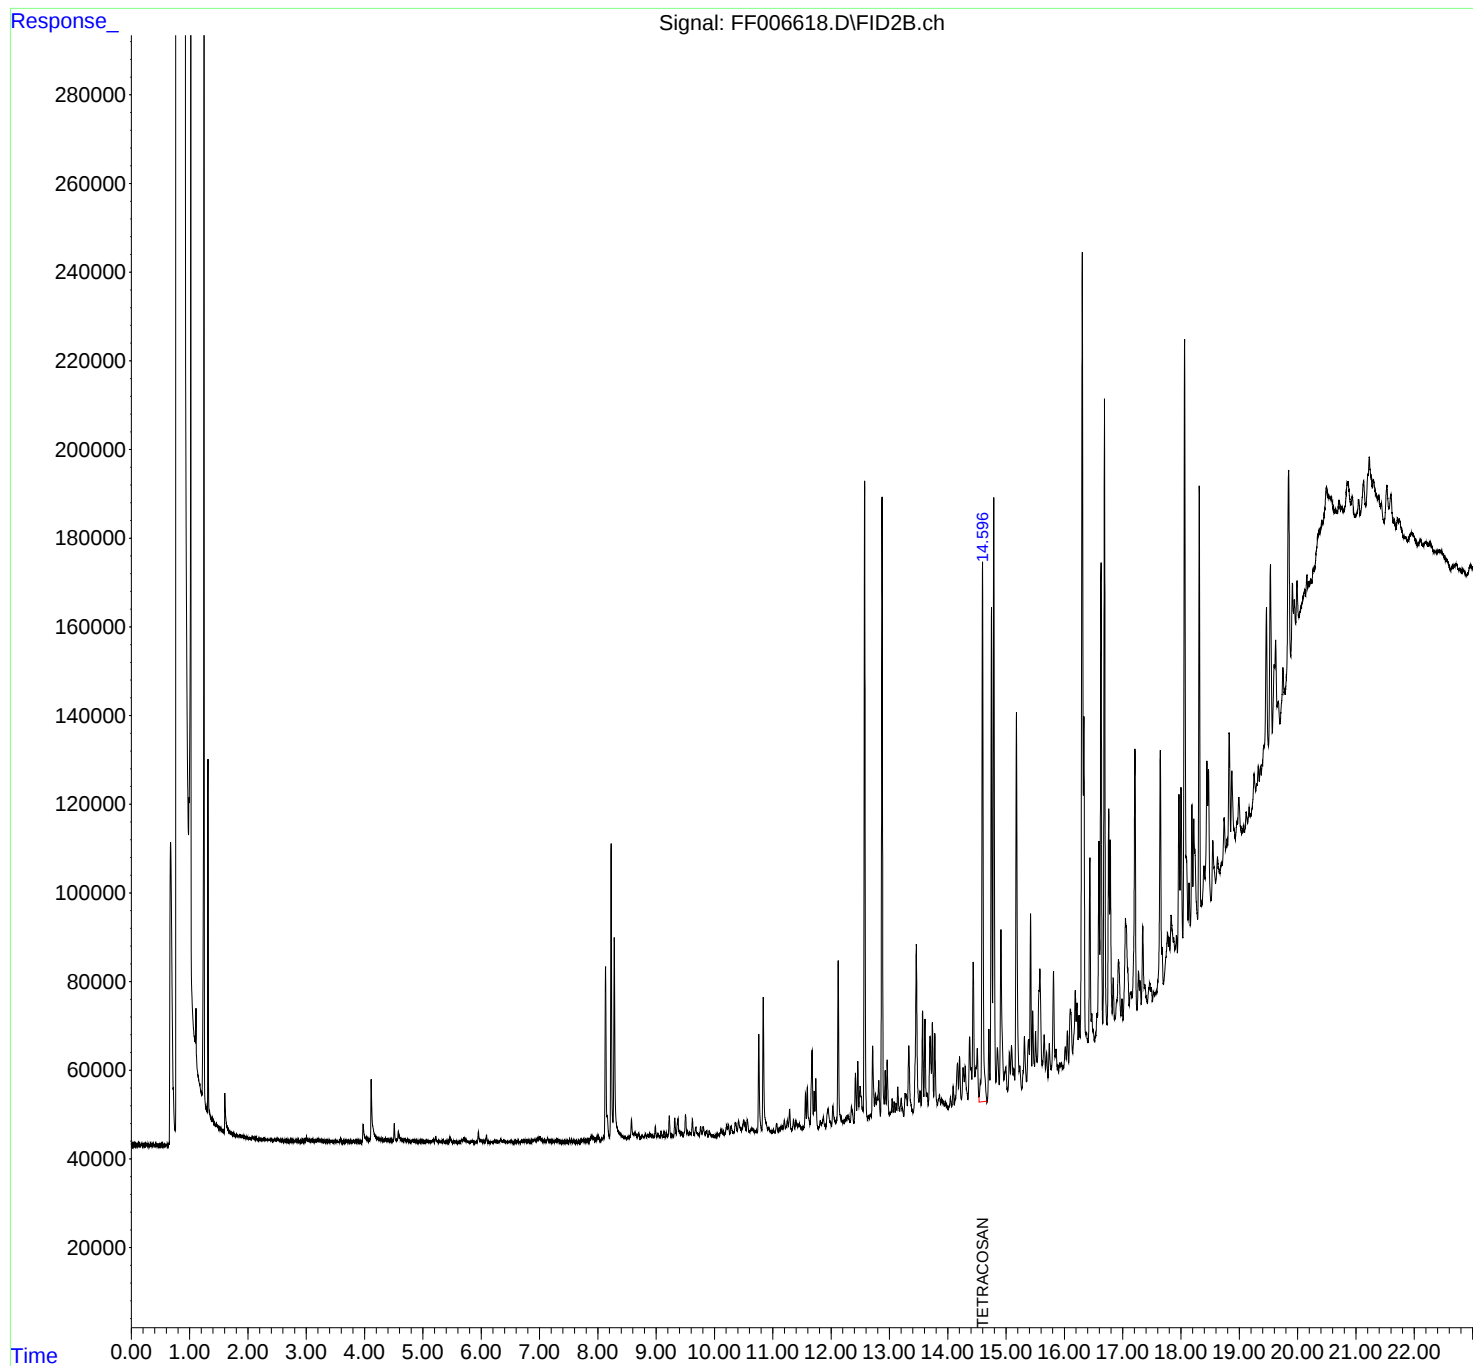

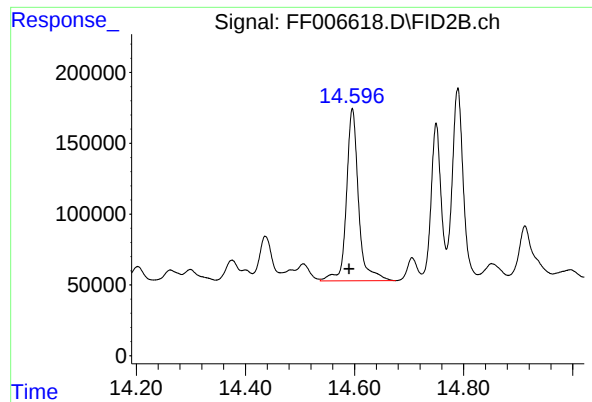

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.596 min
Delta R.T.: 0.006 min
Response: 1876803
Conc: 14.58 ug/ml