

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032019\
 Data File : FF003919.D
 Signal(s) : FID2B.ch
 Acq On : 20 Mar 2019 22:30
 Operator : AJ\SJ
 Sample : K1994-02 200X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 21 09:09:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds	R.T.	Response	Conc Units
2) N-DECANE	4.315	1041410	6.770 ug/ml
3) N-DODECANE	6.337	3419616	21.912 ug/ml
4) N-TETRADECANE	8.131	4379374	27.314 ug/ml
5) N-HEXADECANE	9.732	4353314	26.729 ug/ml
6) N-OCTADECANE	11.174	3347039	20.315 ug/ml
7) N-EICOSANE	12.486	1632827	9.981 ug/ml
8) N-DOCOSANE	13.686	656989	4.071 ug/ml
10) N-TETRACOSANE	14.791	219119	1.385 ug/ml
14) N-DOTRIACONTANE	18.494	84253	0.592 ug/ml
15) N-TETRATRIACONTANE	19.279	84905	0.634 ug/ml
16) N-HEXATRIACONTANE	20.055	1036894	7.947 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032019\
Data File : FF003919.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2019 22:30
Operator : AJ\SJ
Sample : K1994-02 200X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 09:09:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

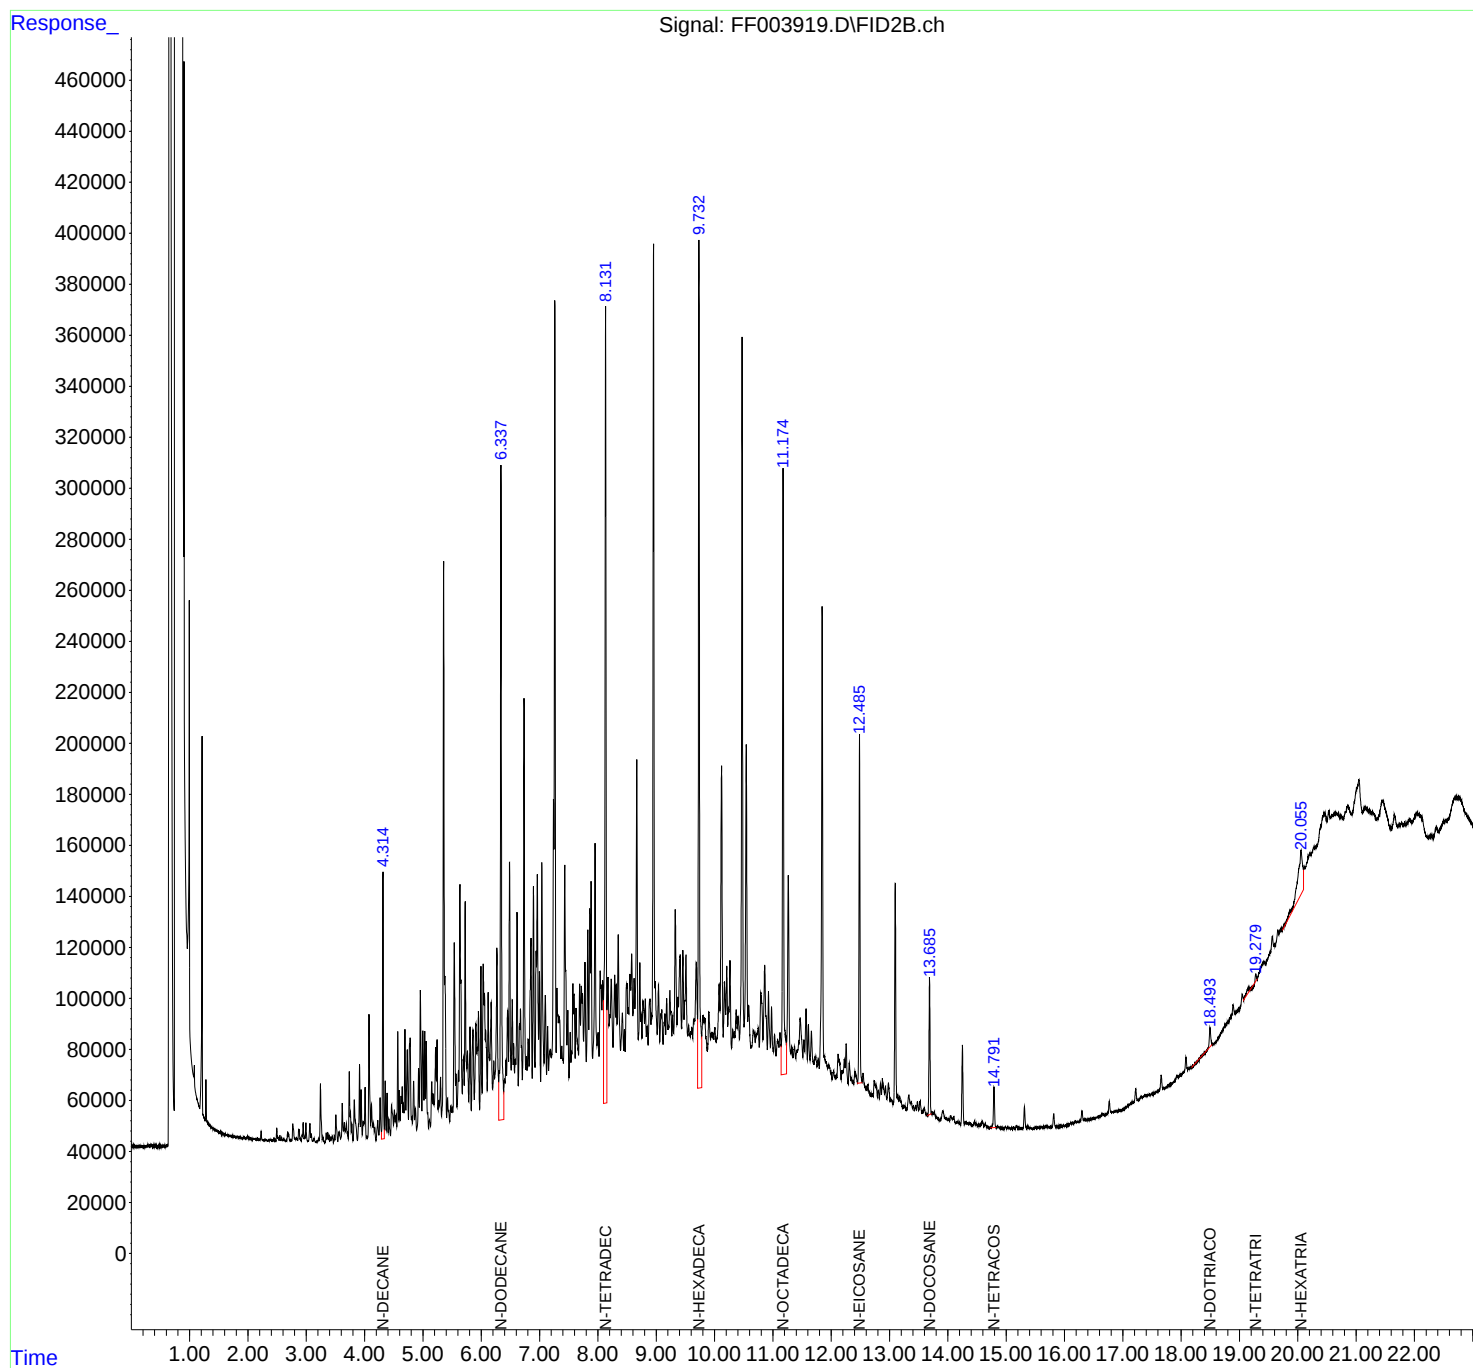

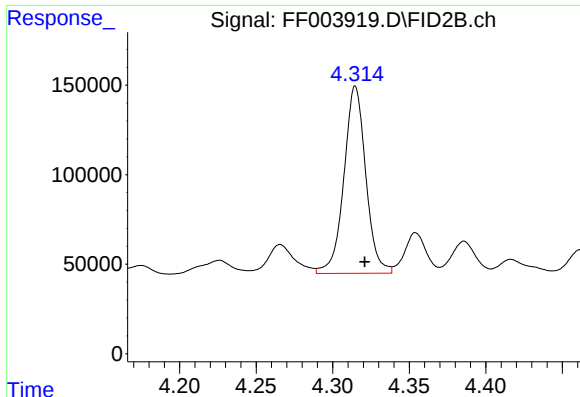


#2 N-DECANE

R.T.: 4.315 min
Delta R.T.: -0.006 min
Response: 1041410
Conc: 6.77 ug/ml

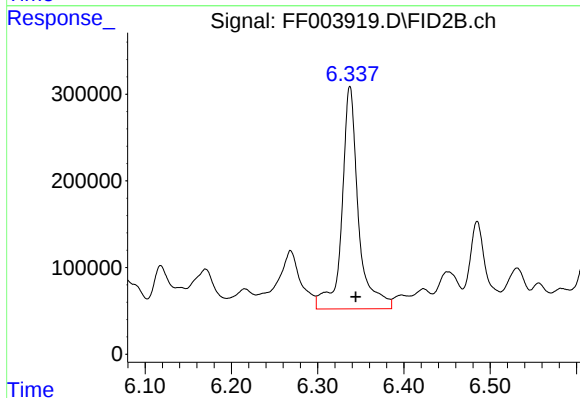


#3 N-DODECANE

R.T.: 6.337 min
Delta R.T.: -0.007 min
Response: 3419616
Conc: 21.91 ug/ml

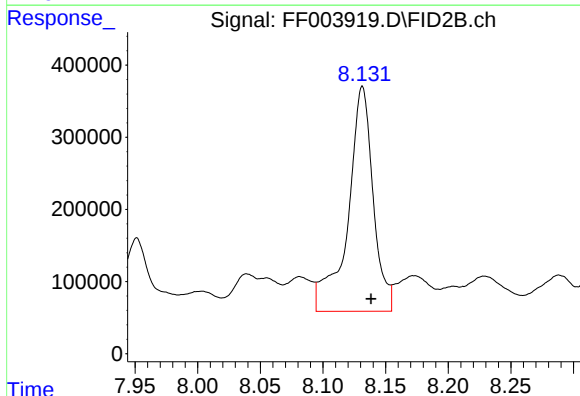


#4 N-TETRADECANE

R.T.: 8.131 min
Delta R.T.: -0.007 min
Response: 4379374
Conc: 27.31 ug/ml

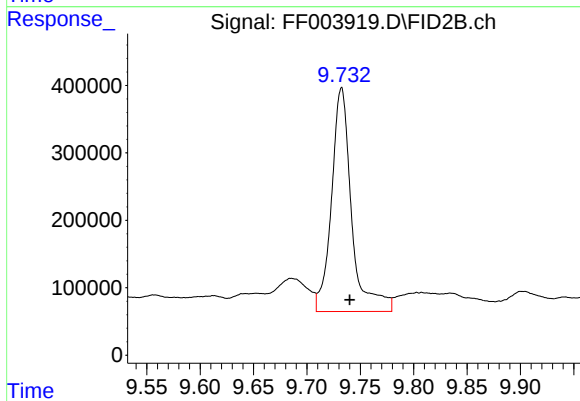


#5 N-HEXADECANE

R.T.: 9.732 min
Delta R.T.: -0.008 min
Response: 4353314
Conc: 26.73 ug/ml

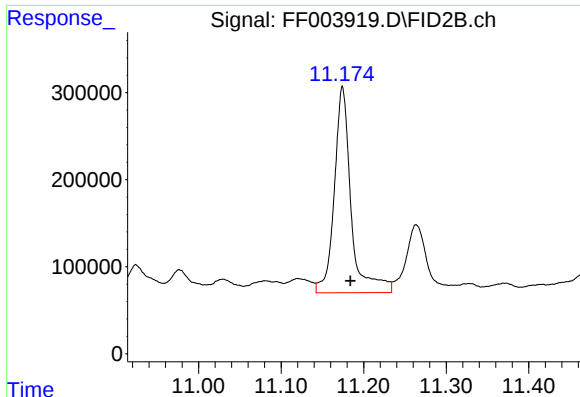


#6 N-OCTADECANE

R.T.: 11.174 min
Delta R.T.: -0.009 min
Response: 3347039
Conc: 20.32 ug/ml

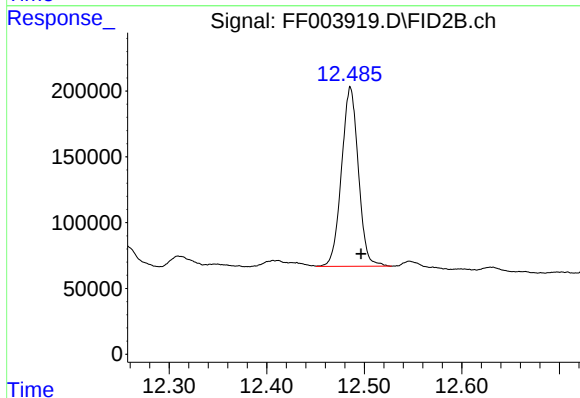


#7 N-EICOSANE

R.T.: 12.486 min
Delta R.T.: -0.011 min
Response: 1632827
Conc: 9.98 ug/ml

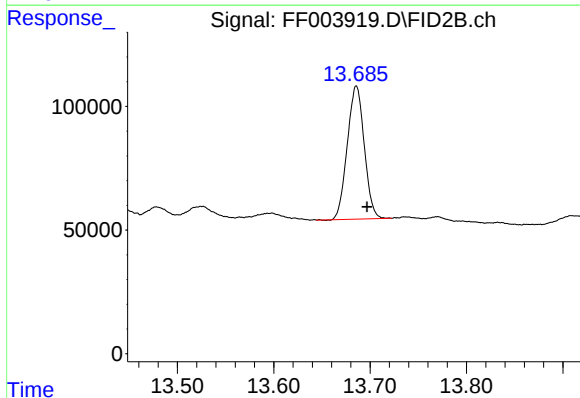


#8 N-DOCOSANE

R.T.: 13.686 min
Delta R.T.: -0.011 min
Response: 656989
Conc: 4.07 ug/ml

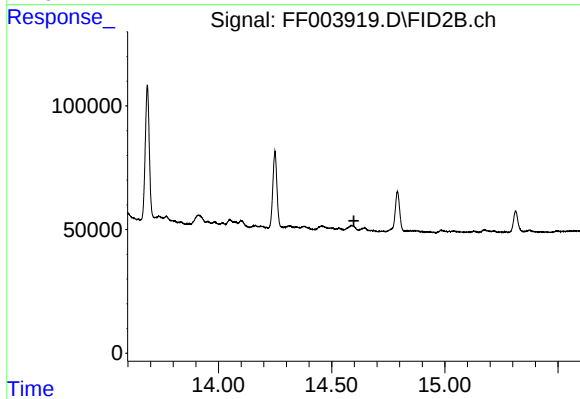


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T.: 14.598 min
Response: 0
Conc: N.D.

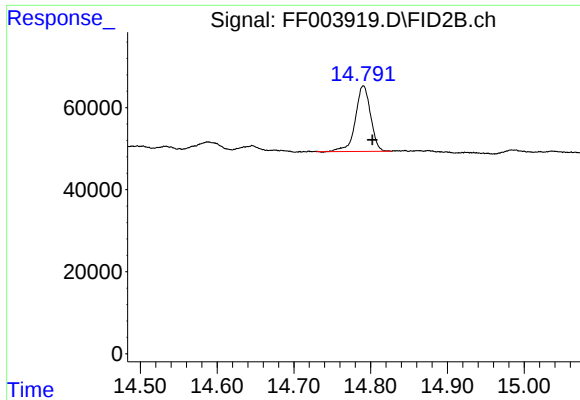


#10 N-TETRACOSANE

R.T.: 14.791 min
Delta R.T.: -0.012 min
Response: 219119
Conc: 1.38 ug/ml

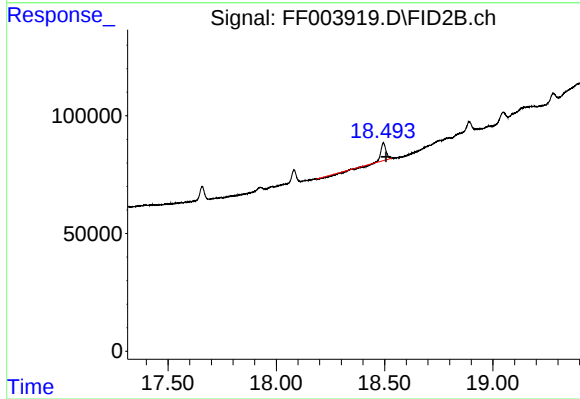


#14 N-DOTRIACONTANE

R.T.: 18.494 min
Delta R.T.: -0.013 min
Response: 84253
Conc: 0.59 ug/ml

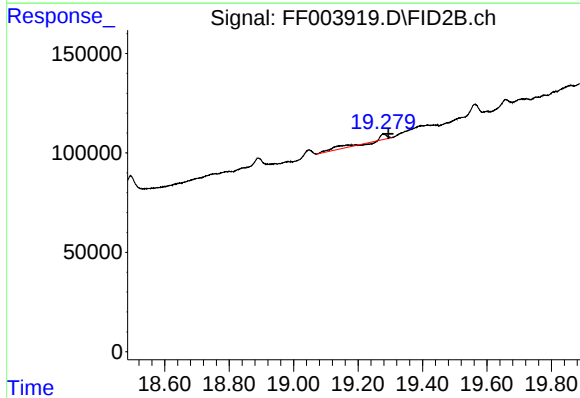

#15 N-TETRATRIACONTANE

R.T.: 19.279 min
Delta R.T.: -0.015 min
Response: 84905
Conc: 0.63 ug/ml

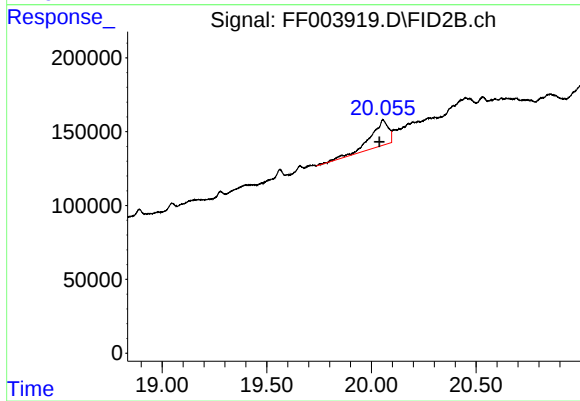

#16 N-HEXATRIACONTANE

R.T.: 20.055 min
Delta R.T.: 0.017 min
Response: 1036894
Conc: 7.95 ug/ml