

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032019\
 Data File : FF003904.D
 Signal(s) : FID2B.ch
 Acq On : 20 Mar 2019 14:50
 Operator : AJ\SJ
 Sample : PB118084BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 20 19:00:14 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.583	1966787	14.126 ug/ml
Target Compounds				
2)	N-DECANE	4.313	2645830	17.201 ug/ml
3)	N-DODECANE	6.334	2616919	16.768 ug/ml
4)	N-TETRADECANE	8.127	2569182	16.024 ug/ml
5)	N-HEXADECANE	9.727	2505938	15.386 ug/ml
6)	N-OCTADECANE	11.170	2447316	14.854 ug/ml
7)	N-EICOSANE	12.481	2359726	14.424 ug/ml
8)	N-DOCOSANE	13.682	2289803	14.188 ug/ml
10)	N-TETRACOSANE	14.787	2241161	14.165 ug/ml
11)	N-HEXACOSANE	15.812	2231220	14.456 ug/ml
12)	N-OCTACOSANE	16.764	2252769	14.908 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032019\
Data File : FF003904.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2019 14:50
Operator : AJ\SJ
Sample : PB118084BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 19:00:14 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

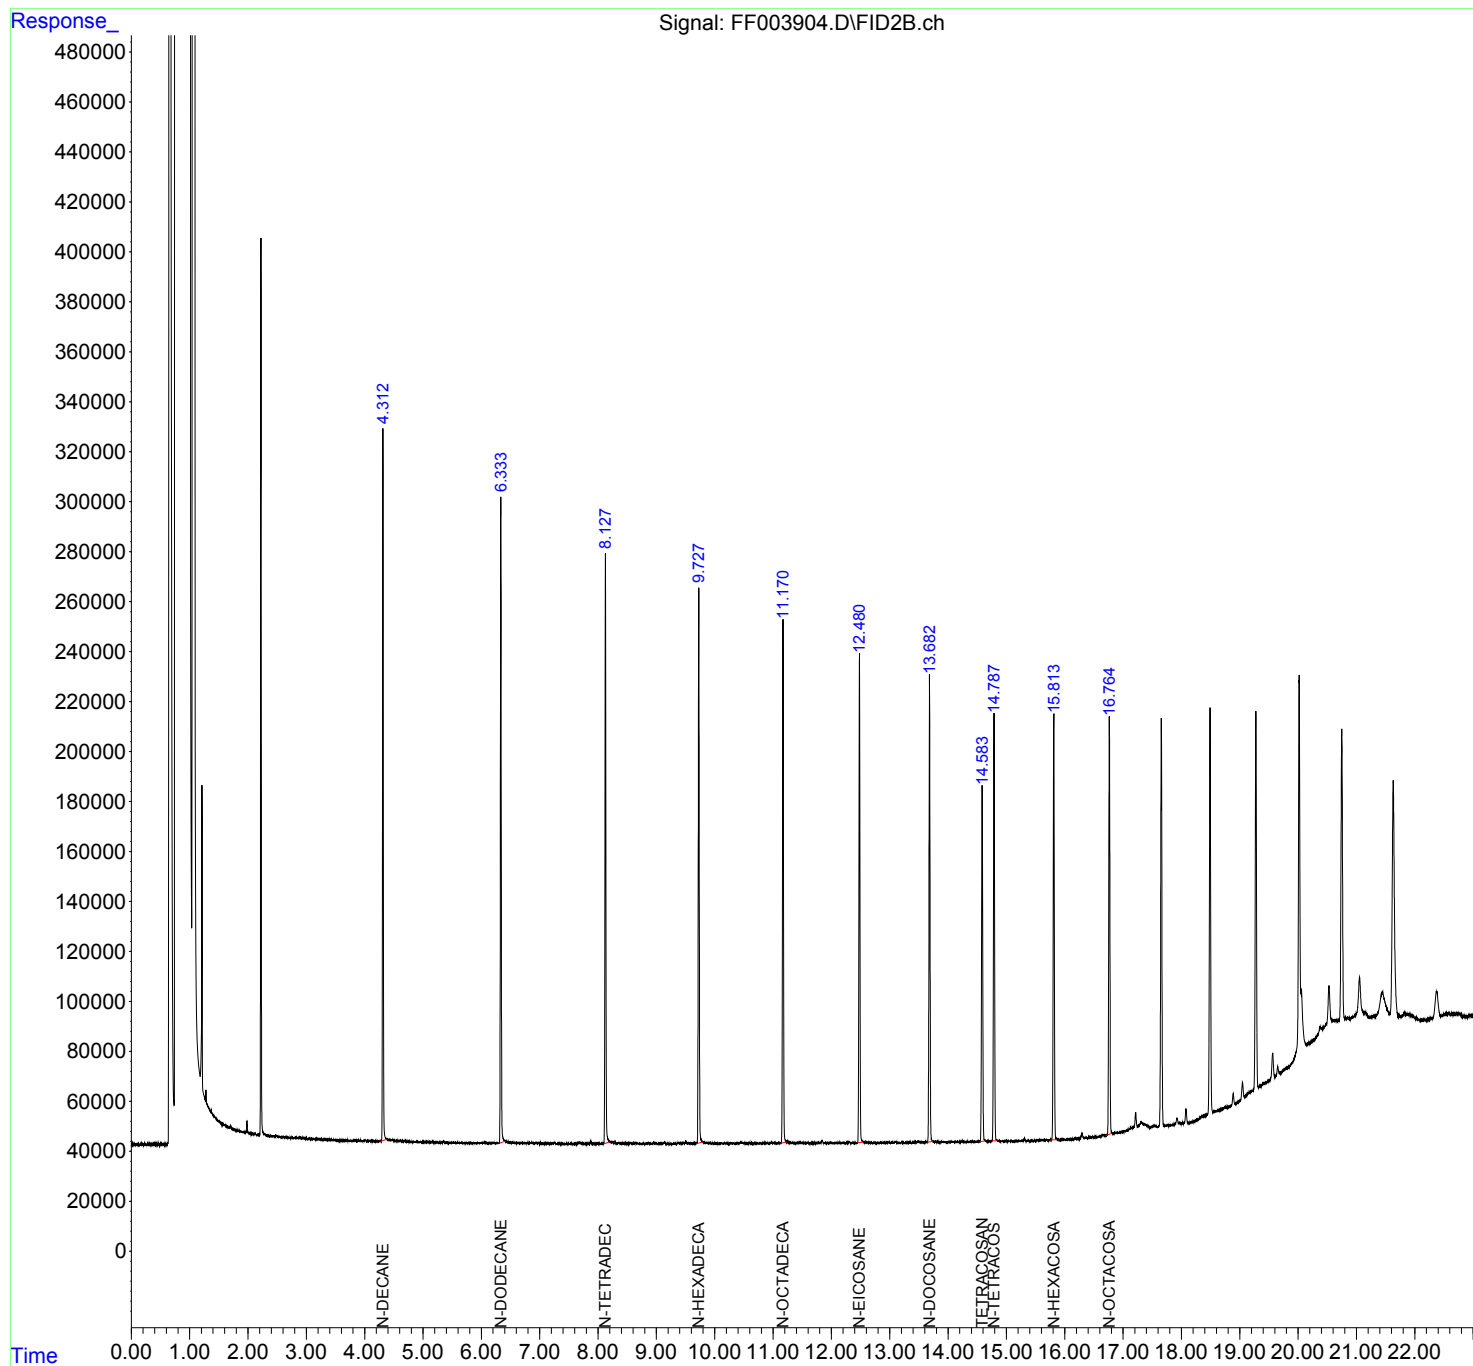

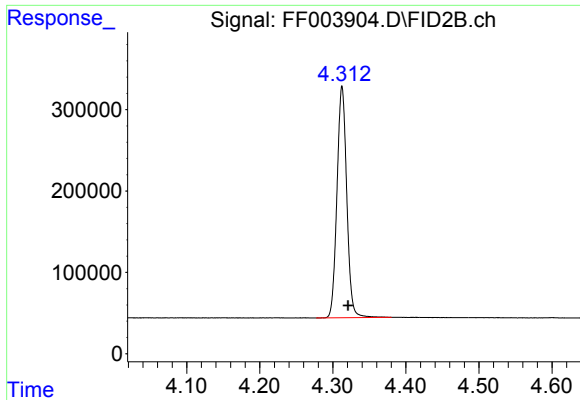


#2 N-DECANE

R.T.: 4.313 min
Delta R.T.: -0.008 min
Response: 2645830
Conc: 17.20 ug/ml

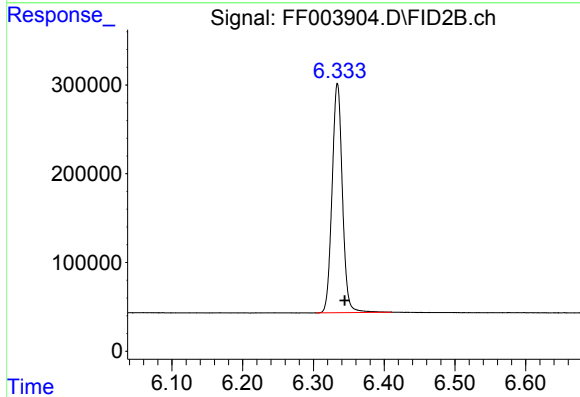


#3 N-DODECANE

R.T.: 6.334 min
Delta R.T.: -0.010 min
Response: 2616919
Conc: 16.77 ug/ml

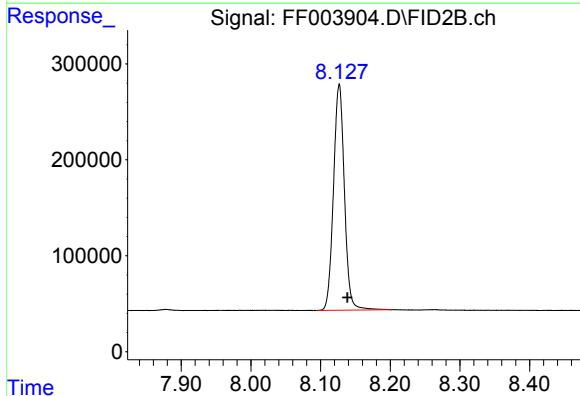


#4 N-TETRADECANE

R.T.: 8.127 min
Delta R.T.: -0.012 min
Response: 2569182
Conc: 16.02 ug/ml

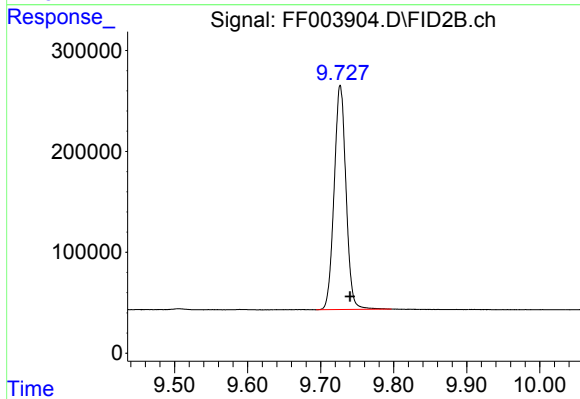


#5 N-HEXADECANE

R.T.: 9.727 min
Delta R.T.: -0.013 min
Response: 2505938
Conc: 15.39 ug/ml

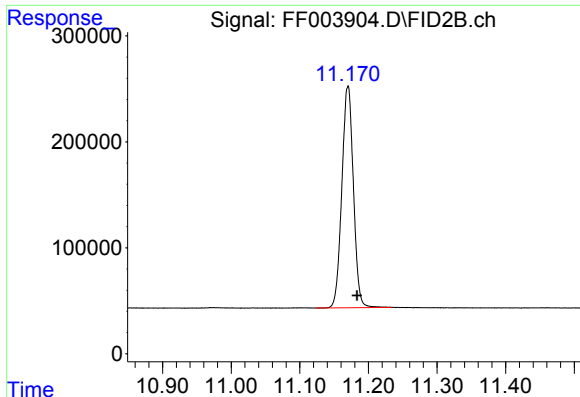


#6 N-OCTADECANE

R.T.: 11.170 min
Delta R.T.: -0.014 min
Response: 2447316
Conc: 14.85 ug/ml

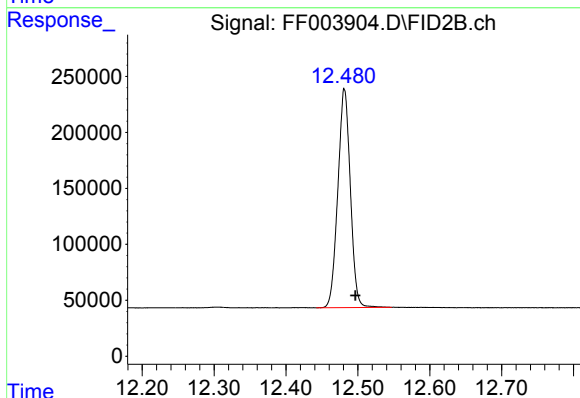


#7 N-EICOSANE

R.T.: 12.481 min
Delta R.T.: -0.015 min
Response: 2359726
Conc: 14.42 ug/ml

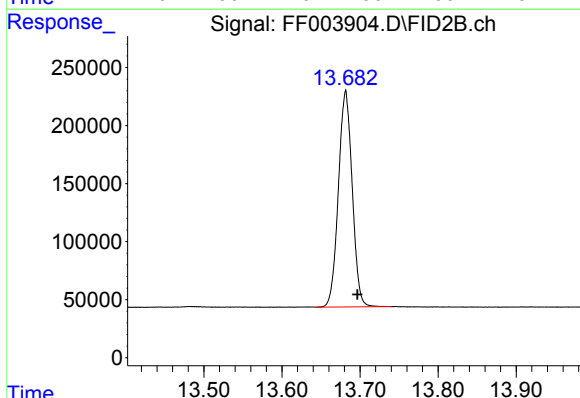


#8 N-DOCOSANE

R.T.: 13.682 min
Delta R.T.: -0.015 min
Response: 2289803
Conc: 14.19 ug/ml

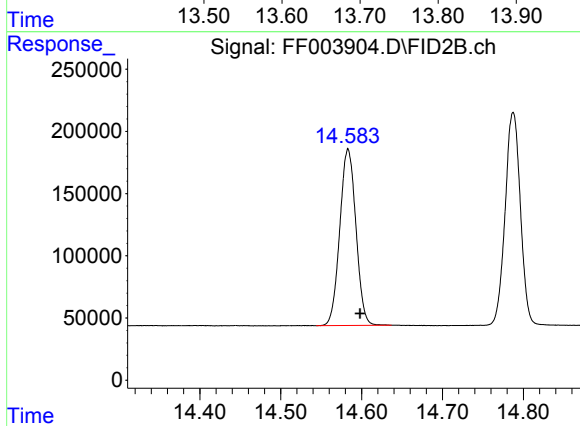


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.583 min
Delta R.T.: -0.015 min
Response: 1966787
Conc: 14.13 ug/ml

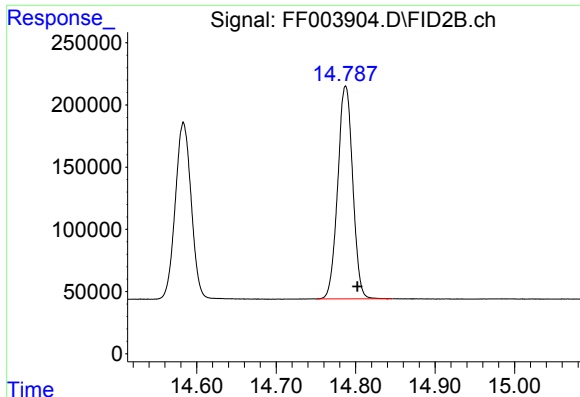


#10 N-TETRACOSANE

R.T.: 14.787 min
Delta R.T.: -0.015 min
Response: 2241161
Conc: 14.16 ug/ml

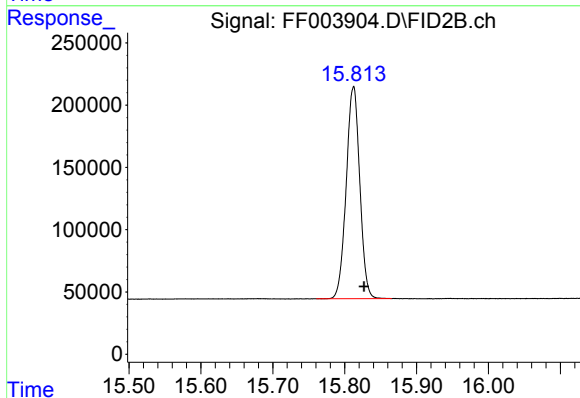

#11 N-HEXACOSANE

R.T.: 15.812 min
Delta R.T.: -0.015 min
Response: 2231220
Conc: 14.46 ug/ml

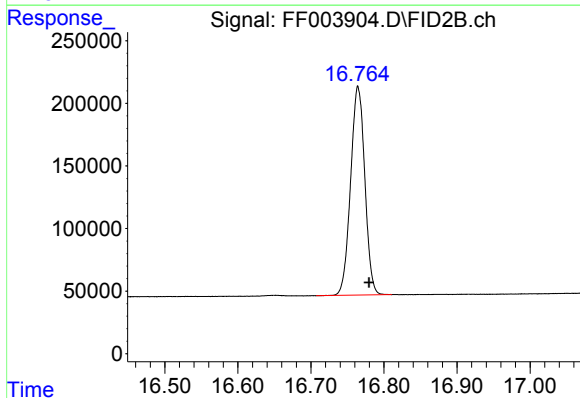

#12 N-OCTACOSANE

R.T.: 16.764 min
Delta R.T.: -0.015 min
Response: 2252769
Conc: 14.91 ug/ml