

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032019\
 Data File : FF003923.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2019 00:33
 Operator : AJ\SJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 21 09:09:53 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	6341033	45.544 ug/ml
Target Compounds			
2) N-DECANE	4.316	8335126	54.187 ug/ml
3) N-DODECANE	6.339	8330477	53.379 ug/ml
4) N-TETRADECANE	8.131	8214893	51.236 ug/ml
5) N-HEXADECANE	9.733	8048981	49.420 ug/ml
6) N-OCTADECANE	11.175	7851228	47.654 ug/ml
7) N-EICOSANE	12.487	7567354	46.257 ug/ml
8) N-DOCOSANE	13.687	7342111	45.493 ug/ml
10) N-TETRACOSANE	14.794	7216207	45.608 ug/ml
11) N-HEXACOSANE	15.817	7166874	46.435 ug/ml
12) N-OCTACOSANE	16.769	7273062	48.130 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032019\
Data File : FF003923.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 00:33
Operator : AJ\SJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 53 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 21 09:09:53 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

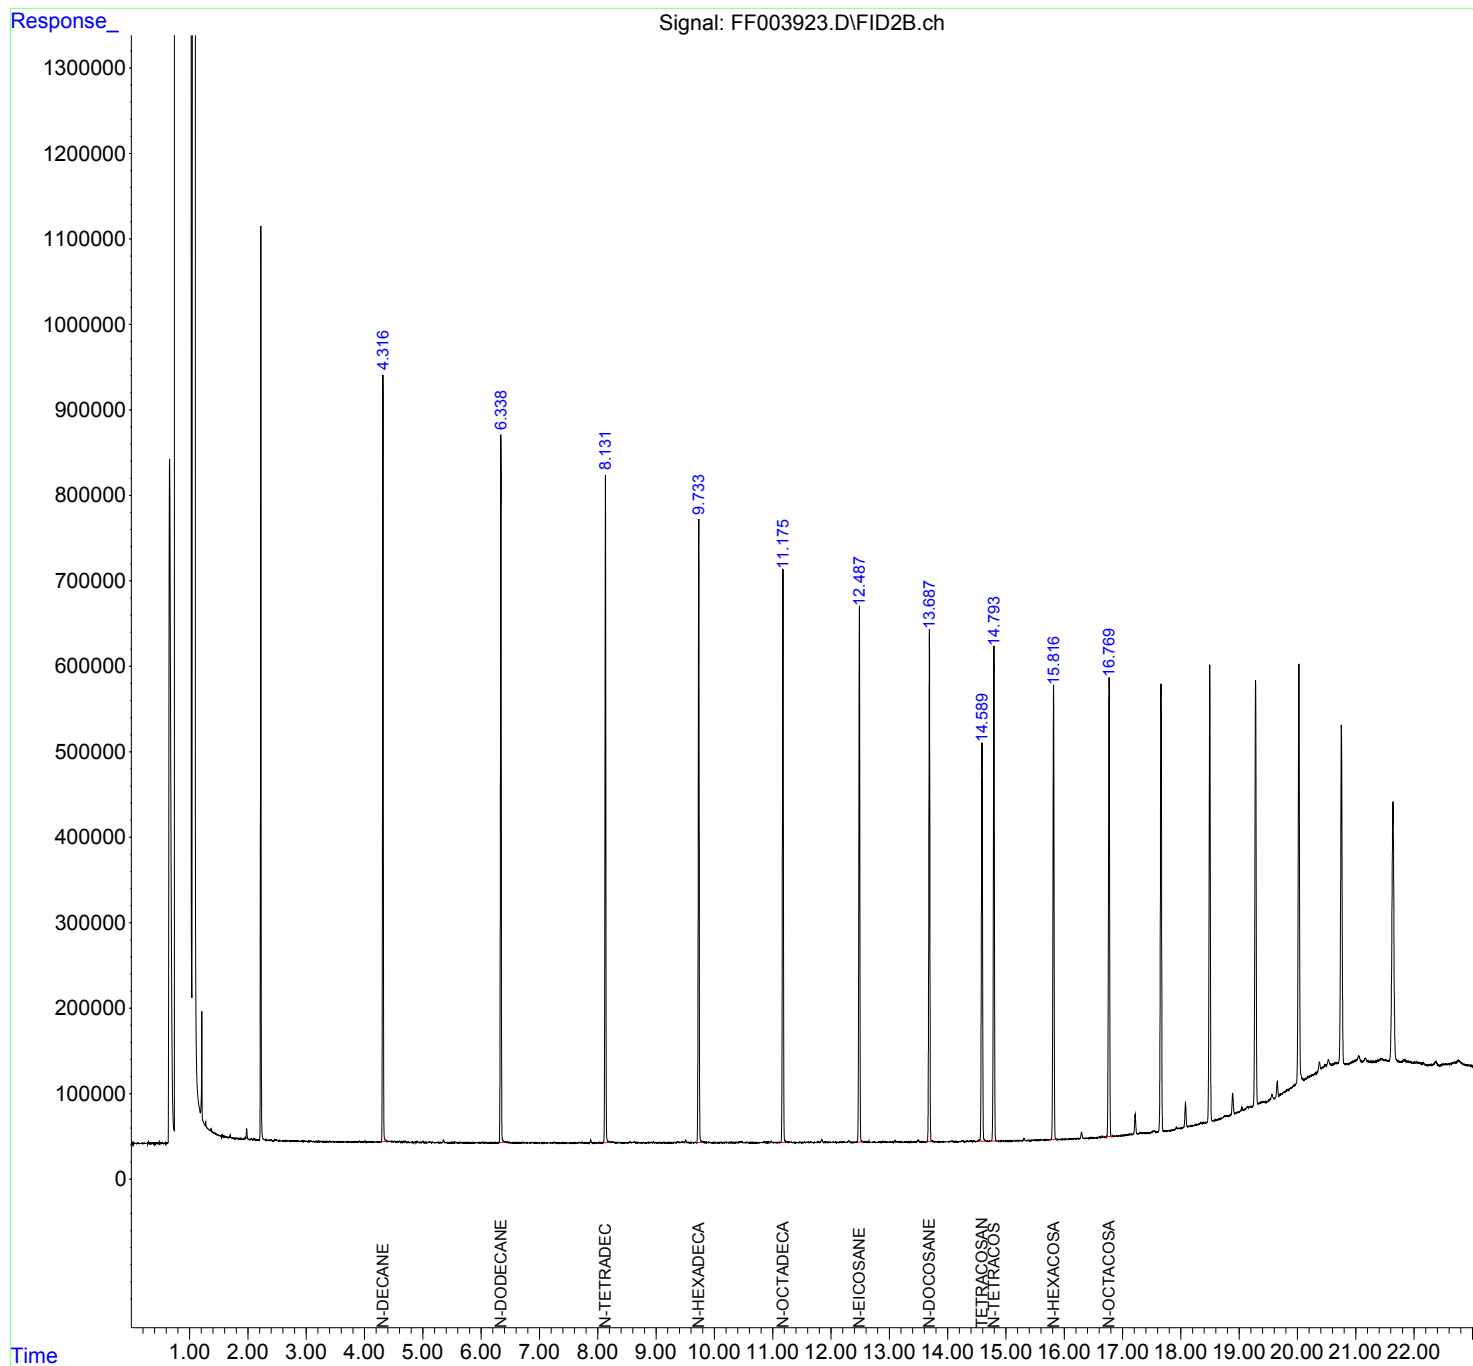

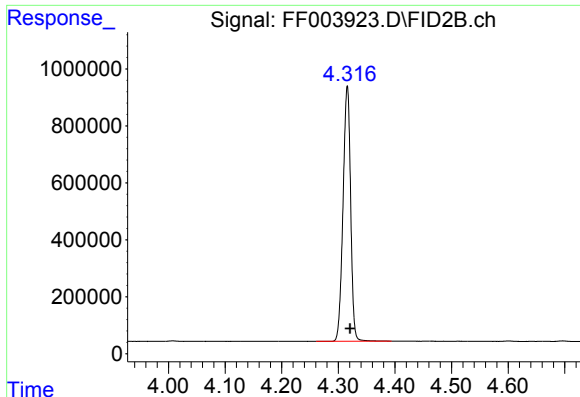


#2 N-DECANE

R.T.: 4.316 min
Delta R.T.: -0.005 min
Response: 8335126
Conc: 54.19 ug/ml

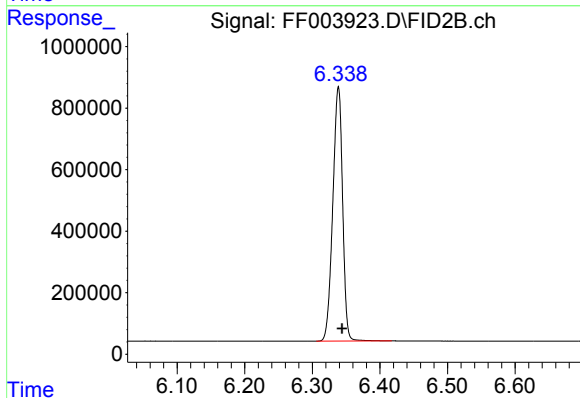


#3 N-DODECANE

R.T.: 6.339 min
Delta R.T.: -0.005 min
Response: 8330477
Conc: 53.38 ug/ml

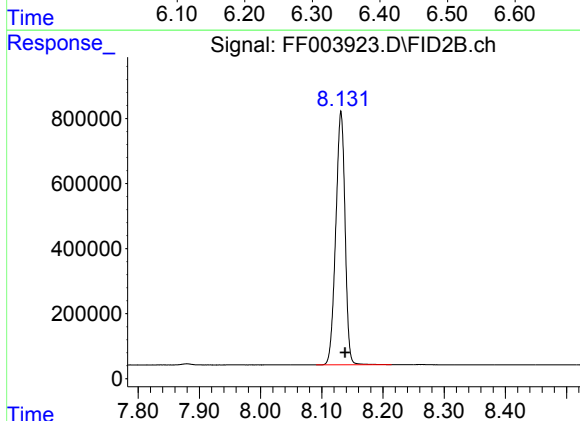


#4 N-TETRADECANE

R.T.: 8.131 min
Delta R.T.: -0.007 min
Response: 8214893
Conc: 51.24 ug/ml

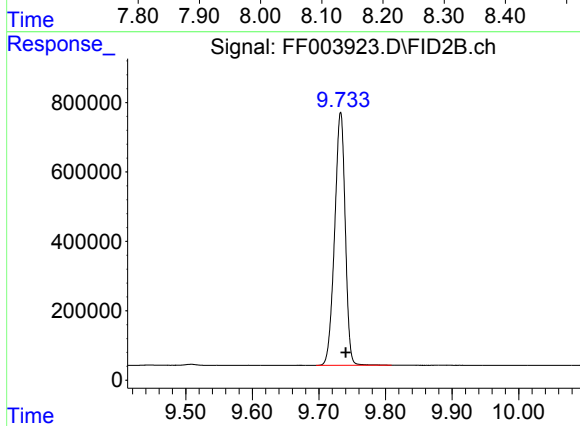


#5 N-HEXADECANE

R.T.: 9.733 min
Delta R.T.: -0.008 min
Response: 8048981
Conc: 49.42 ug/ml

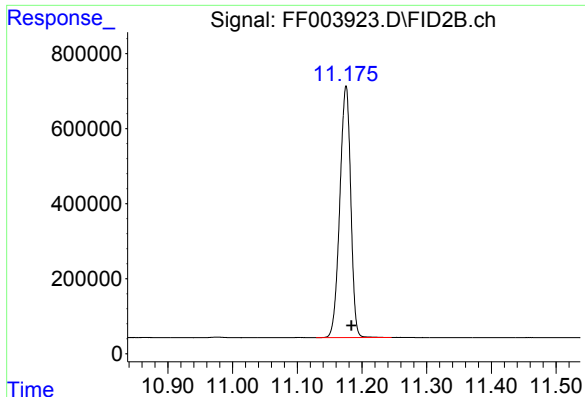


#6 N-OCTADECANE

R.T.: 11.175 min
Delta R.T.: -0.008 min
Response: 7851228
Conc: 47.65 ug/ml

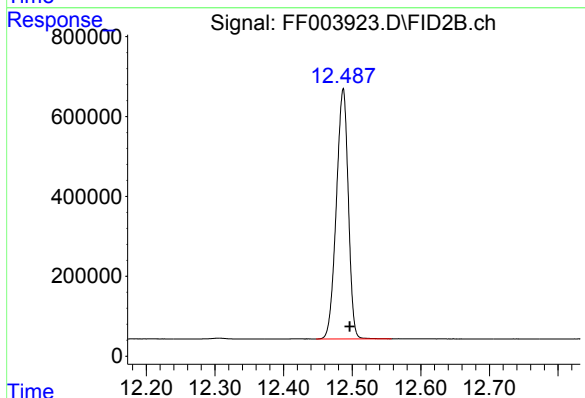


#7 N-EICOSANE

R.T.: 12.487 min
Delta R.T.: -0.010 min
Response: 7567354
Conc: 46.26 ug/ml

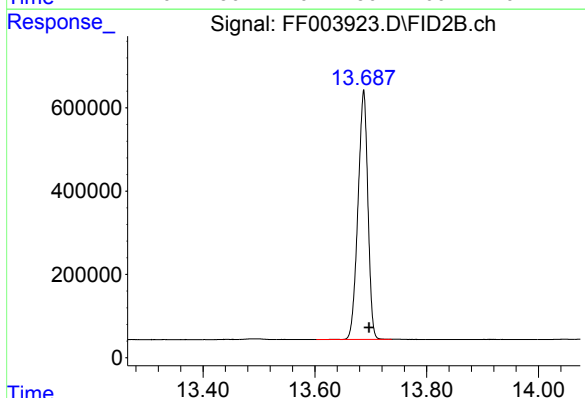


#8 N-DOCOSANE

R.T.: 13.687 min
Delta R.T.: -0.009 min
Response: 7342111
Conc: 45.49 ug/ml

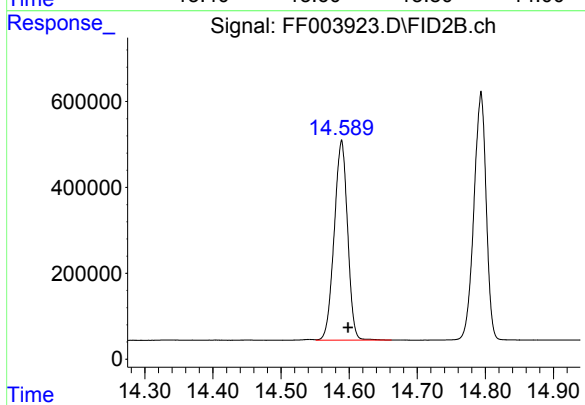


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.589 min
Delta R.T.: -0.009 min
Response: 6341033
Conc: 45.54 ug/ml

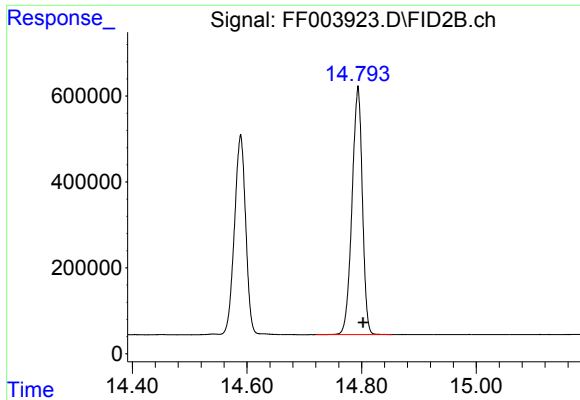


#10 N-TETRACOSANE

R.T.: 14.794 min
Delta R.T.: -0.009 min
Response: 7216207
Conc: 45.61 ug/ml

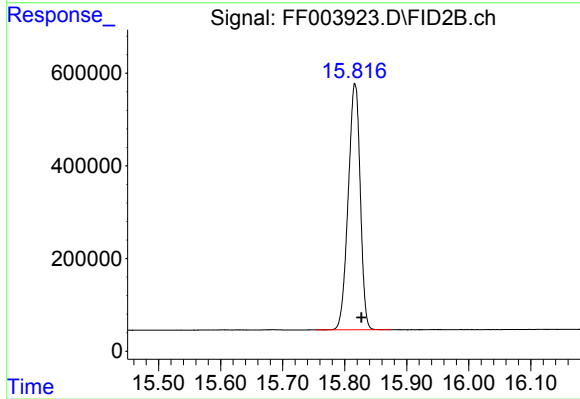

#11 N-HEXACOSANE

R.T.: 15.817 min
Delta R.T.: -0.010 min
Response: 7166874
Conc: 46.43 ug/ml

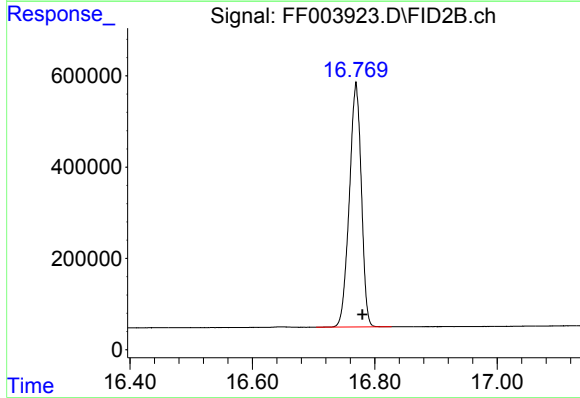

#12 N-OCTACOSANE

R.T.: 16.769 min
Delta R.T.: -0.010 min
Response: 7273062
Conc: 48.13 ug/ml