

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032020\
 Data File : FF006634.D
 Signal(s) : FID2B.ch
 Acq On : 20 Mar 2020 16:27
 Operator : DD\AJ
 Sample : L1749-01MS
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 20 23:43:03 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.595	2007124	15.595 ug/ml
Target Compounds			
2) N-DECANE	4.361	2990633	21.727 ug/ml
3) N-DODECANE	6.376	3152036	22.348 ug/ml
4) N-TETRADECANE	8.166	3092600	21.624 ug/ml
5) N-HEXADECANE	9.762	3176135	21.667 ug/ml
6) N-OCTADECANE	11.200	3221353	21.800 ug/ml
7) N-EICOSANE	12.505	3154036	21.221 ug/ml
8) N-DOCOSANE	13.700	3015511	20.304 ug/ml
10) N-TETRACOSANE	14.797	3524344	23.846 ug/ml
11) N-HEXACOSANE	15.816	3023733	20.865 ug/ml
12) N-OCTACOSANE	16.763	3408424	23.798 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032020\
Data File : FF006634.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2020 16:27
Operator : DD\AJ
Sample : L1749-01MS
Misc :
ALS Vial : 60 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 20 23:43:03 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

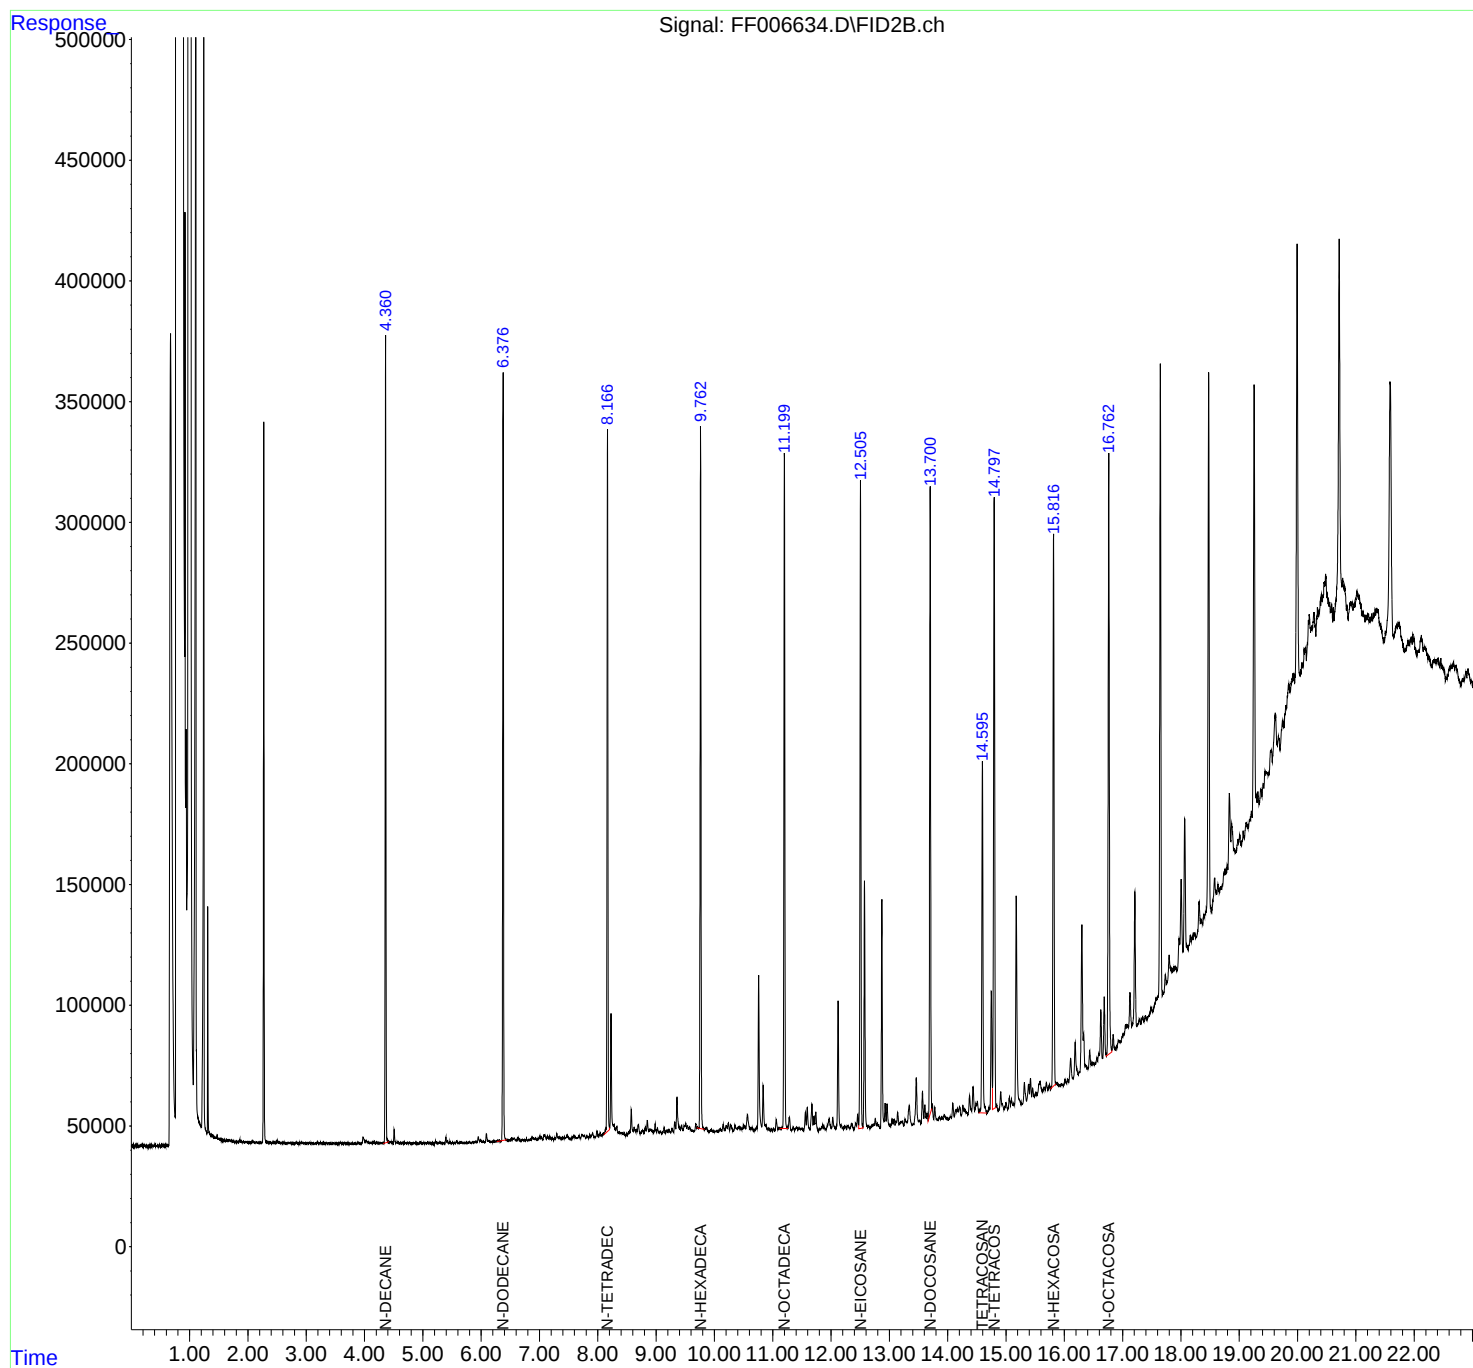

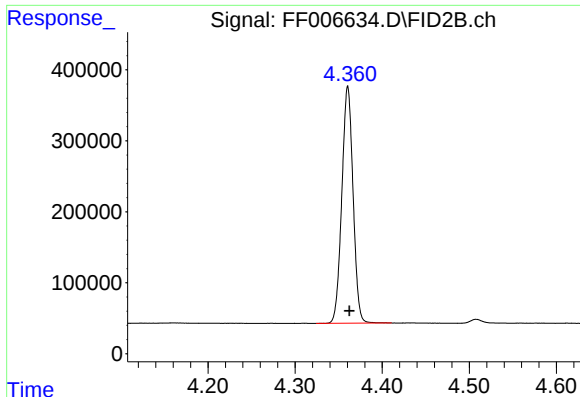


#2 N-DECANE

R.T.: 4.361 min
Delta R.T.: -0.002 min
Response: 2990633
Conc: 21.73 ug/ml

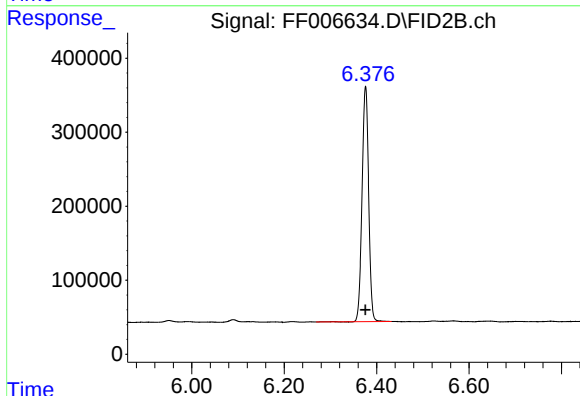


#3 N-DODECANE

R.T.: 6.376 min
Delta R.T.: 0.000 min
Response: 3152036
Conc: 22.35 ug/ml

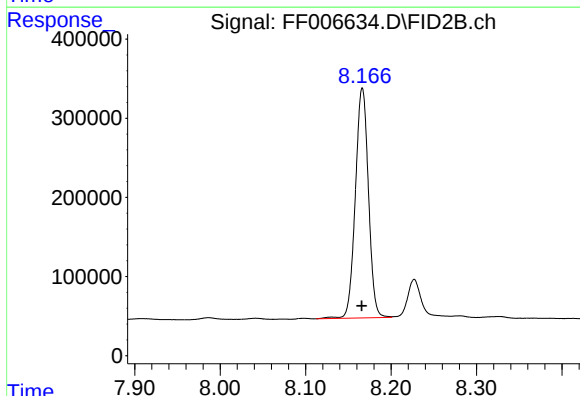


#4 N-TETRADECANE

R.T.: 8.166 min
Delta R.T.: 0.000 min
Response: 3092600
Conc: 21.62 ug/ml

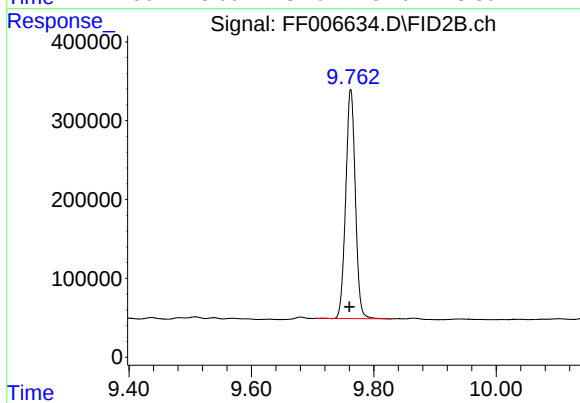


#5 N-HEXADECANE

R.T.: 9.762 min
Delta R.T.: 0.002 min
Response: 3176135
Conc: 21.67 ug/ml

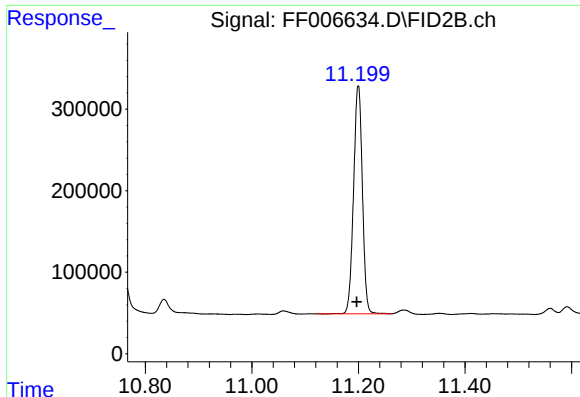


#6 N-OCTADECANE

R.T.: 11.200 min
Delta R.T.: 0.003 min
Response: 3221353
Conc: 21.80 ug/ml

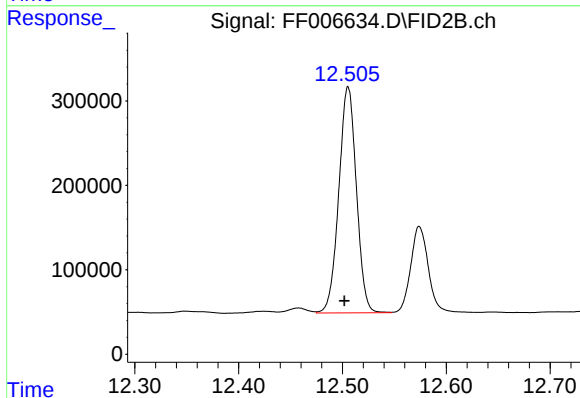


#7 N-EICOSANE

R.T.: 12.505 min
Delta R.T.: 0.004 min
Response: 3154036
Conc: 21.22 ug/ml

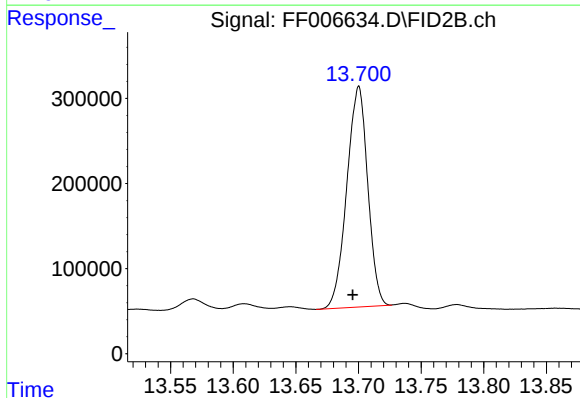


#8 N-DOCOSANE

R.T.: 13.700 min
Delta R.T.: 0.005 min
Response: 3015511
Conc: 20.30 ug/ml

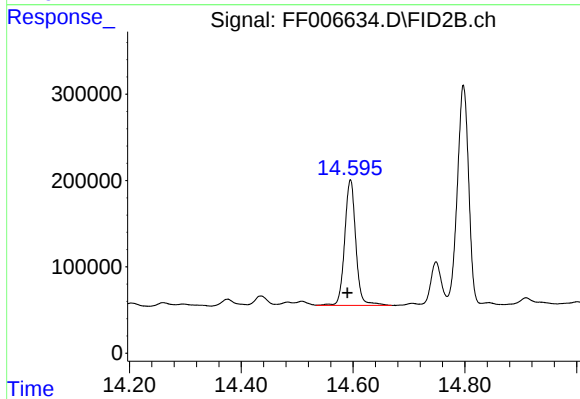


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.595 min
Delta R.T.: 0.006 min
Response: 2007124
Conc: 15.60 ug/ml

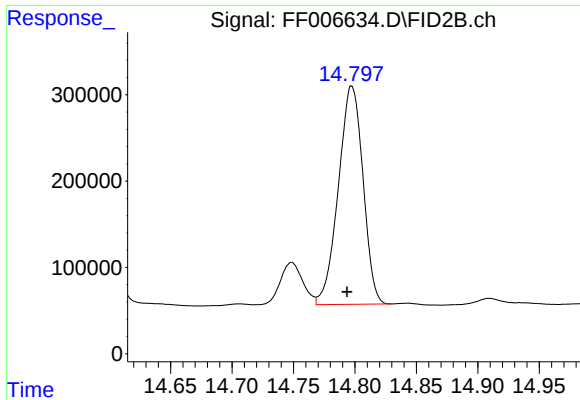


#10 N-TETRACOSANE

R.T.: 14.797 min
Delta R.T.: 0.004 min
Response: 3524344
Conc: 23.85 ug/ml

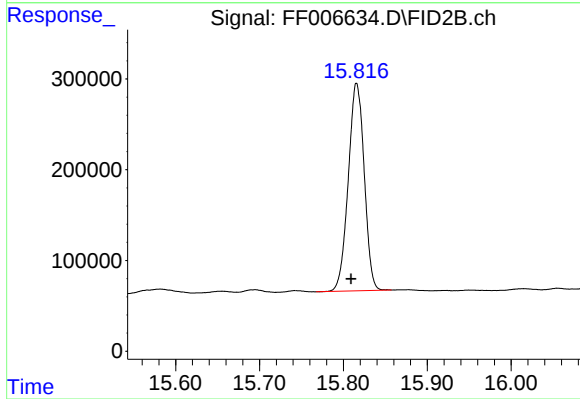

#11 N-HEXACOSANE

R.T.: 15.816 min
Delta R.T.: 0.007 min
Response: 3023733
Conc: 20.87 ug/ml

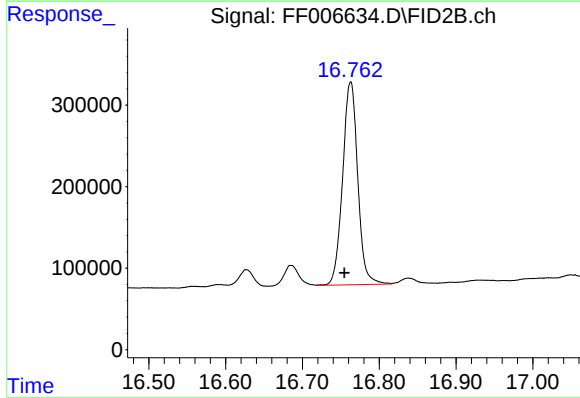

#12 N-OCTACOSANE

R.T.: 16.763 min
Delta R.T.: 0.008 min
Response: 3408424
Conc: 23.80 ug/ml