

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
Data File : FF012312.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2023 14:07
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 21 03:32:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.028	2134287	19.071 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.918	41431	0.399 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
Data File : FF012312.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2023 14:07
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 21 03:32:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

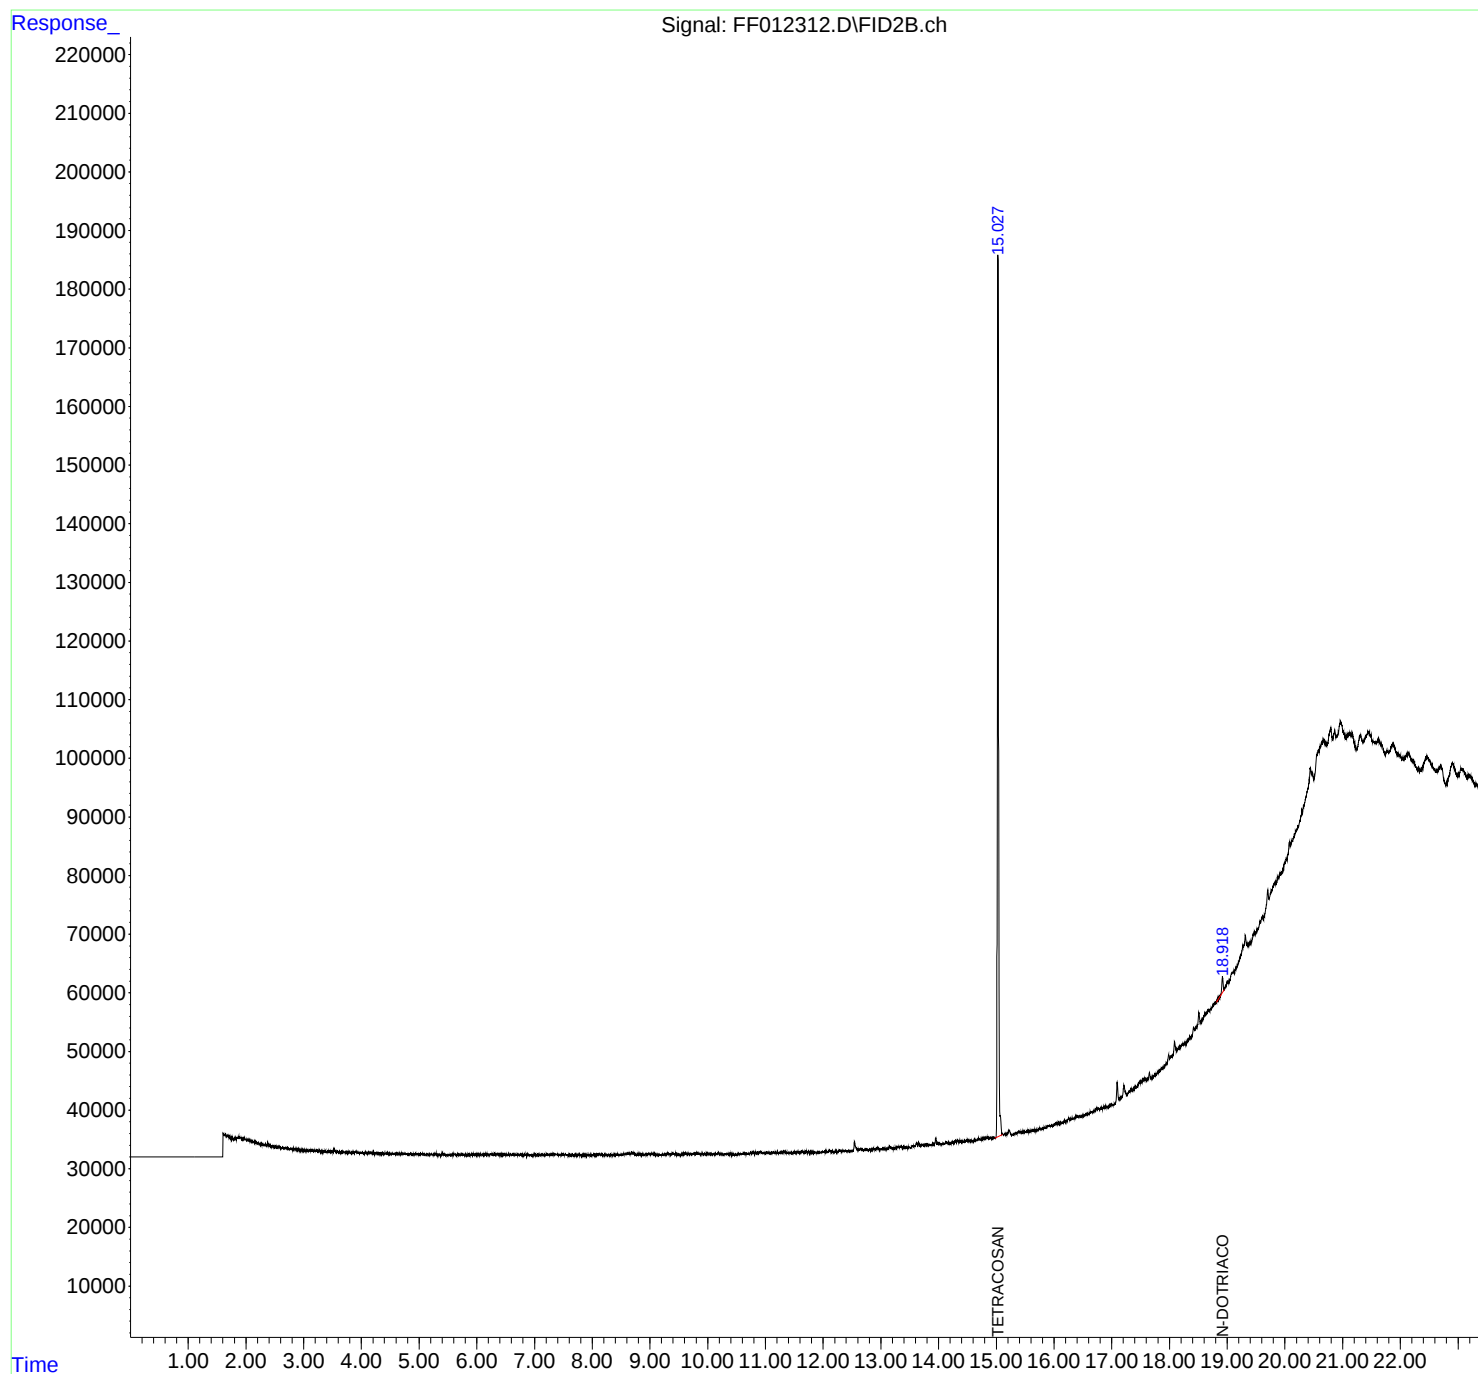

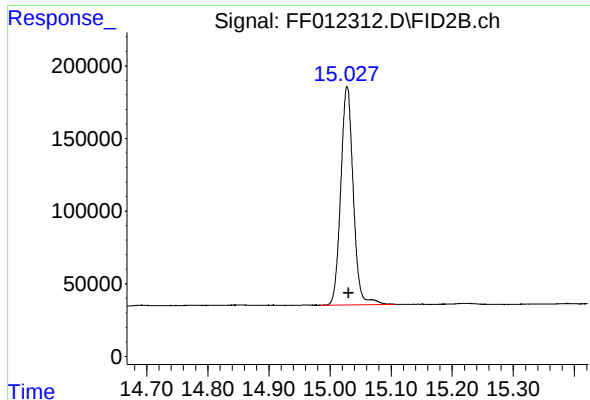


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.028 min
Delta R.T.: -0.002 min
Response: 2134287
Conc: 19.07 ug/ml

Instrument :

FID_F

ClientSampleId :

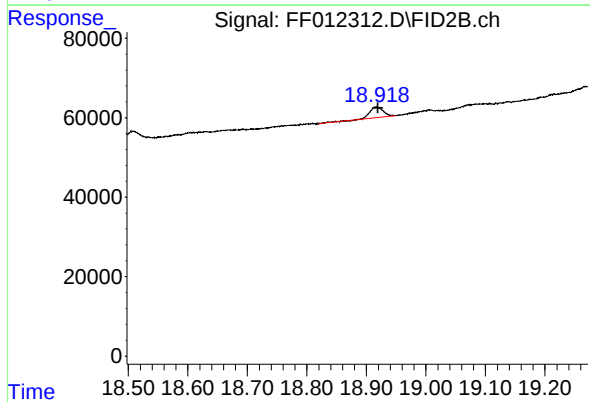

#14 N-DOTRIACONTANE

R.T.: 18.918 min
Delta R.T.: -0.002 min
Response: 41431
Conc: 0.40 ug/ml