

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
 Data File : FF012320.D
 Signal(s) : FID2B.ch
 Acq On : 20 Mar 2023 19:06
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 21 03:33:40 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.027	2079974	18.586 ug/ml
Target Compounds			
14) N-DOTRIACONTANE	18.917	45805	0.441 ug/ml
16) N-HEXATRIACONTANE	20.438	45060	0.514 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
Data File : FF012320.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2023 19:06
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 21 03:33:40 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

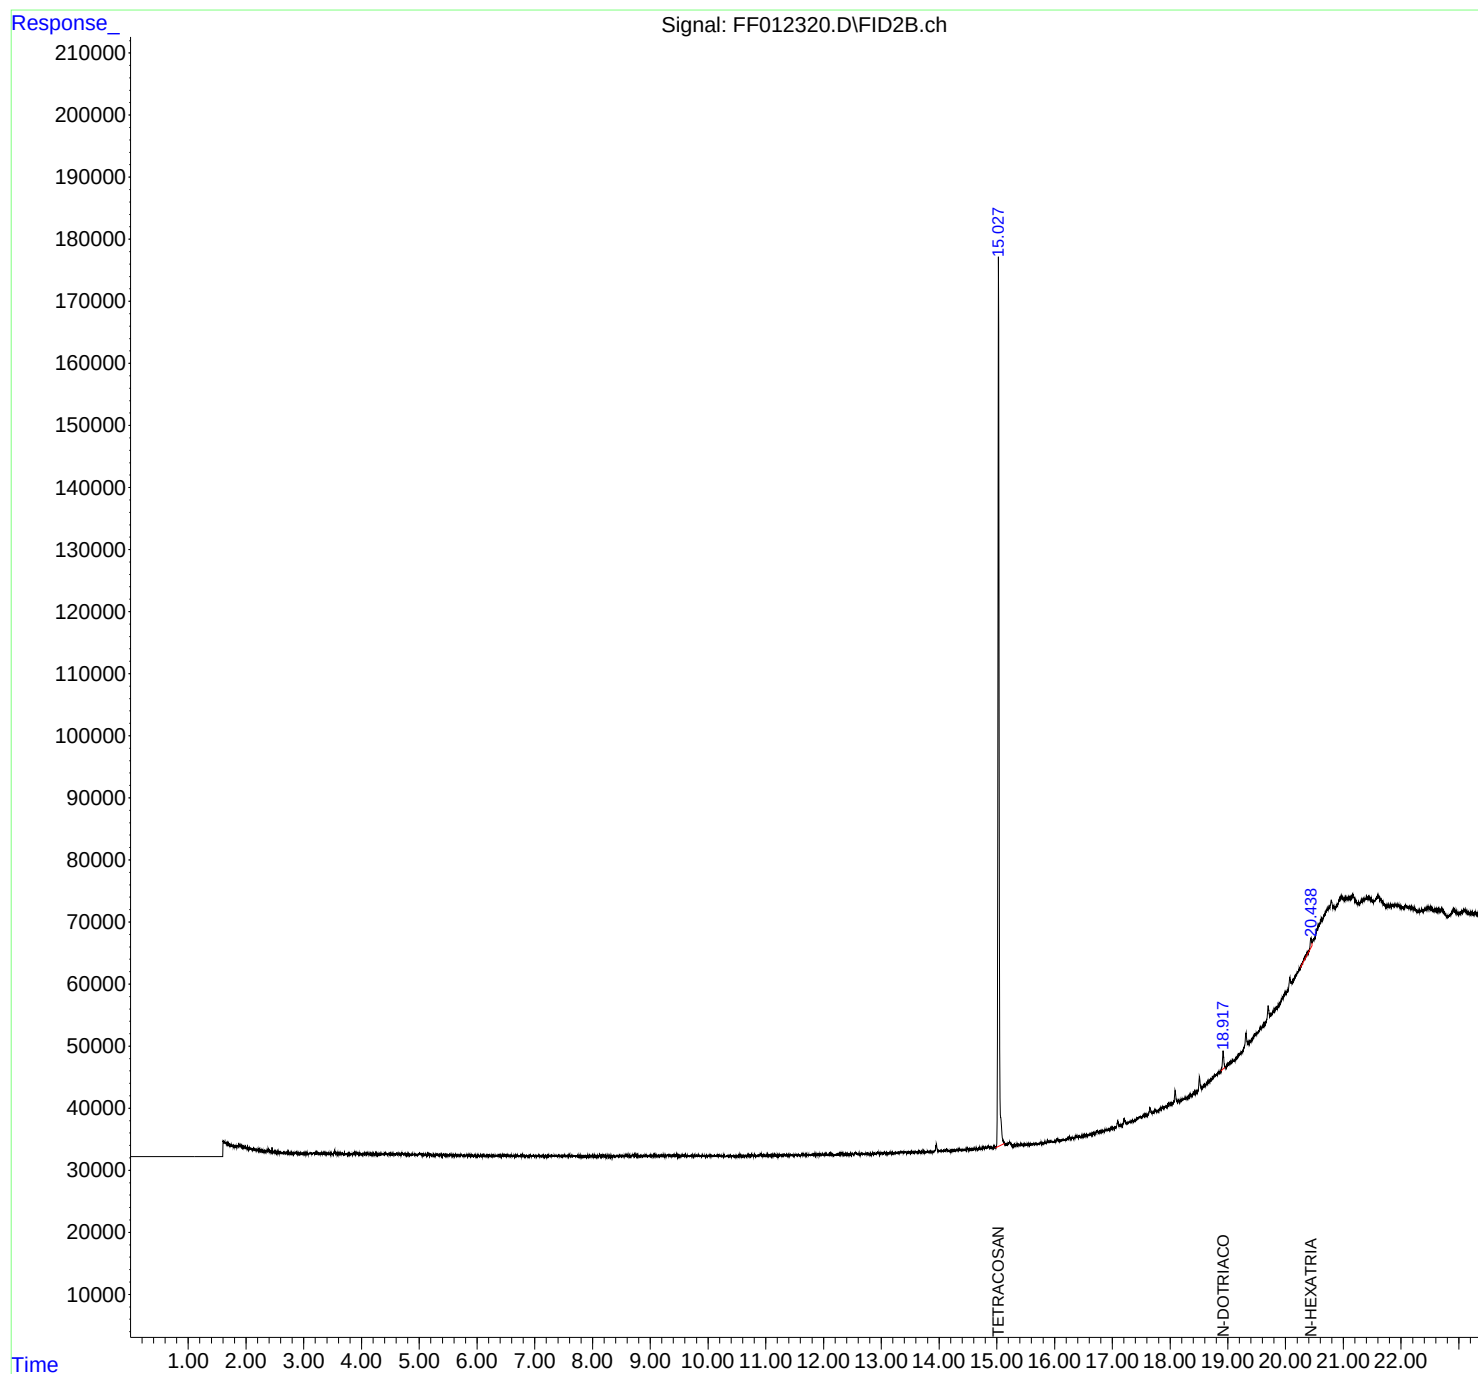

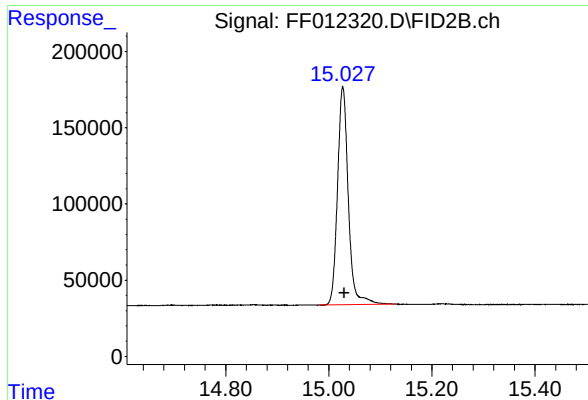


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.027 min
Delta R.T.: -0.003 min
Response: 2079974
Conc: 18.59 ug/ml

Instrument :


FID_F

ClientSampleId :

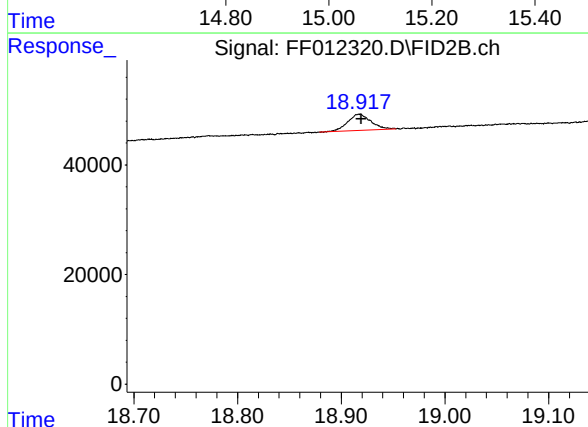

#14 N-DOTRIACONTANE

R.T.: 18.917 min
Delta R.T.: -0.002 min
Response: 45805
Conc: 0.44 ug/ml

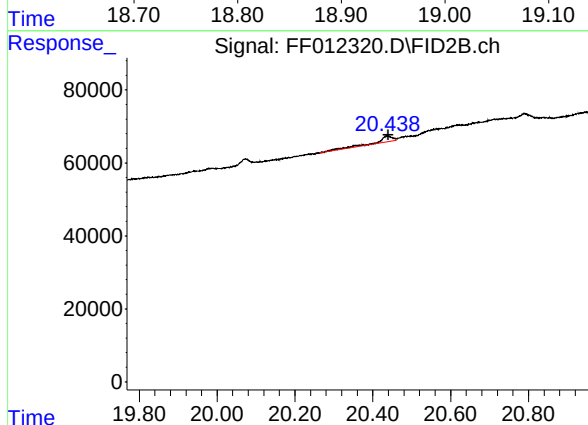

#16 N-HEXATRIACONTANE

R.T.: 20.438 min
Delta R.T.: -0.002 min
Response: 45060
Conc: 0.51 ug/ml