

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
Data File : FF012308.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2023 11:34
Operator : YP\AJ
Sample : 01975-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CHAMBER-B-72-WEST

Integration File: autoint1.e
Quant Time: Mar 21 03:32:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.028	1764058	15.763 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
Data File : FF012308.D
Signal(s) : FID2B.ch
Acq On : 20 Mar 2023 11:34
Operator : YP\AJ
Sample : 01975-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CHAMBER-B-72-WEST

Integration File: autoint1.e
Quant Time: Mar 21 03:32:24 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

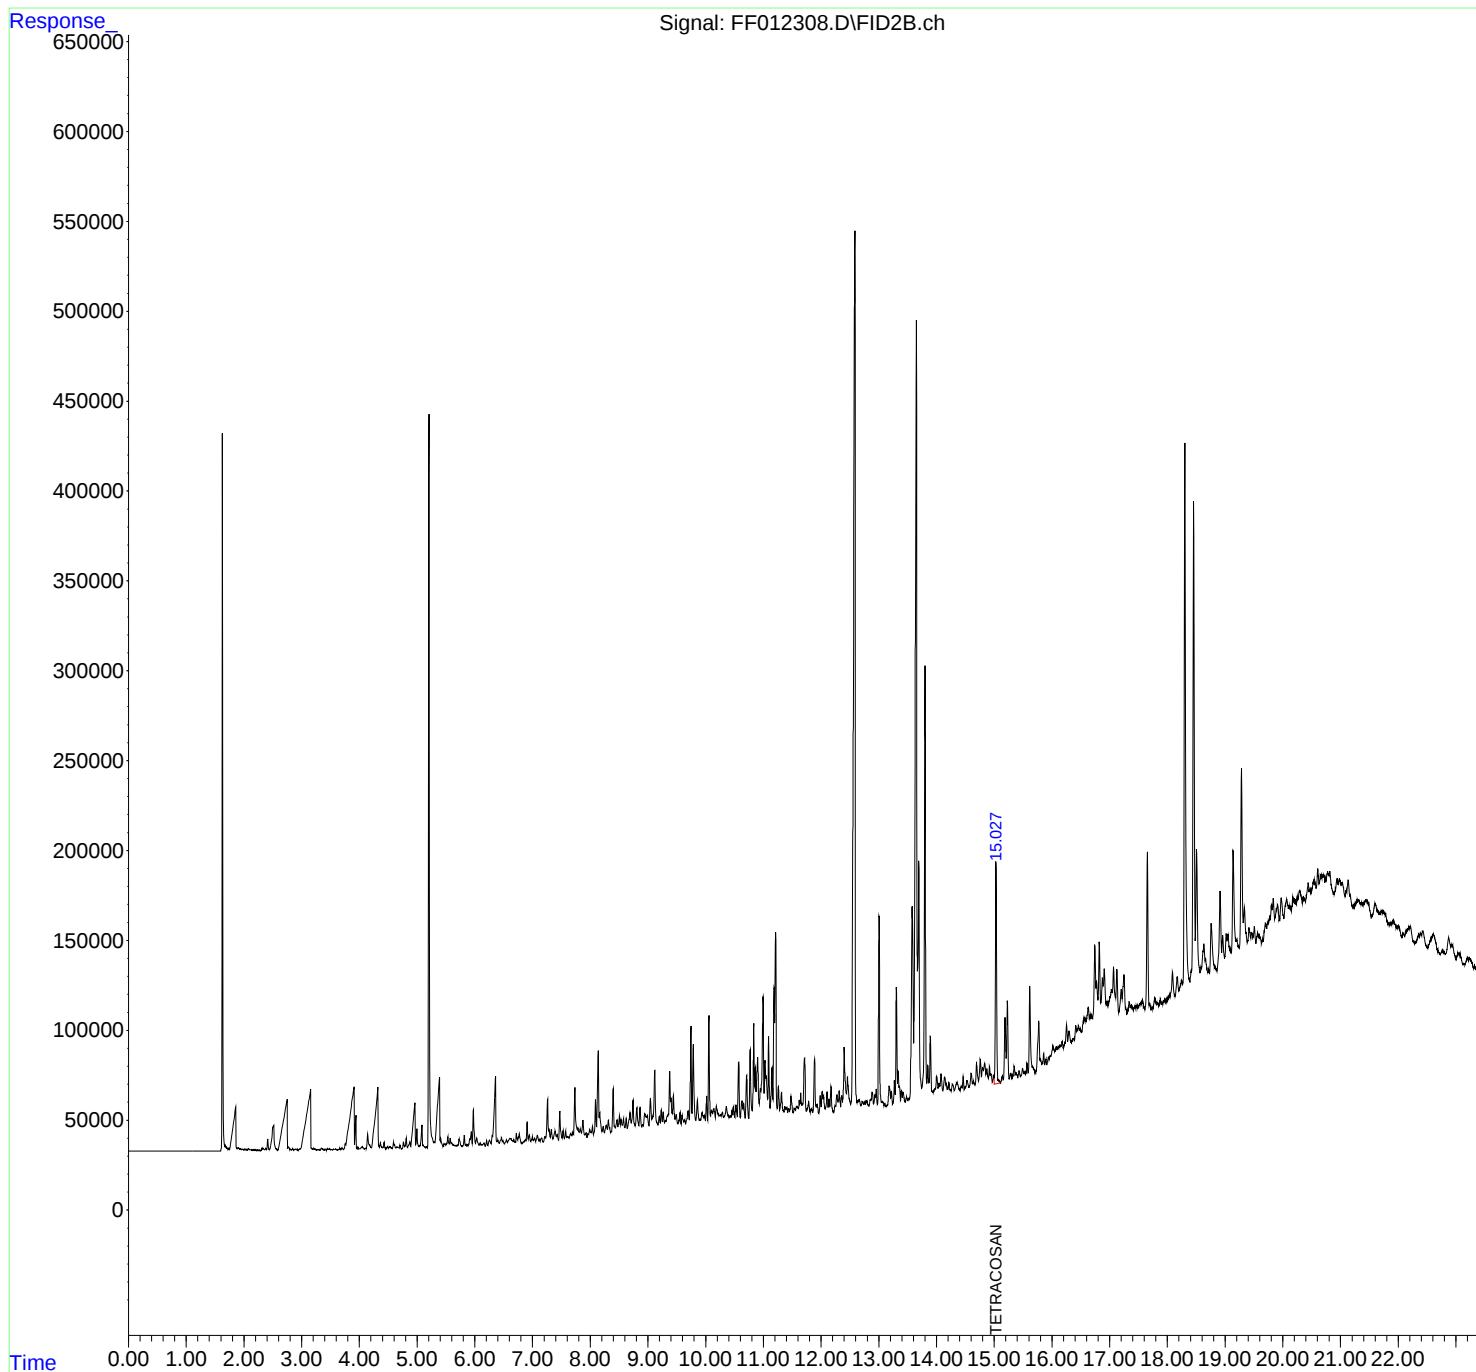

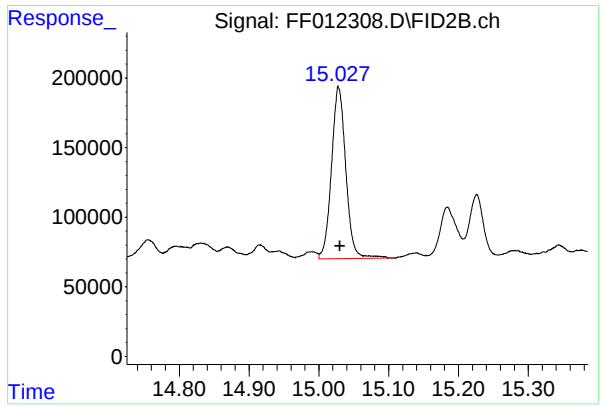

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.028 min
Delta R.T.: -0.002 min
Response: 1764058
Conc: 15.76 ug/ml

Instrument :
FID_F
ClientSampleId :
CHAMBER-B-72-WEST