

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032023\  
 Data File : FF012319.D  
 Signal(s) : FID2B.ch  
 Acq On : 20 Mar 2023 18:07  
 Operator : YP\AJ  
 Sample : 01998-03 5X  
 Misc :  
 ALS Vial : 72 Sample Multiplier: 1

**Instrument :**  
 FID\_F  
**ClientSampleId :**  
 BRAOD-CHANNEL-SUBSTATION-TP2

**Manual Integrations**  
**APPROVED**

Reviewed By :Yogesh Patel 03/21/2023  
 Supervised By :Ankita Jodhani 03/21/2023

Integration File: autoint1.e  
 Quant Time: Mar 21 03:33:34 2023  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031623.M  
 Quant Title :  
 QLast Update : Wed Mar 15 18:07:23 2023  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1uL  
 Signal Phase : Rxi-1ms  
 Signal Info : 20mx0.18mmx0.18um

| Compound                      | R.T.   | Response | Conc Units   |
|-------------------------------|--------|----------|--------------|
| -----                         |        |          |              |
| System Monitoring Compounds   |        |          |              |
| 9) S TETRACOSANE-d50 (SURR... | 15.025 | 449844   | 4.020 ug/mlm |
| Target Compounds              |        |          |              |
| -----                         |        |          |              |

(f)=RT Delta > 1/2 Window

(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032023\  
Data File : FF012319.D  
Signal(s) : FID2B.ch  
Acq On : 20 Mar 2023 18:07  
Operator : YP\AJ  
Sample : 01998-03 5X  
Misc :  
ALS Vial : 72 Sample Multiplier: 1

**Instrument :**

FID\_F

**ClientSampleId :**

BRAOD-CHANNEL-SUBSTATION-TP2


**Manual Integrations****APPROVED**


Reviewed By :Yogesh Patel 03/21/2023

Supervised By :Ankita Jodhani 03/21/2023

Integration File: autoint1.e  
Quant Time: Mar 21 03:33:34 2023  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031623.M  
Quant Title :  
QLast Update : Wed Mar 15 18:07:23 2023  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

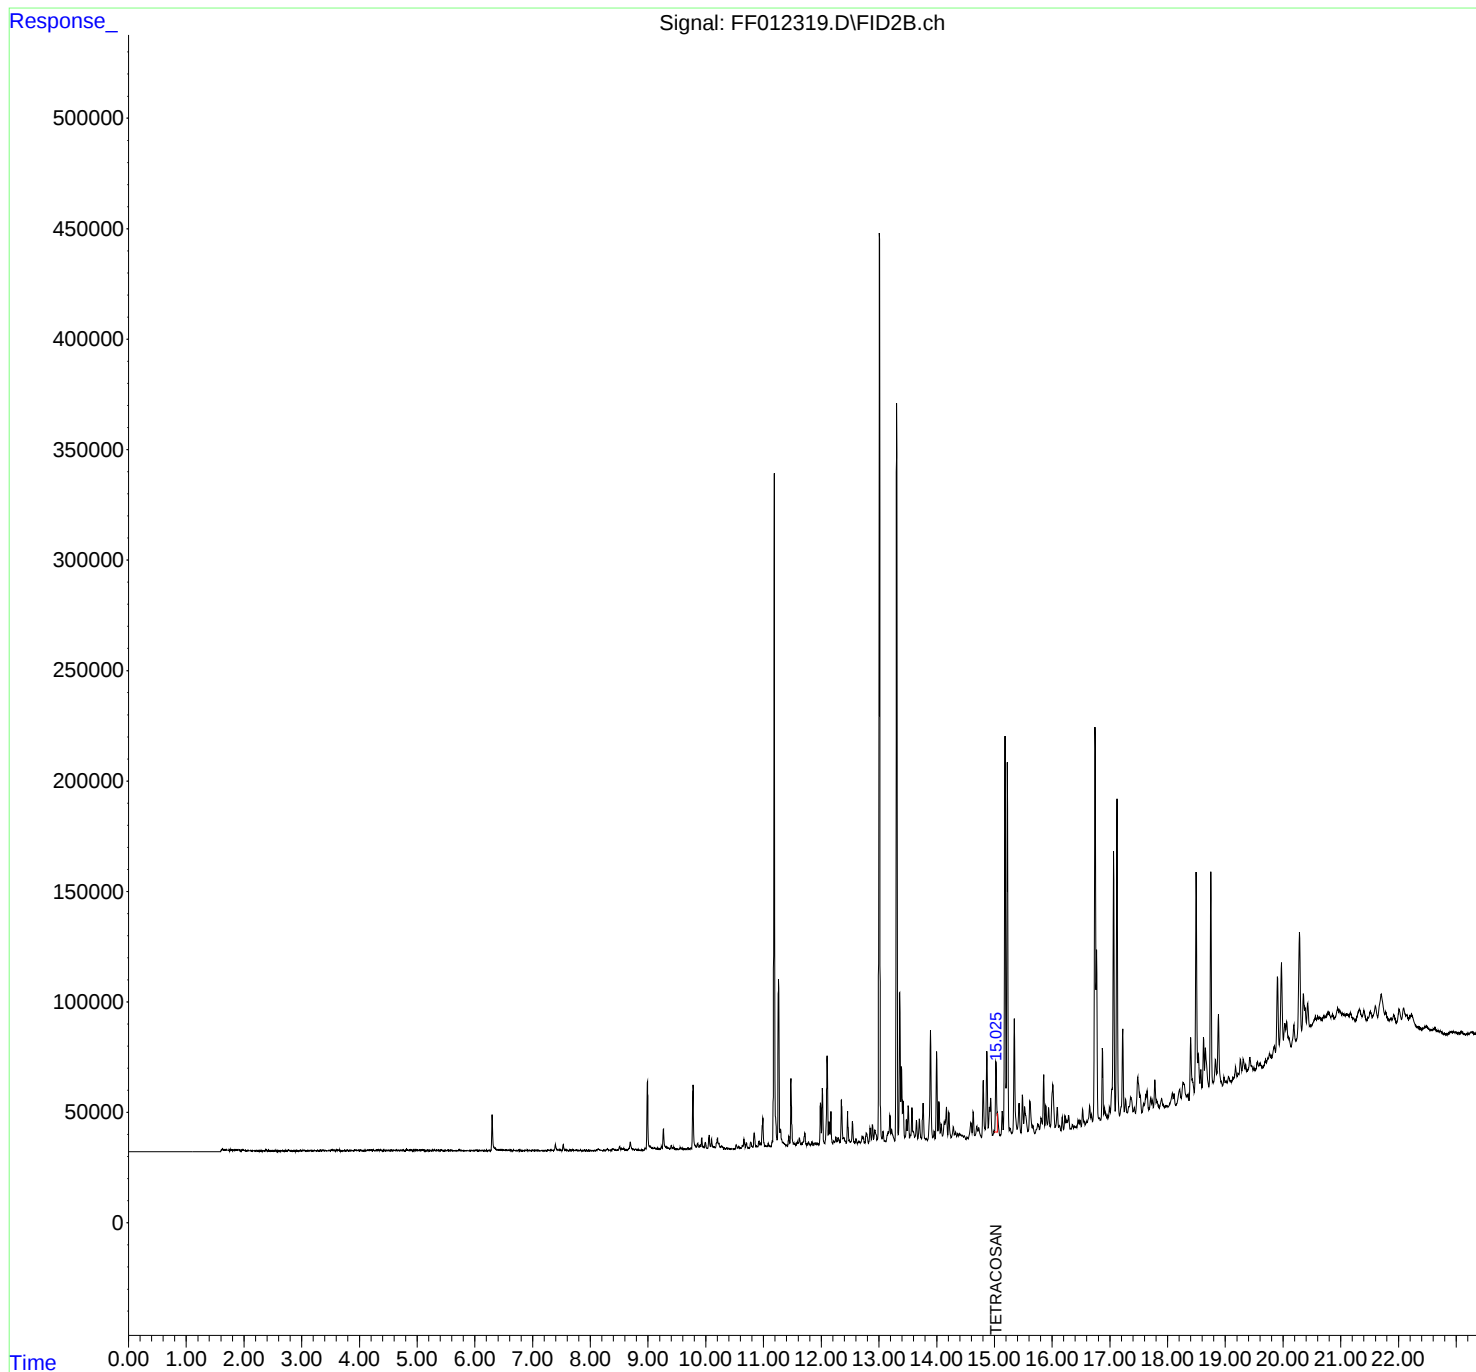

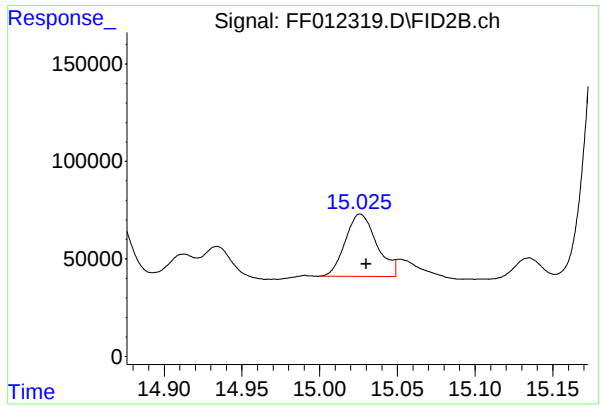

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.025 min  
Delta R.T.: -0.005 min  
Response: 449844  
Conc: 4.02 ug/ml

Instrument : FID\_F  
ClientSampleId :  
BRAOD-CHANNEL-SUBSTATION-TP2

Manual Integrations  
APPROVED

Reviewed By :Yogesh Patel 03/21/2023  
Supervised By :Ankita Jodhani 03/21/2023