

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
 Data File : FF012327.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2023 01:03
 Operator : YP\AJ
 Sample : 50 PPM TRPH STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 50 PPM TRPH STD

Integration File: autoint1.e
 Quant Time: Mar 21 03:34:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.026	4509221	40.292 ug/ml
Target Compounds			
2) N-DECANE	4.592	5387150	43.028 ug/ml
3) N-DODECANE	6.754	5437587	43.863 ug/ml
4) N-TETRADECANE	8.579	5467603	41.959 ug/ml
5) N-HEXADECANE	10.184	5523000	41.389 ug/ml
6) N-OCTADECANE	11.624	5486381	40.844 ug/ml
7) N-EICOSANE	12.933	5406348	40.641 ug/ml
8) N-DOCOSANE	14.128	5171644	40.698 ug/ml
10) N-TETRACOSANE	15.230	5130448	41.139 ug/ml
11) N-HEXACOSANE	16.250	4964935	41.464 ug/ml
12) N-OCTACOSANE	17.198	4863015	42.276 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032023\
Data File : FF012327.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2023 01:03
Operator : YP\AJ
Sample : 50 PPM TRPH STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

Integration File: autoint1.e
Quant Time: Mar 21 03:34:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

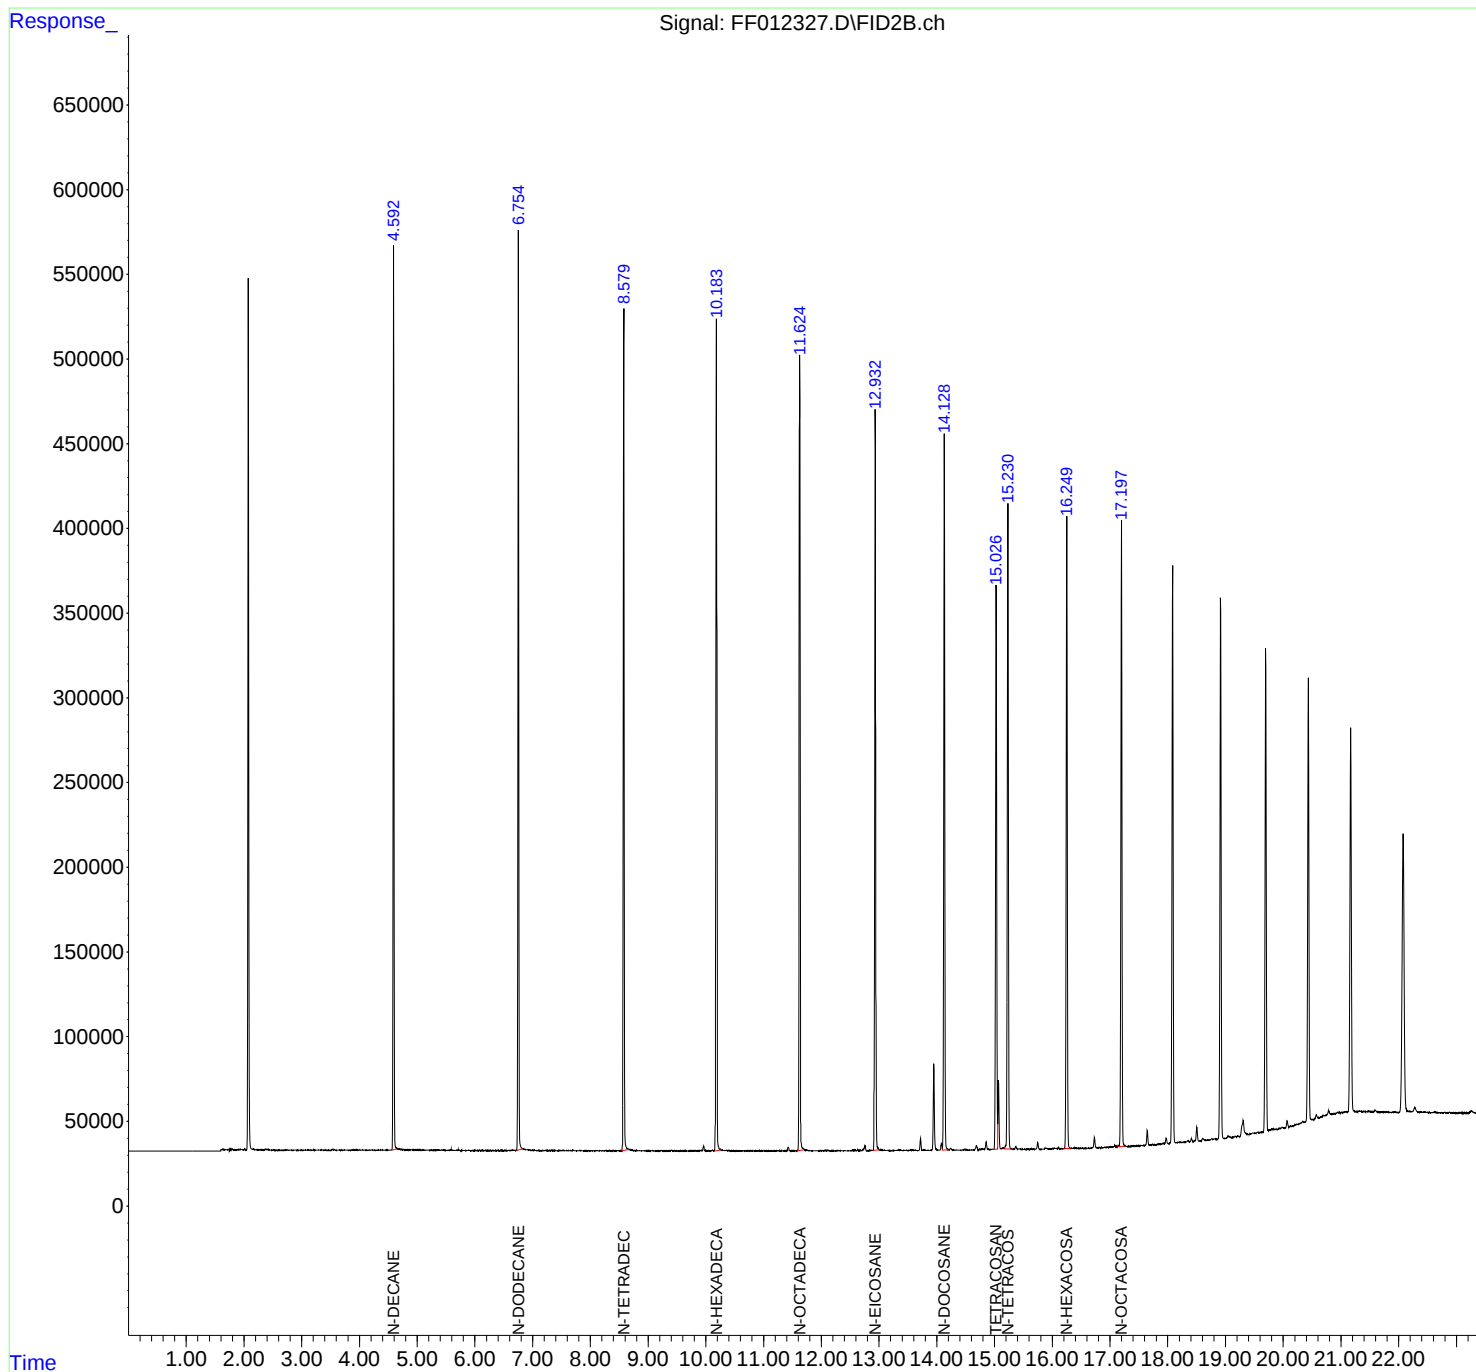


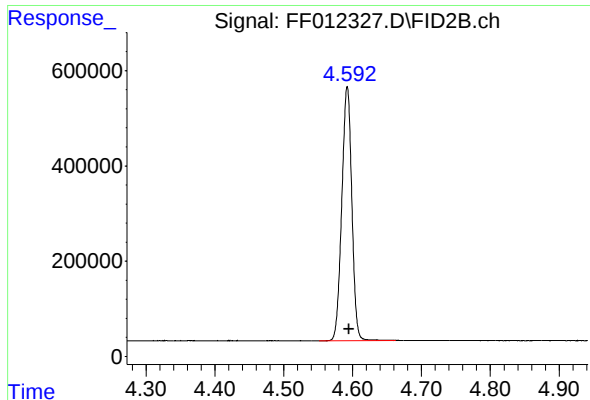

#2 N-DECANE


R.T.: 4.592 min
Delta R.T.: -0.002 min
Response: 5387150
Conc: 43.03 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

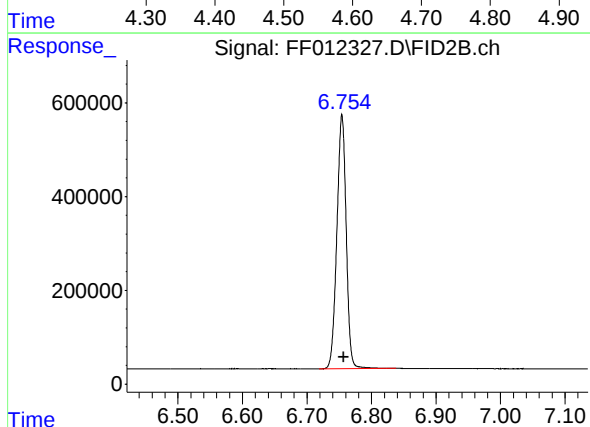


#3 N-DODECANE

R.T.: 6.754 min
Delta R.T.: -0.003 min
Response: 5437587
Conc: 43.86 ug/ml

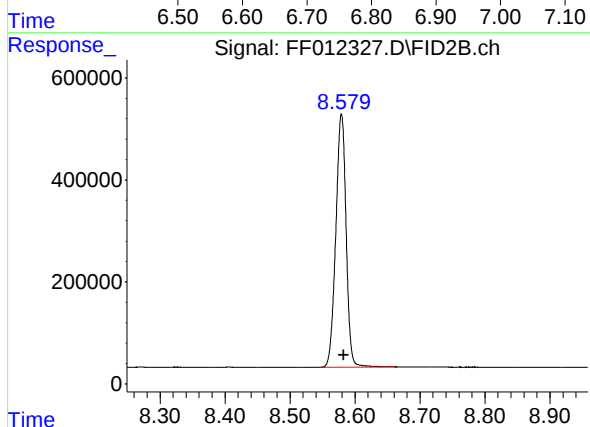


#4 N-TETRADECANE

R.T.: 8.579 min
Delta R.T.: -0.003 min
Response: 5467603
Conc: 41.96 ug/ml

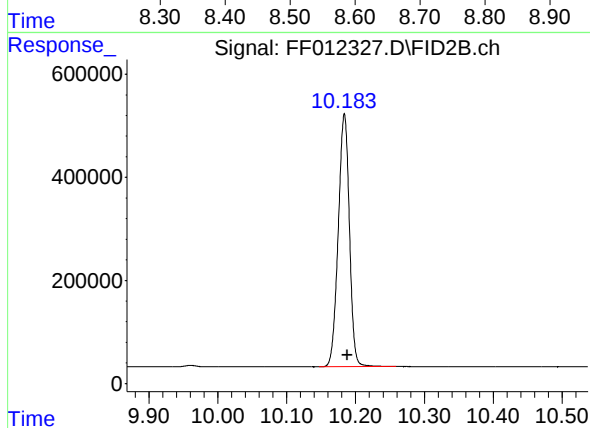

#5 N-HEXADECANE


R.T.: 10.184 min
Delta R.T.: -0.004 min
Response: 5523000
Conc: 41.39 ug/ml

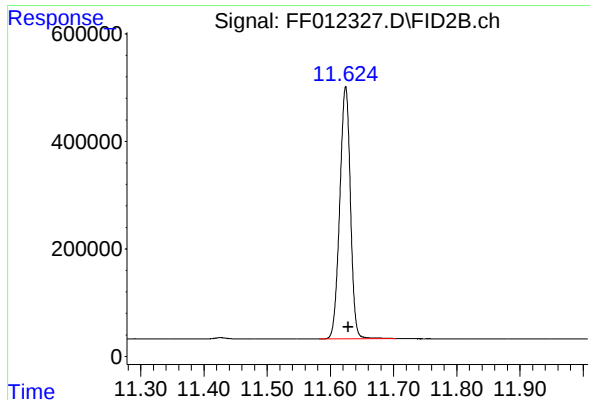

#6 N-OCTADECANE


R.T.: 11.624 min
Delta R.T.: -0.004 min
Response: 5486381
Conc: 40.84 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

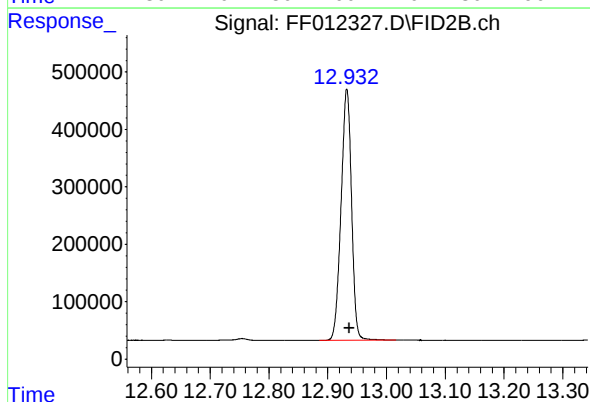


#7 N-EICOSANE

R.T.: 12.933 min
Delta R.T.: -0.005 min
Response: 5406348
Conc: 40.64 ug/ml

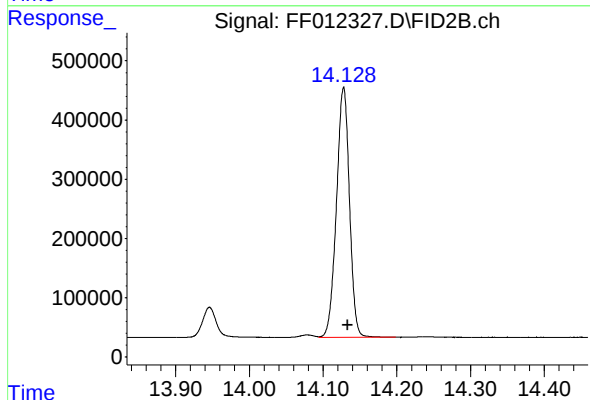


#8 N-DOCOSANE

R.T.: 14.128 min
Delta R.T.: -0.005 min
Response: 5171644
Conc: 40.70 ug/ml

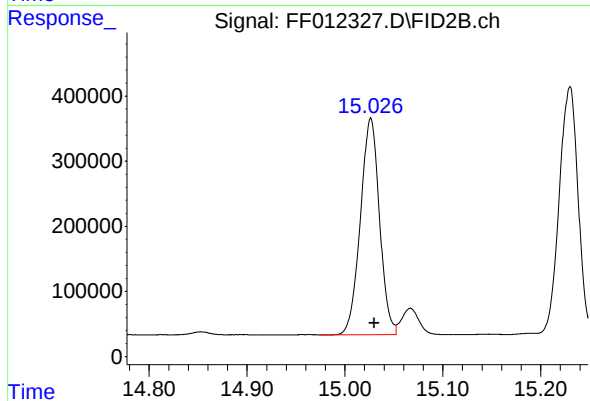

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 15.026 min
Delta R.T.: -0.004 min
Response: 4509221
Conc: 40.29 ug/ml

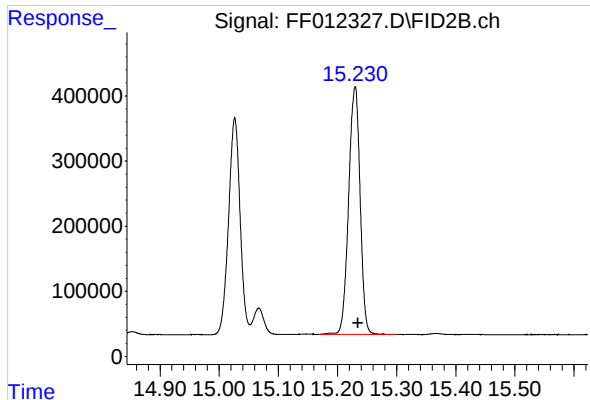

#10 N-TETRACOSANE


R.T.: 15.230 min
Delta R.T.: -0.005 min
Response: 5130448
Conc: 41.14 ug/ml

Instrument :
FID_F
ClientSampleId :
50 PPM TRPH STD

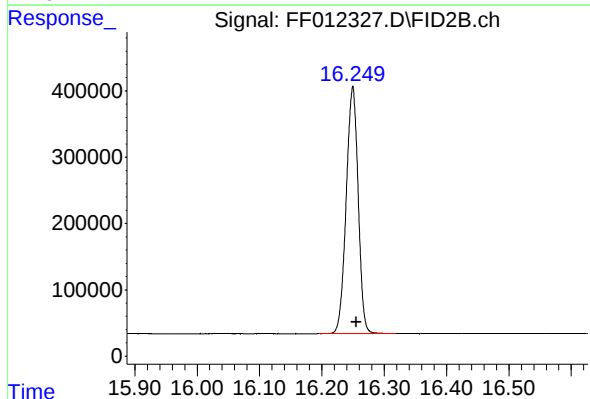

#11 N-HEXACOSANE

R.T.: 16.250 min
Delta R.T.: -0.006 min
Response: 4964935
Conc: 41.46 ug/ml

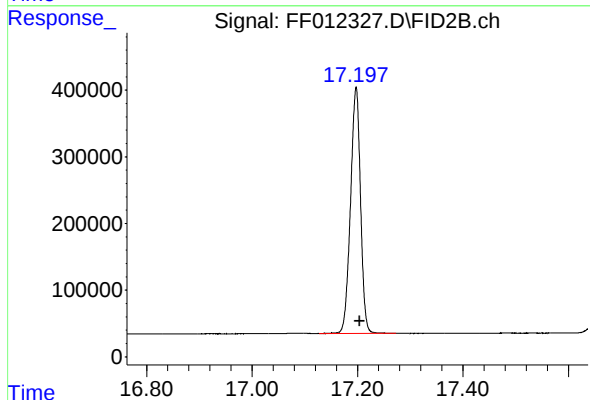

#12 N-OCTACOSANE

R.T.: 17.198 min
Delta R.T.: -0.007 min
Response: 4863015
Conc: 42.28 ug/ml