

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032119\  
Data File : FF003924.D  
Signal(s) : FID2B.ch  
Acq On : 21 Mar 2019 10:19  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
MECL2

Integration File: autoint1.e  
Quant Time: Mar 22 00:51:04 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 14) N-DOTRIACONTANE         | 18.497 | 164645   | 1.158 ug/ml |
| 16) N-HEXATRIACONTANE       | 20.054 | 469144   | 3.595 ug/ml |
| 18) N-TETRACONTANE          | 21.654 | 655697   | 5.271 ug/ml |
| -----                       |        |          |             |

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032119\  
Data File : FF003924.D  
Signal(s) : FID2B.ch  
Acq On : 21 Mar 2019 10:19  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Instrument :  
FID\_F  
ClientSampleId :  
MECL2

Integration File: autoint1.e  
Quant Time: Mar 22 00:51:04 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

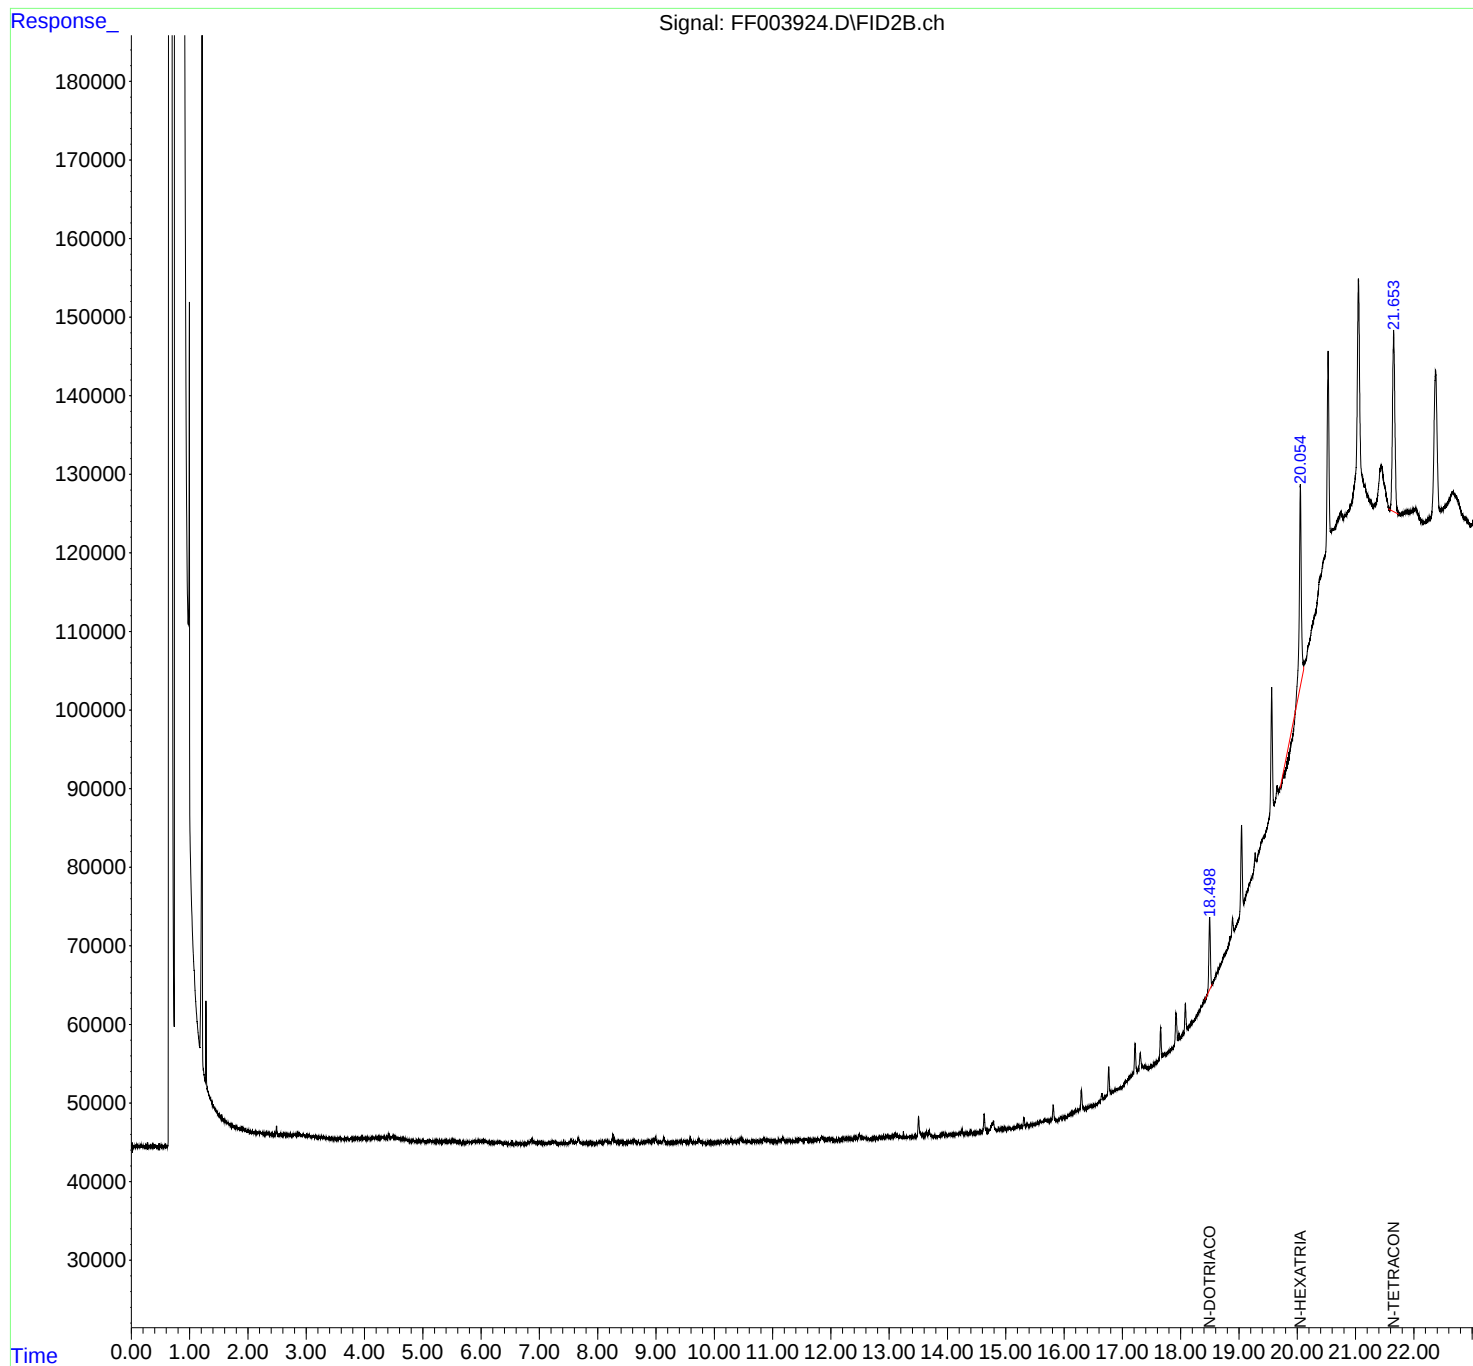


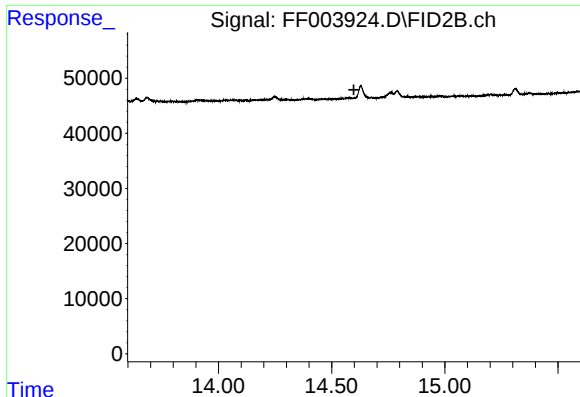

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min  
Exp R.T.: 14.598 min  
Response: 0  
Conc: N.D.

Instrument :  
FID\_F  
ClientSampleId :  
MECL2

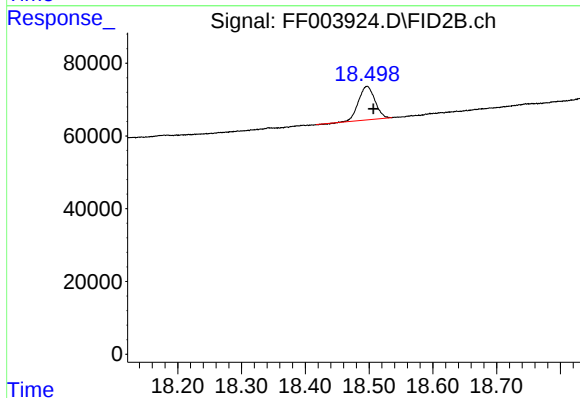


#14 N-DOTRIACONTANE

R.T.: 18.497 min  
Delta R.T.: -0.010 min  
Response: 164645  
Conc: 1.16 ug/ml

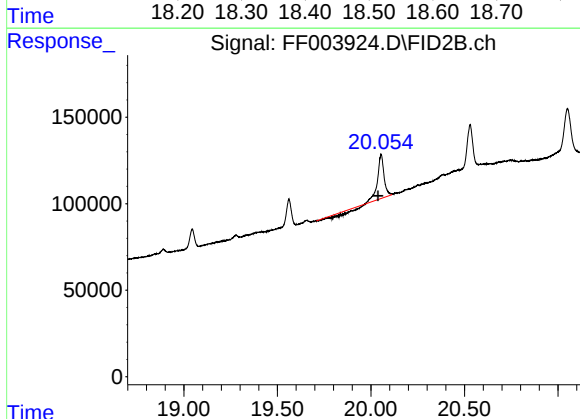

#16 N-HEXATRIACONTANE

R.T.: 20.054 min  
Delta R.T.: 0.016 min  
Response: 469144  
Conc: 3.60 ug/ml

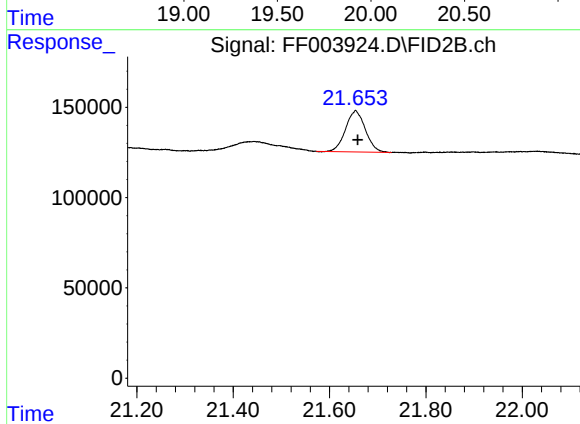

#18 N-TETRACONTANE

R.T.: 21.654 min  
Delta R.T.: -0.005 min  
Response: 655697  
Conc: 5.27 ug/ml