

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003925.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 10:49
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 00:51:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.586	2174937	15.621 ug/ml
Target Compounds			
15) N-TETRATRIACONTANE	19.275	63126	0.471 ug/ml
16) N-HEXATRIACONTANE	20.054	404362	3.099 ug/ml
18) N-TETRACONTANE	21.655	240601	1.934 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003925.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 10:49
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 00:51:12 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

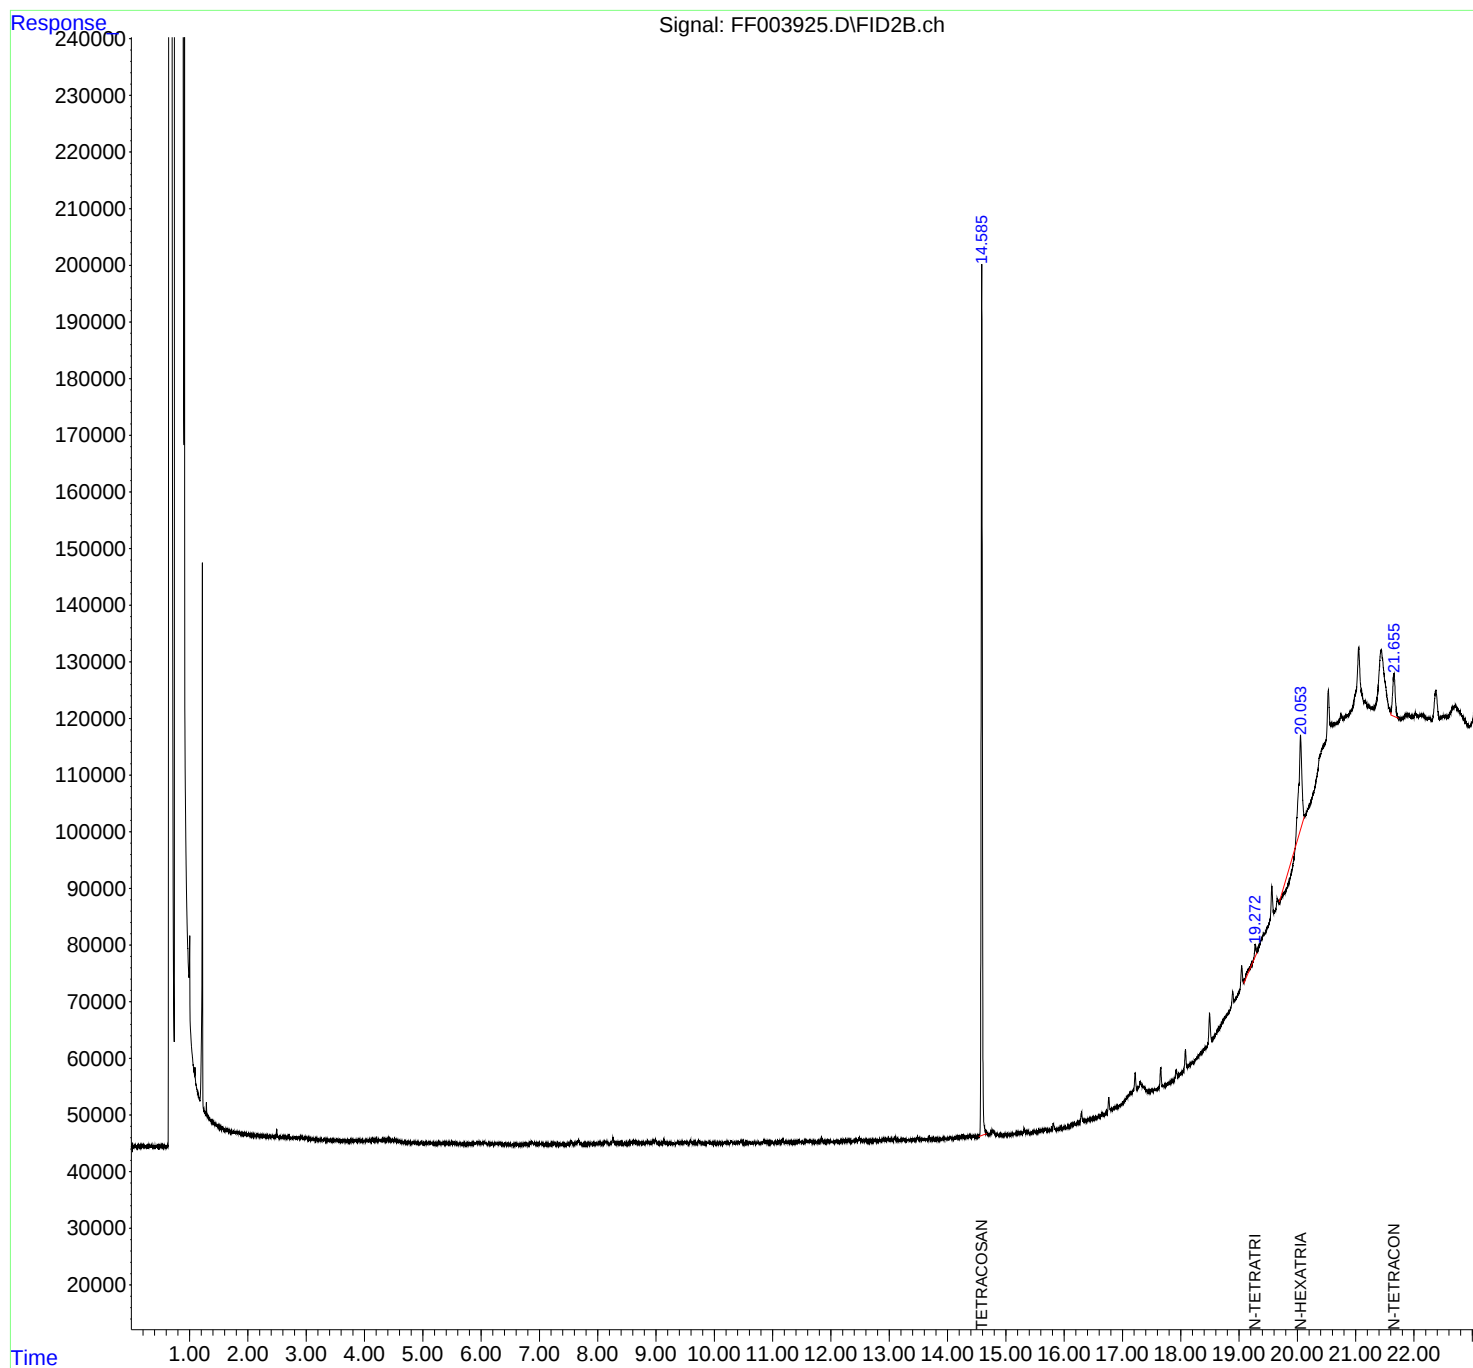


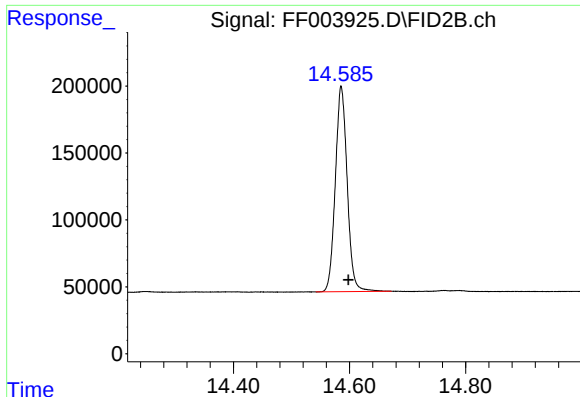

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.586 min
Delta R.T.: -0.013 min
Response: 2174937
Conc: 15.62 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

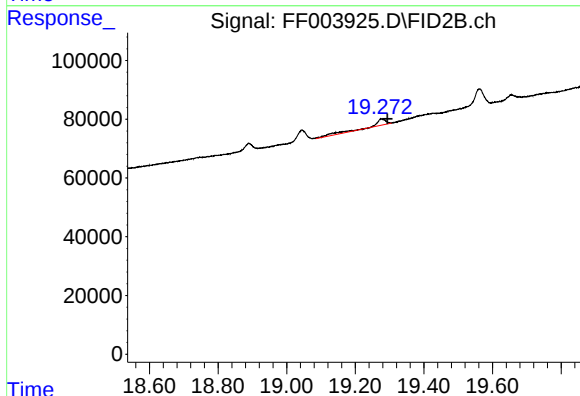


#15 N-TETRATRIACONTANE

R.T.: 19.275 min
Delta R.T.: -0.018 min
Response: 63126
Conc: 0.47 ug/ml

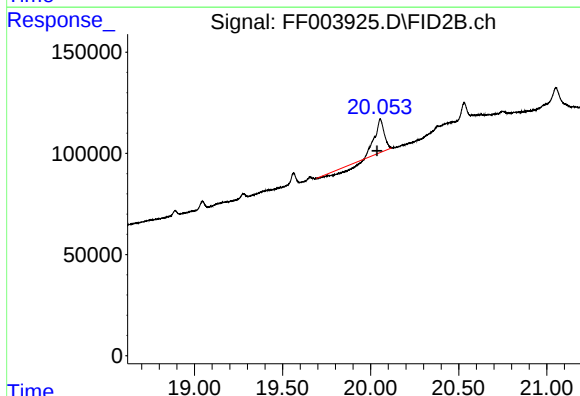

#16 N-HEXATRIACONTANE

R.T.: 20.054 min
Delta R.T.: 0.016 min
Response: 404362
Conc: 3.10 ug/ml

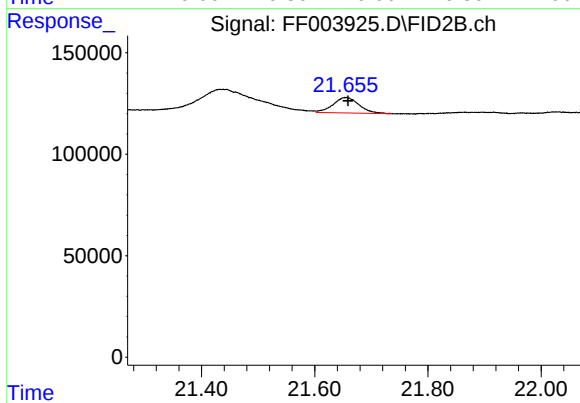

#18 N-TETRACONTANE

R.T.: 21.655 min
Delta R.T.: -0.003 min
Response: 240601
Conc: 1.93 ug/ml