

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
 Data File : FF003928.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2019 13:22
 Operator : AJ\SJ
 Sample : K1994-01 500X
 Misc :
 ALS Vial : 55 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 30200-05

Integration File: autoint1.e
 Quant Time: Mar 22 00:51:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds	R.T.	Response	Conc Units
2) N-DECANE	4.313	978505	6.361 ug/ml
3) N-DODECANE	6.335	2980618	19.099 ug/ml
4) N-TETRADECANE	8.129	3984905	24.854 ug/ml
5) N-HEXADECANE	9.729	3857851	23.687 ug/ml
6) N-OCTADECANE	11.172	2929744	17.782 ug/ml
7) N-EICOSANE	12.482	1443578	8.824 ug/ml
8) N-DOCOSANE	13.683	576947	3.575 ug/ml
10) N-TETRACOSANE	14.789	181929	1.150 ug/ml
14) N-DOTRIACONTANE	18.496	149447	1.051 ug/ml
16) N-HEXATRIACONTANE	20.055	340229	2.607 ug/ml
18) N-TETRACONTANE	21.655	196191	1.577 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003928.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 13:22
Operator : AJ\SJ
Sample : K1994-01 500X
Misc :
ALS Vial : 55 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
30200-05

Integration File: autoint1.e
Quant Time: Mar 22 00:51:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

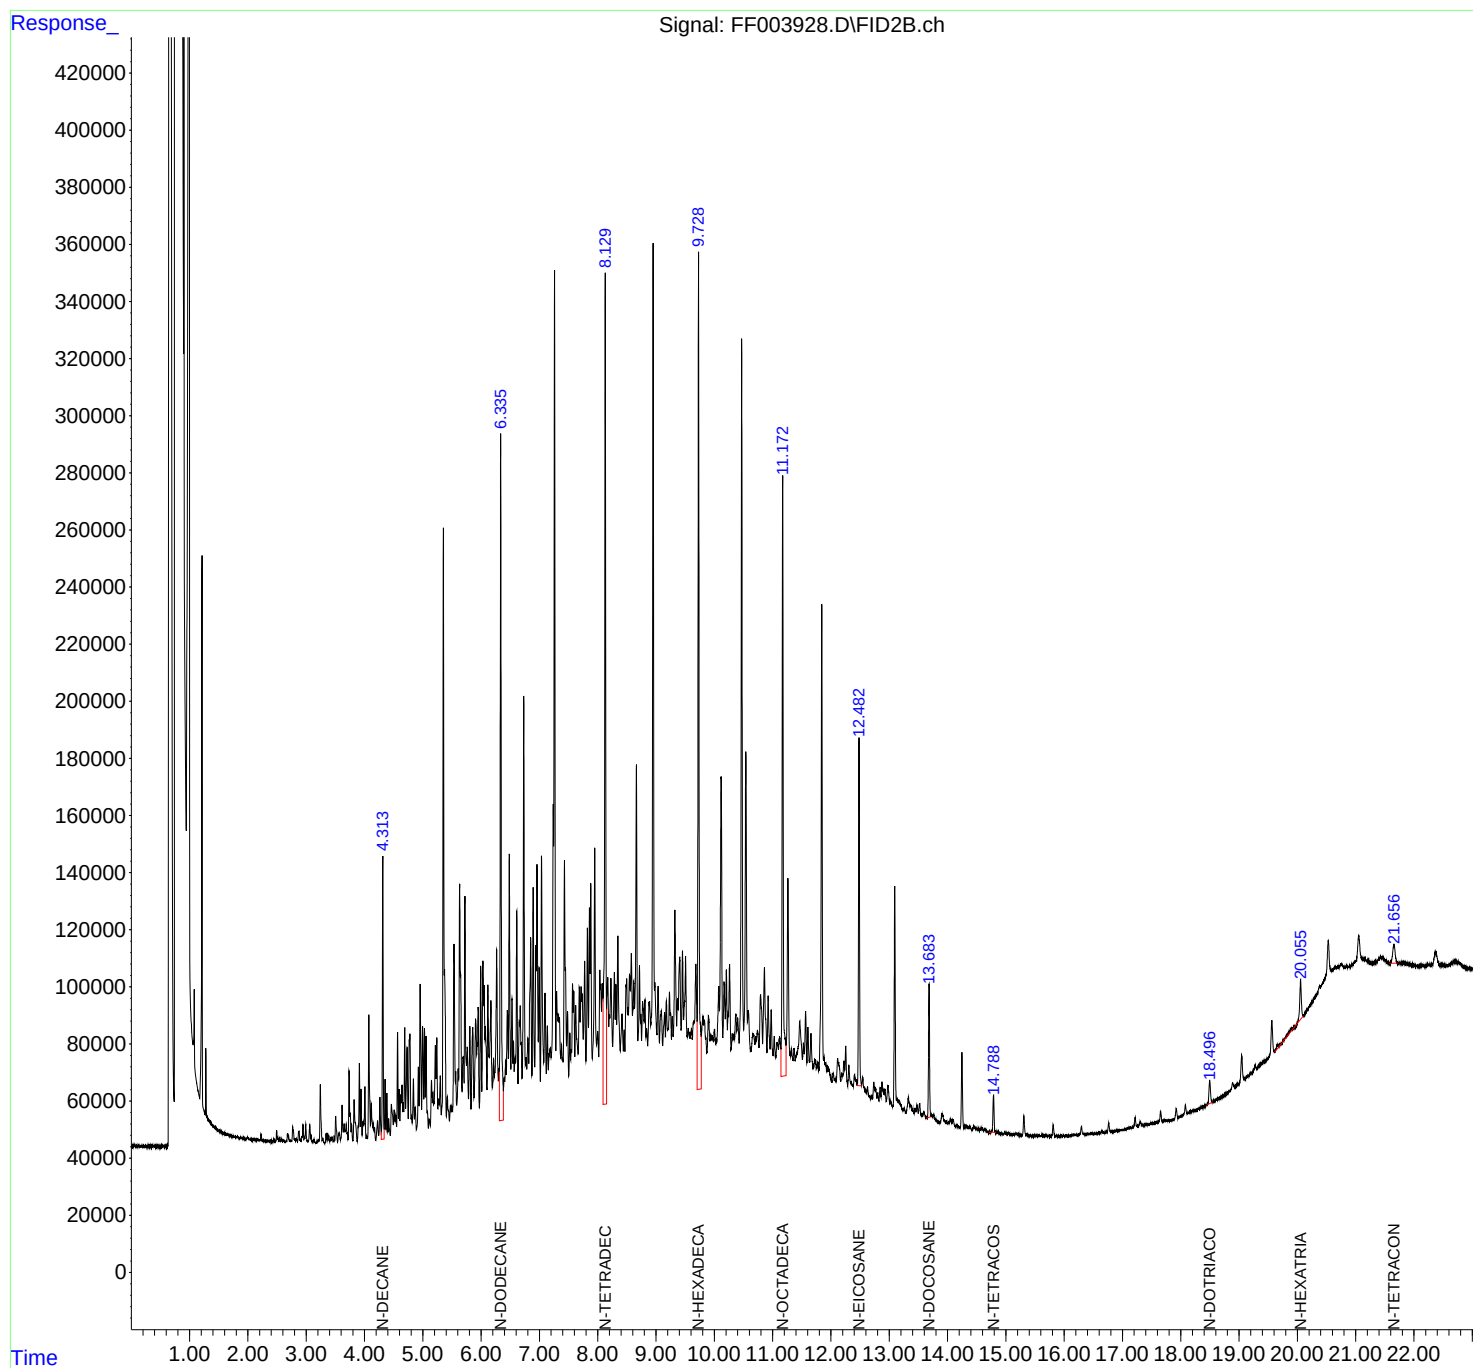


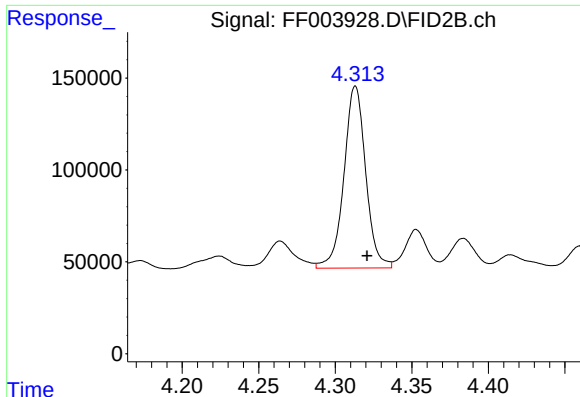

#2 N-DECANE


R.T.: 4.313 min
Delta R.T.: -0.008 min
Response: 978505
Conc: 6.36 ug/ml

Instrument :
FID_F
ClientSampleId :
30200-05

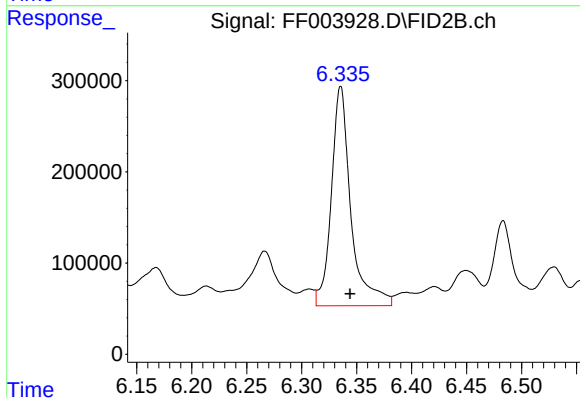


#3 N-DODECANE

R.T.: 6.335 min
Delta R.T.: -0.009 min
Response: 2980618
Conc: 19.10 ug/ml

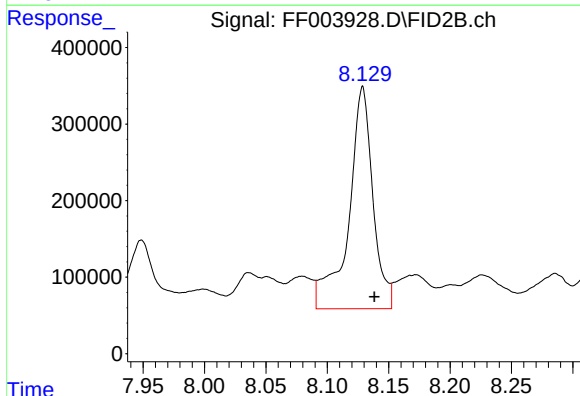


#4 N-TETRADECANE

R.T.: 8.129 min
Delta R.T.: -0.010 min
Response: 3984905
Conc: 24.85 ug/ml

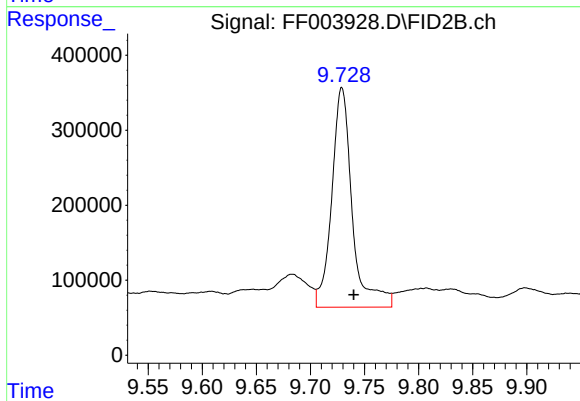

#5 N-HEXADECANE


R.T.: 9.729 min
Delta R.T.: -0.011 min
Response: 3857851
Conc: 23.69 ug/ml

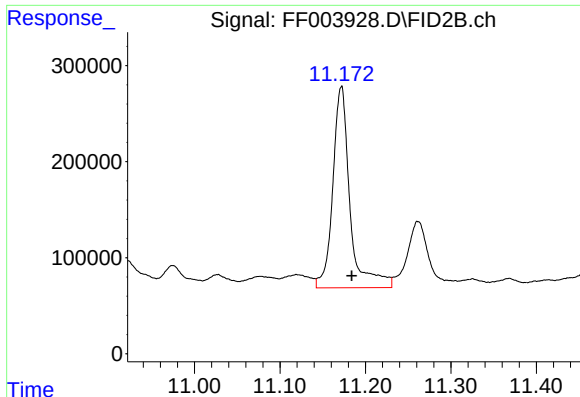

#6 N-OCTADECANE


R.T.: 11.172 min
Delta R.T.: -0.012 min
Response: 2929744
Conc: 17.78 ug/ml

Instrument :
FID_F
ClientSampleId :
30200-05

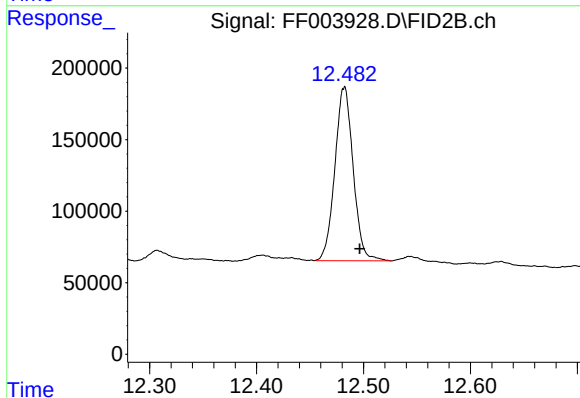


#7 N-EICOSANE

R.T.: 12.482 min
Delta R.T.: -0.014 min
Response: 1443578
Conc: 8.82 ug/ml

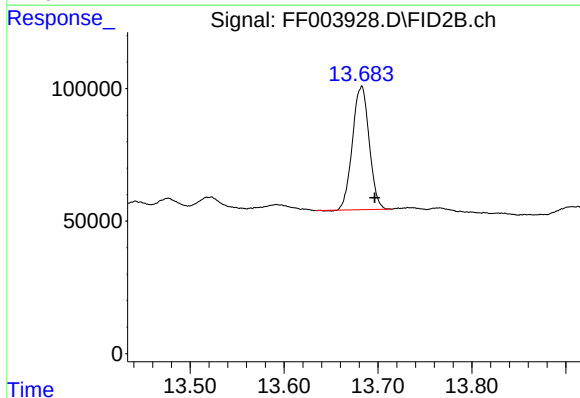


#8 N-DOCOSANE

R.T.: 13.683 min
Delta R.T.: -0.014 min
Response: 576947
Conc: 3.57 ug/ml

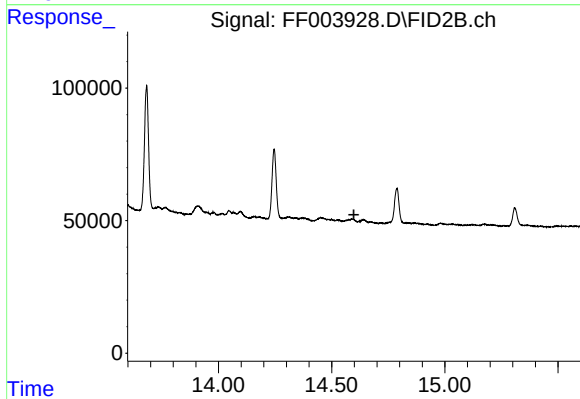

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.598 min
Response: 0
Conc: N.D.

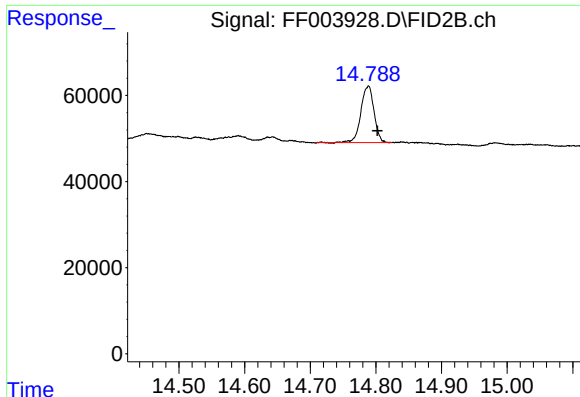

#10 N-TETRACOSANE


R.T.: 14.789 min
Delta R.T.: -0.014 min
Response: 181929
Conc: 1.15 ug/ml

Instrument :
FID_F
ClientSampleId :
30200-05

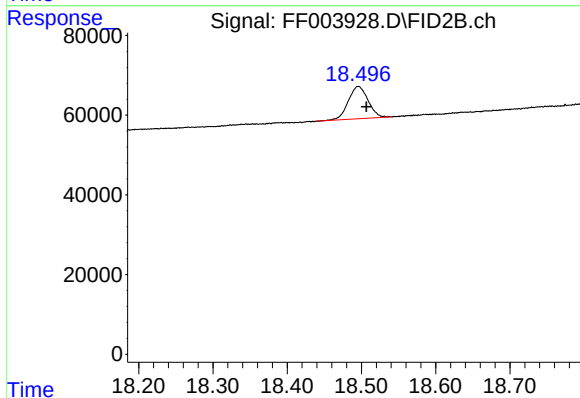


#14 N-DOTRIACONTANE

R.T.: 18.496 min
Delta R.T.: -0.011 min
Response: 149447
Conc: 1.05 ug/ml

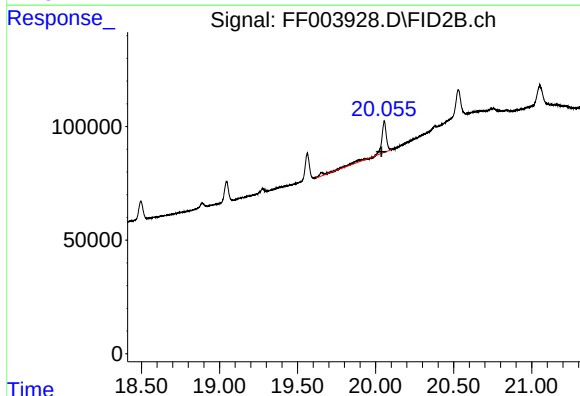

#16 N-HEXATRIACONTANE

R.T.: 20.055 min
Delta R.T.: 0.018 min
Response: 340229
Conc: 2.61 ug/ml

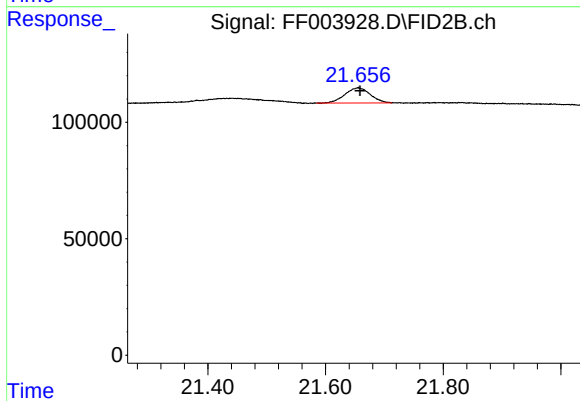

#18 N-TETRACONTANE

R.T.: 21.655 min
Delta R.T.: -0.003 min
Response: 196191
Conc: 1.58 ug/ml