

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003935.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 16:55
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 00:52:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.333	3104243	19.891 ug/ml
12)	N-OCTACOSANE	16.762	2940956	19.462 ug/ml
13)	N-TRIACONTANE	17.651	301558	2.050 ug/ml
14)	N-DOTRIACONTANE	18.485	341470	2.401 ug/ml
15)	N-TETRATRIACONTANE	19.271	225671	1.685 ug/ml
16)	N-HEXATRIACONTANE	20.055	129518	0.993 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003935.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 16:55
Operator : AJ\SJ
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
RT MARKER

Integration File: autoint1.e
Quant Time: Mar 22 00:52:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

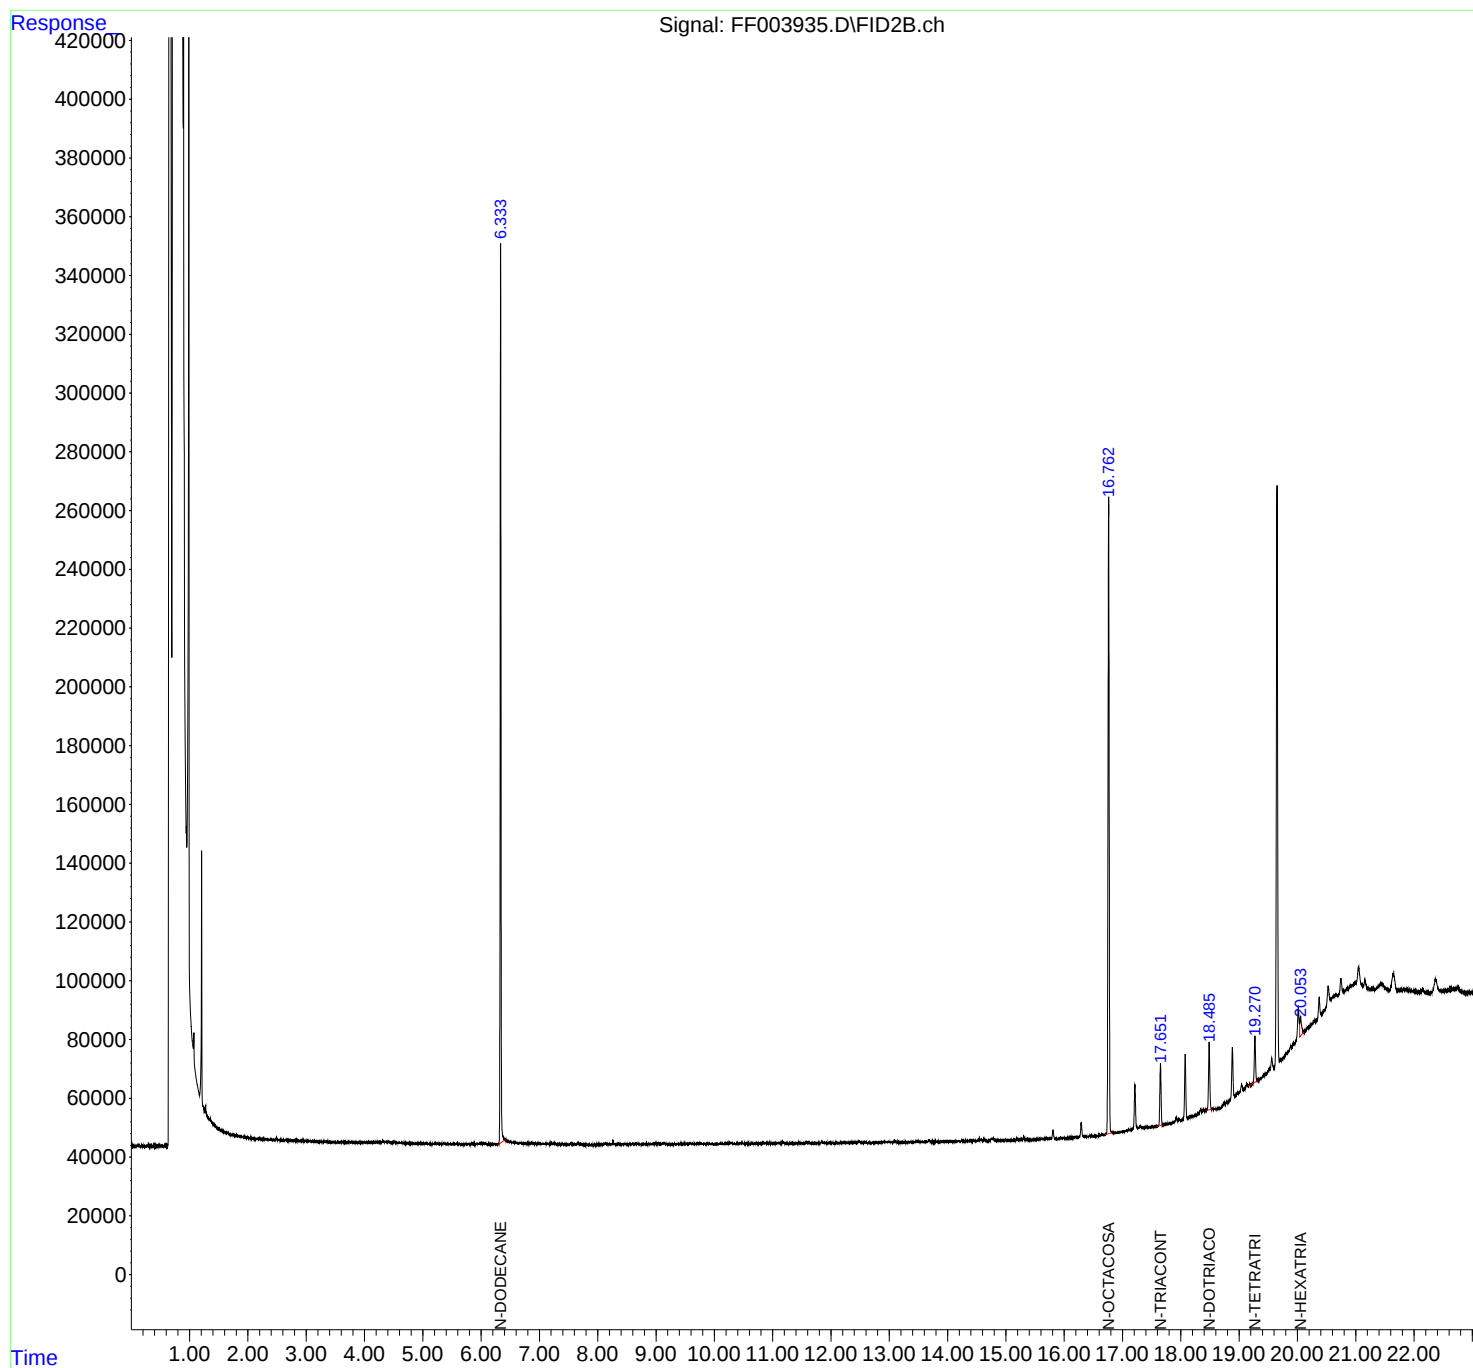


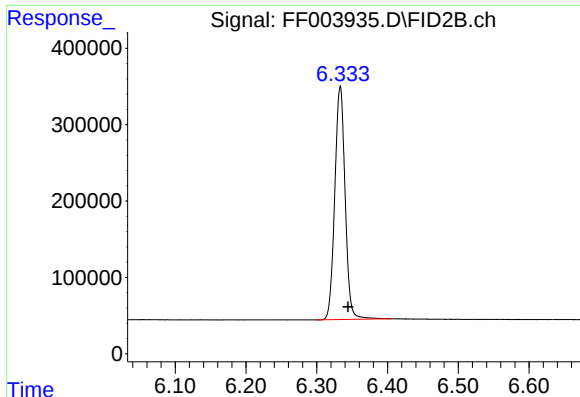

#3 N-DODECANE


R.T.: 6.333 min
Delta R.T.: -0.011 min
Response: 3104243
Conc: 19.89 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

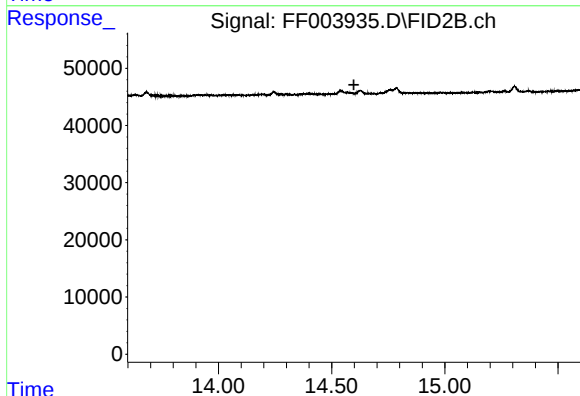


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.598 min
Response: 0
Conc: N.D.

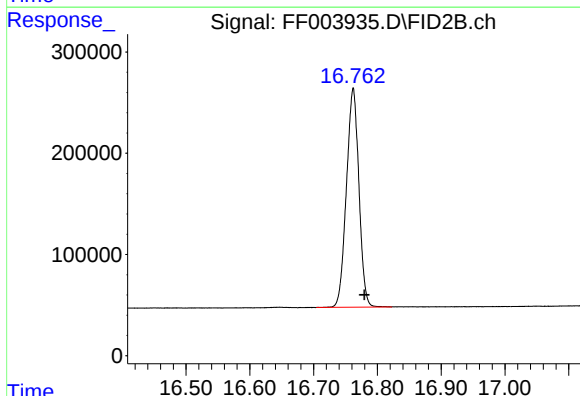


#12 N-OCTACOSANE

R.T.: 16.762 min
Delta R.T.: -0.018 min
Response: 2940956
Conc: 19.46 ug/ml

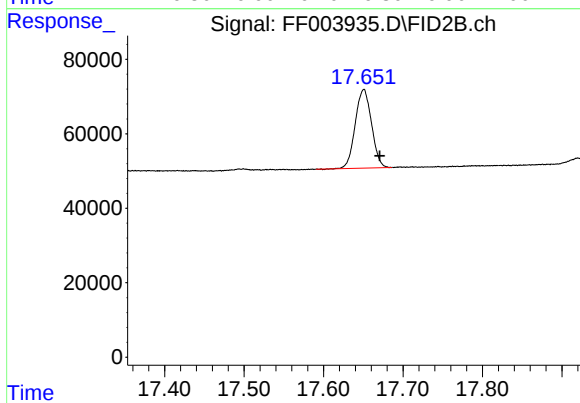

#13 N-TRIACONTANE


R.T.: 17.651 min
Delta R.T.: -0.020 min
Response: 301558
Conc: 2.05 ug/ml

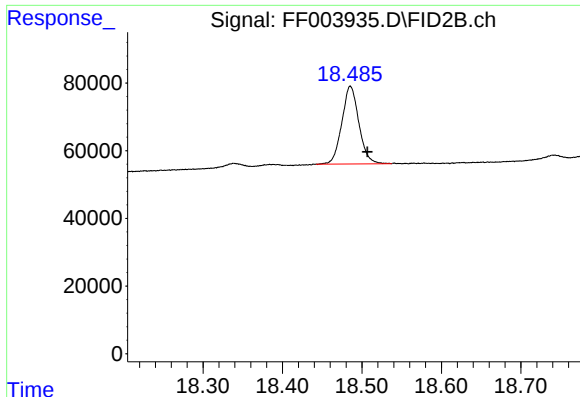

#14 N-DOTRIACONTANE


R.T.: 18.485 min
Delta R.T.: -0.021 min
Response: 341470
Conc: 2.40 ug/ml

Instrument :
FID_F
ClientSampleId :
RT MARKER

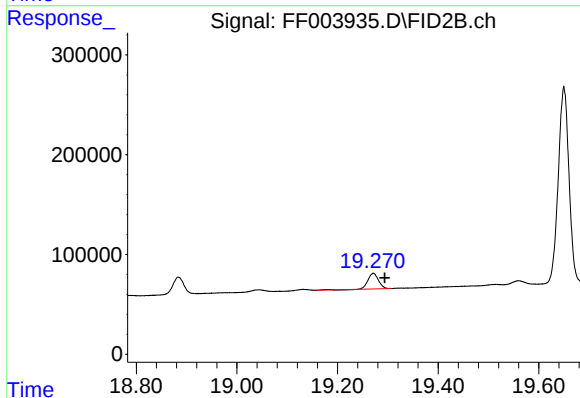

#15 N-TETRATRIACONTANE

R.T.: 19.271 min
Delta R.T.: -0.022 min
Response: 225671
Conc: 1.69 ug/ml

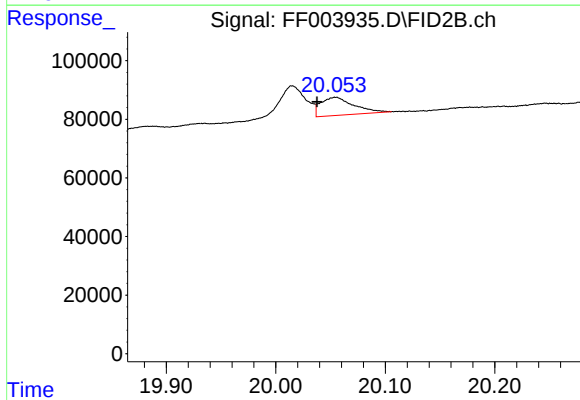

#16 N-HEXATRIACONTANE

R.T.: 20.055 min
Delta R.T.: 0.017 min
Response: 129518
Conc: 0.99 ug/ml