

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
 Data File : FF003940.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2019 19:28
 Operator : AJ\SJ
 Sample : K2037-05
 Misc :
 ALS Vial : 62 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MW-07-20190320

Integration File: autoint1.e
 Quant Time: Mar 22 00:53:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.580	1370689	9.845 ug/ml
Target Compounds			
3) N-DODECANE	6.318	452386	2.899 ug/ml
4) N-TETRADECANE	8.120	103517	0.646 ug/ml
5) N-HEXADECANE	9.750	222718	1.367 ug/ml
6) N-OCTADECANE	11.170	101769	0.618 ug/ml
16) N-HEXATRIACONTANE	20.054	466131	3.572 ug/ml
18) N-TETRACONTANE	21.653	233892	1.880 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003940.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 19:28
Operator : AJ\SJ
Sample : K2037-05
Misc :
ALS Vial : 62 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MW-07-20190320

Integration File: autoint1.e
Quant Time: Mar 22 00:53:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

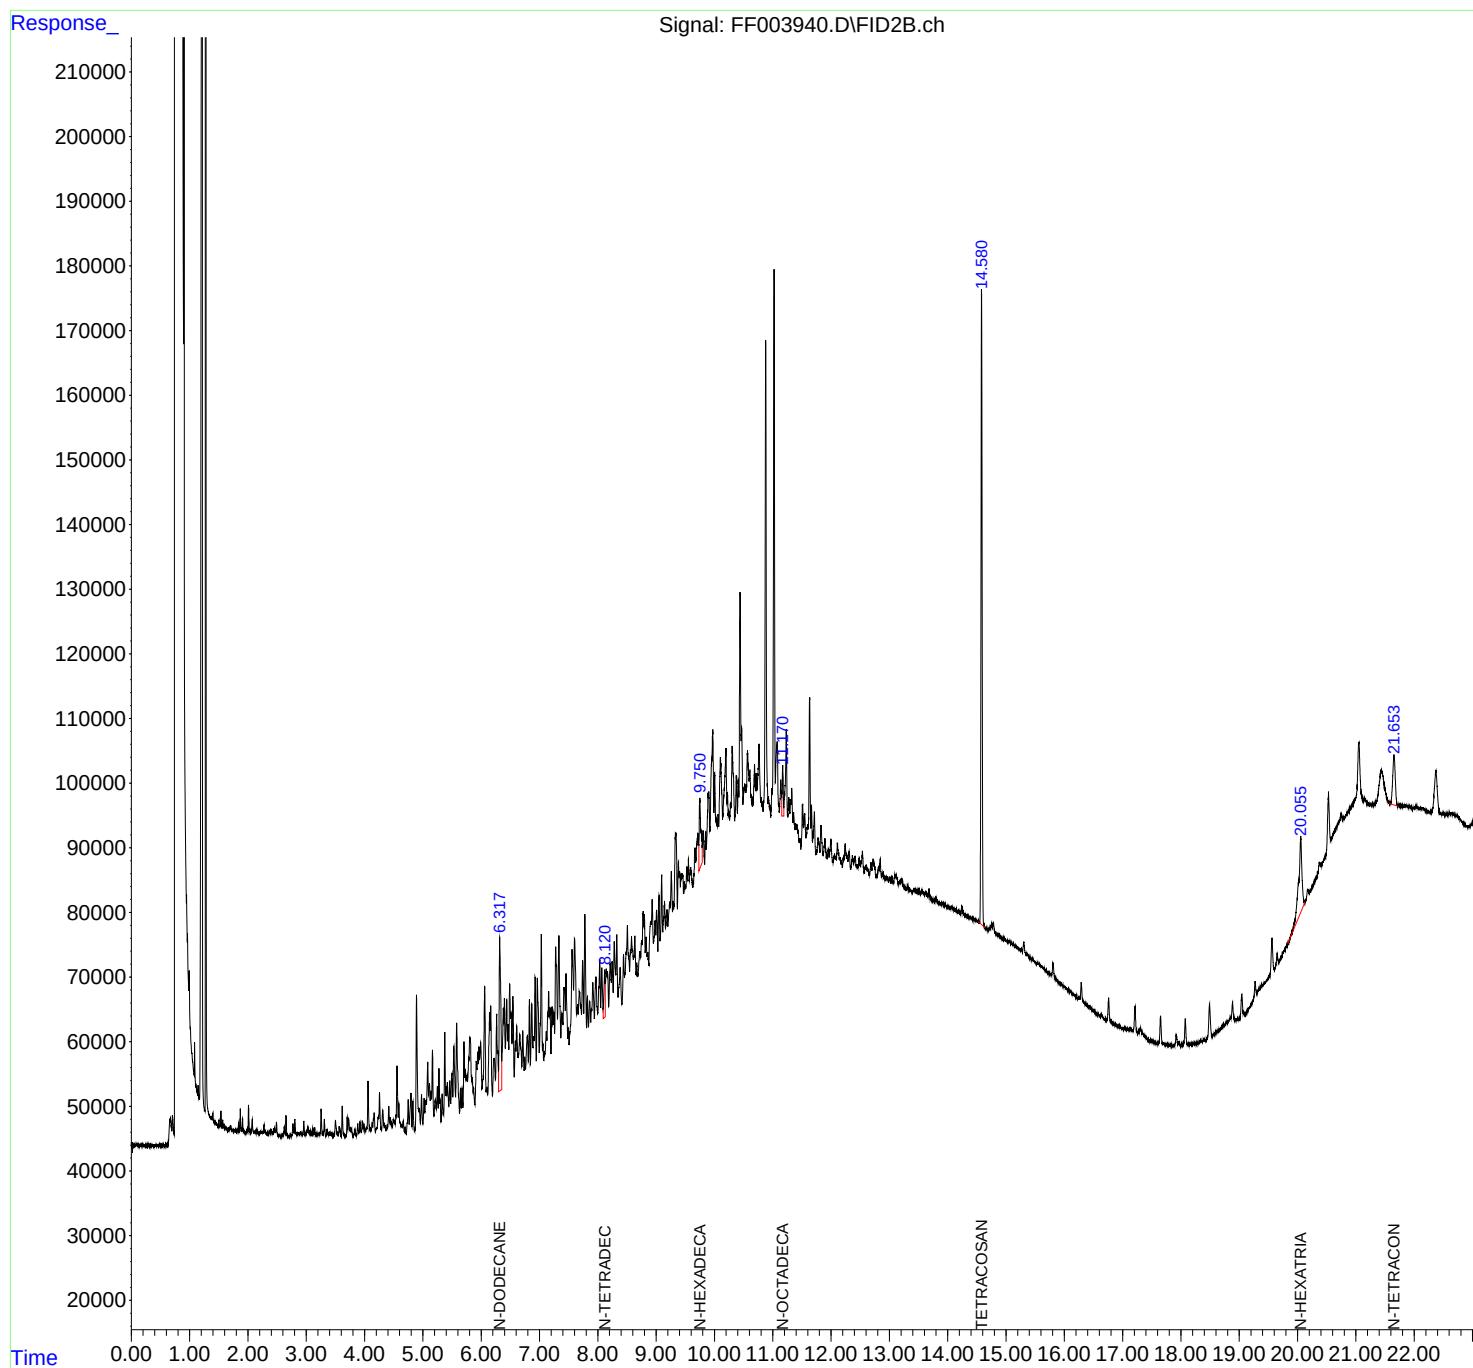


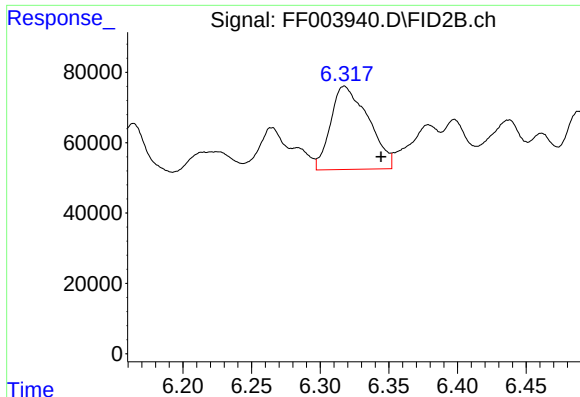

#3 N-DODECANE


R.T.: 6.318 min
Delta R.T.: -0.027 min
Response: 452386
Conc: 2.90 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-07-20190320

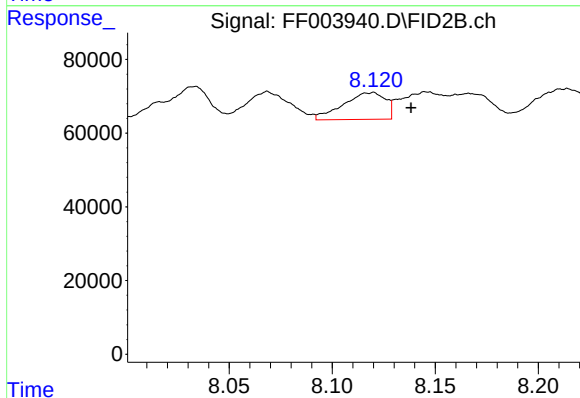


#4 N-TETRADECANE

R.T.: 8.120 min
Delta R.T.: -0.019 min
Response: 103517
Conc: 0.65 ug/ml

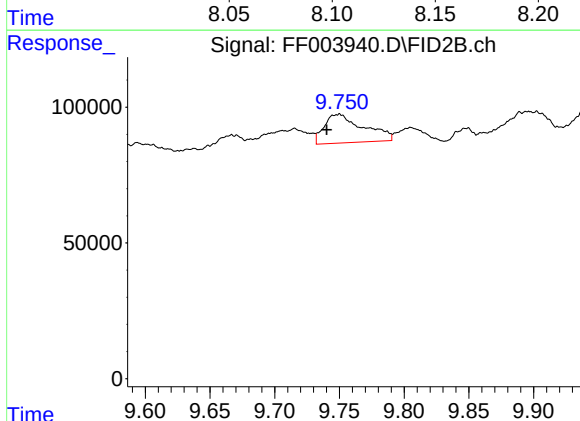


#5 N-HEXADECANE

R.T.: 9.750 min
Delta R.T.: 0.010 min
Response: 222718
Conc: 1.37 ug/ml

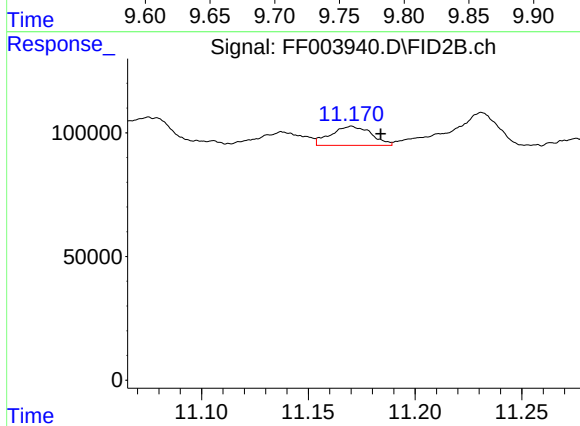

#6 N-OCTADECANE


R.T.: 11.170 min
Delta R.T.: -0.014 min
Response: 101769
Conc: 0.62 ug/ml

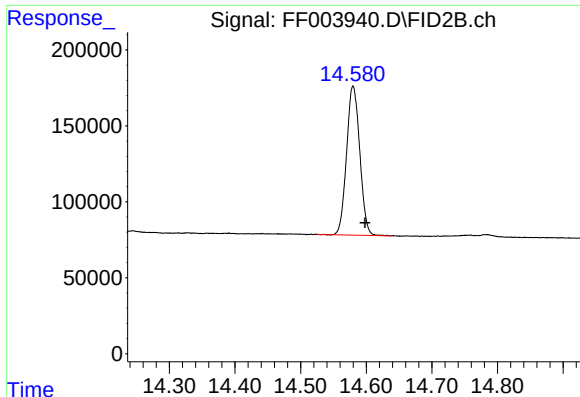

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.580 min
Delta R.T.: -0.018 min
Response: 1370689
Conc: 9.84 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-07-20190320

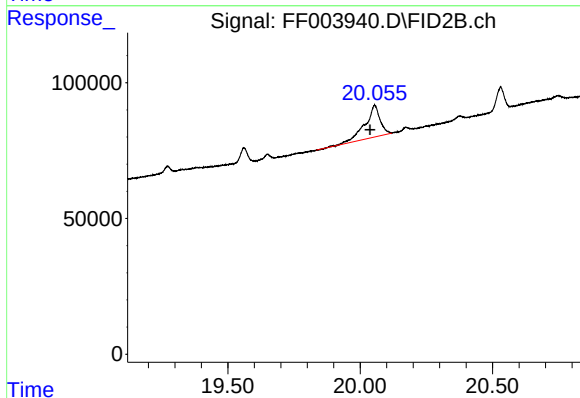

#16 N-HEXATRIACONTANE

R.T.: 20.054 min
Delta R.T.: 0.016 min
Response: 466131
Conc: 3.57 ug/ml

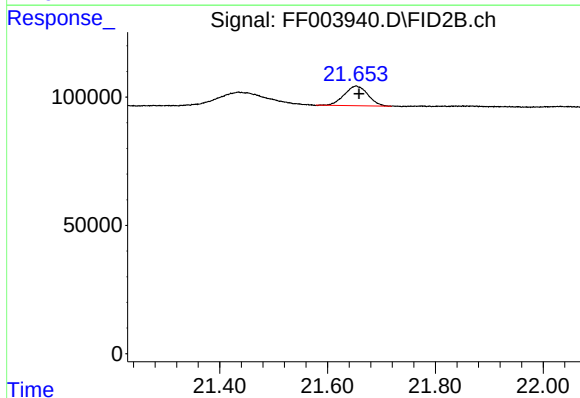

#18 N-TETRACONTANE

R.T.: 21.653 min
Delta R.T.: -0.006 min
Response: 233892
Conc: 1.88 ug/ml