

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
 Data File : FF003941.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2019 19:58
 Operator : AJ\SJ
 Sample : K2037-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :
 MW-01-20190320

Integration File: autoint1.e
 Quant Time: Mar 22 00:53:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.581	2096073	15.055 ug/ml
Target Compounds			
2) N-DECANE	4.267f	105201	0.684 ug/ml
5) N-HEXADECANE	9.748	98363	0.604 ug/ml
13) N-TRIACONTANE	17.649	110476	0.751 ug/ml
14) N-DOTRIACONTANE	18.486	104526	0.735 ug/ml
16) N-HEXATRIACONTANE	20.054	263104	2.016 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003941.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 19:58
Operator : AJ\SJ
Sample : K2037-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
MW-01-20190320

Integration File: autoint1.e
Quant Time: Mar 22 00:53:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

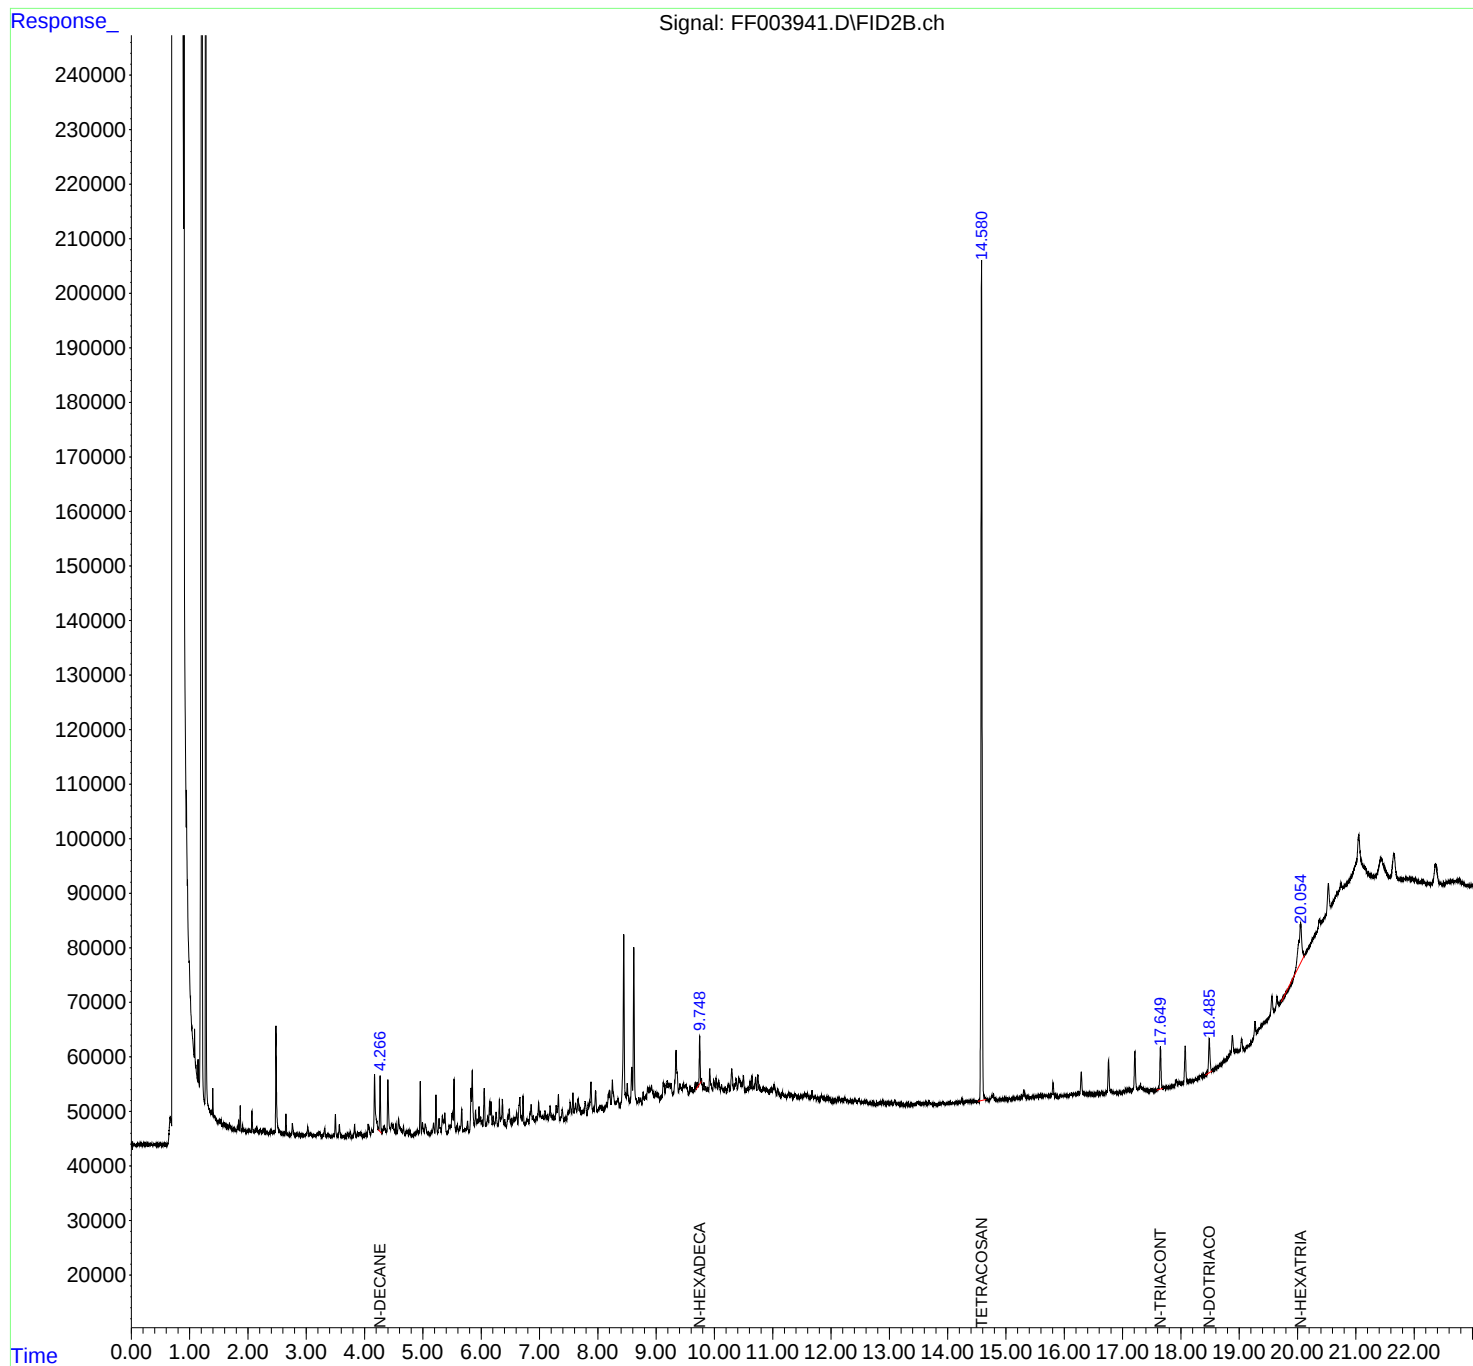


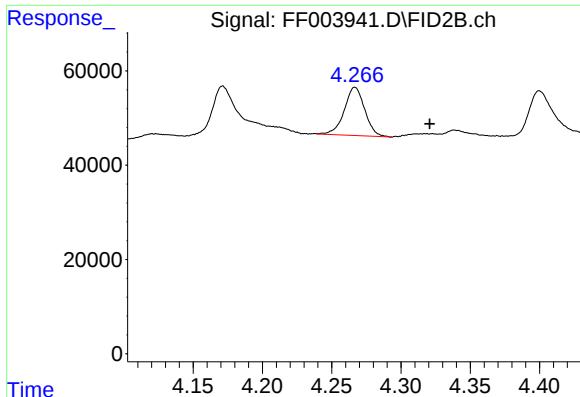

#2 N-DECANE


R.T.: 4.267 min
Delta R.T.: -0.054 min
Response: 105201
Conc: 0.68 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-01-20190320

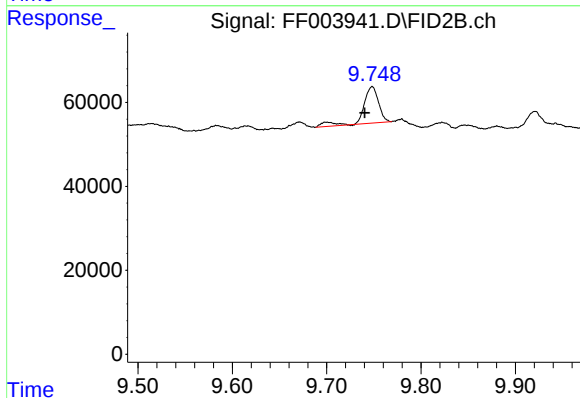


#5 N-HEXADECANE

R.T.: 9.748 min
Delta R.T.: 0.008 min
Response: 98363
Conc: 0.60 ug/ml

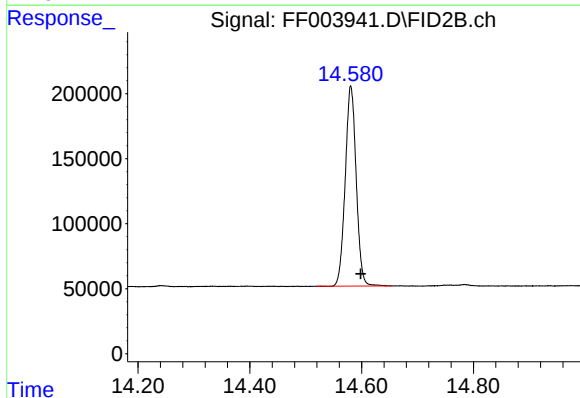


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.581 min
Delta R.T.: -0.018 min
Response: 2096073
Conc: 15.05 ug/ml

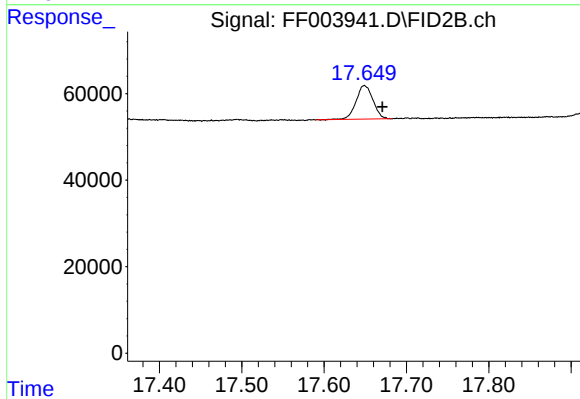

#13 N-TRIACONTANE


R.T.: 17.649 min
Delta R.T.: -0.022 min
Response: 110476
Conc: 0.75 ug/ml

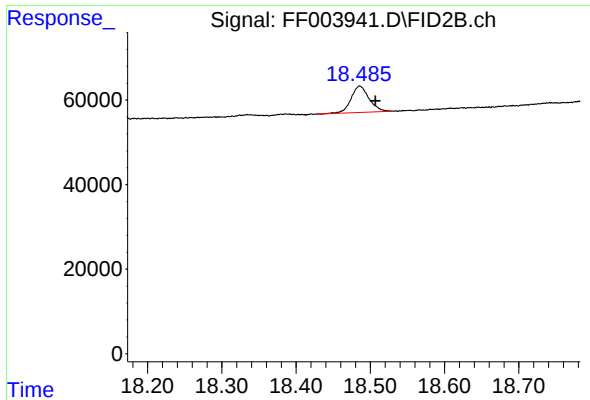

#14 N-DOTRIACONTANE

R.T.: 18.486 min
Delta R.T.: -0.021 min
Response: 104526
Conc: 0.74 ug/ml

Instrument :
FID_F
ClientSampleId :
MW-01-20190320

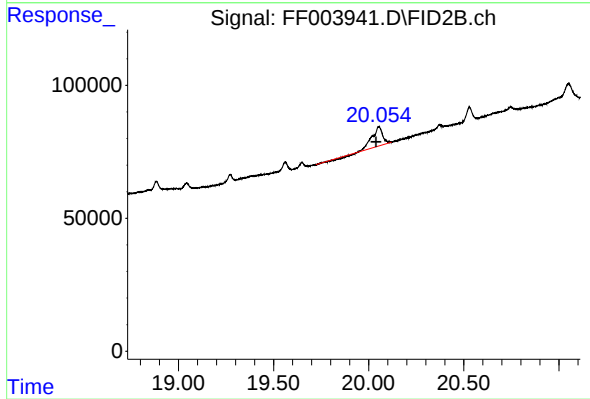

#16 N-HEXATRIACONTANE

R.T.: 20.054 min
Delta R.T.: 0.016 min
Response: 263104
Conc: 2.02 ug/ml