

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003945.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 22:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 00:54:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
9) S	TETRACOSANE-d50 (SURR...	14.580	2115845	15.197 ug/ml
Target Compounds				
13)	N-TRIACONTANE	17.648	111154	0.756 ug/ml
14)	N-DOTRIACONTANE	18.487	189720	1.334 ug/ml
16)	N-HEXATRIACONTANE	20.052	530187	4.063 ug/ml
18)	N-TETRACONTANE	21.651	349824	2.812 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032119\
Data File : FF003945.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2019 22:00
Operator : AJ\SJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
I.BLK

Integration File: autoint1.e
Quant Time: Mar 22 00:54:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

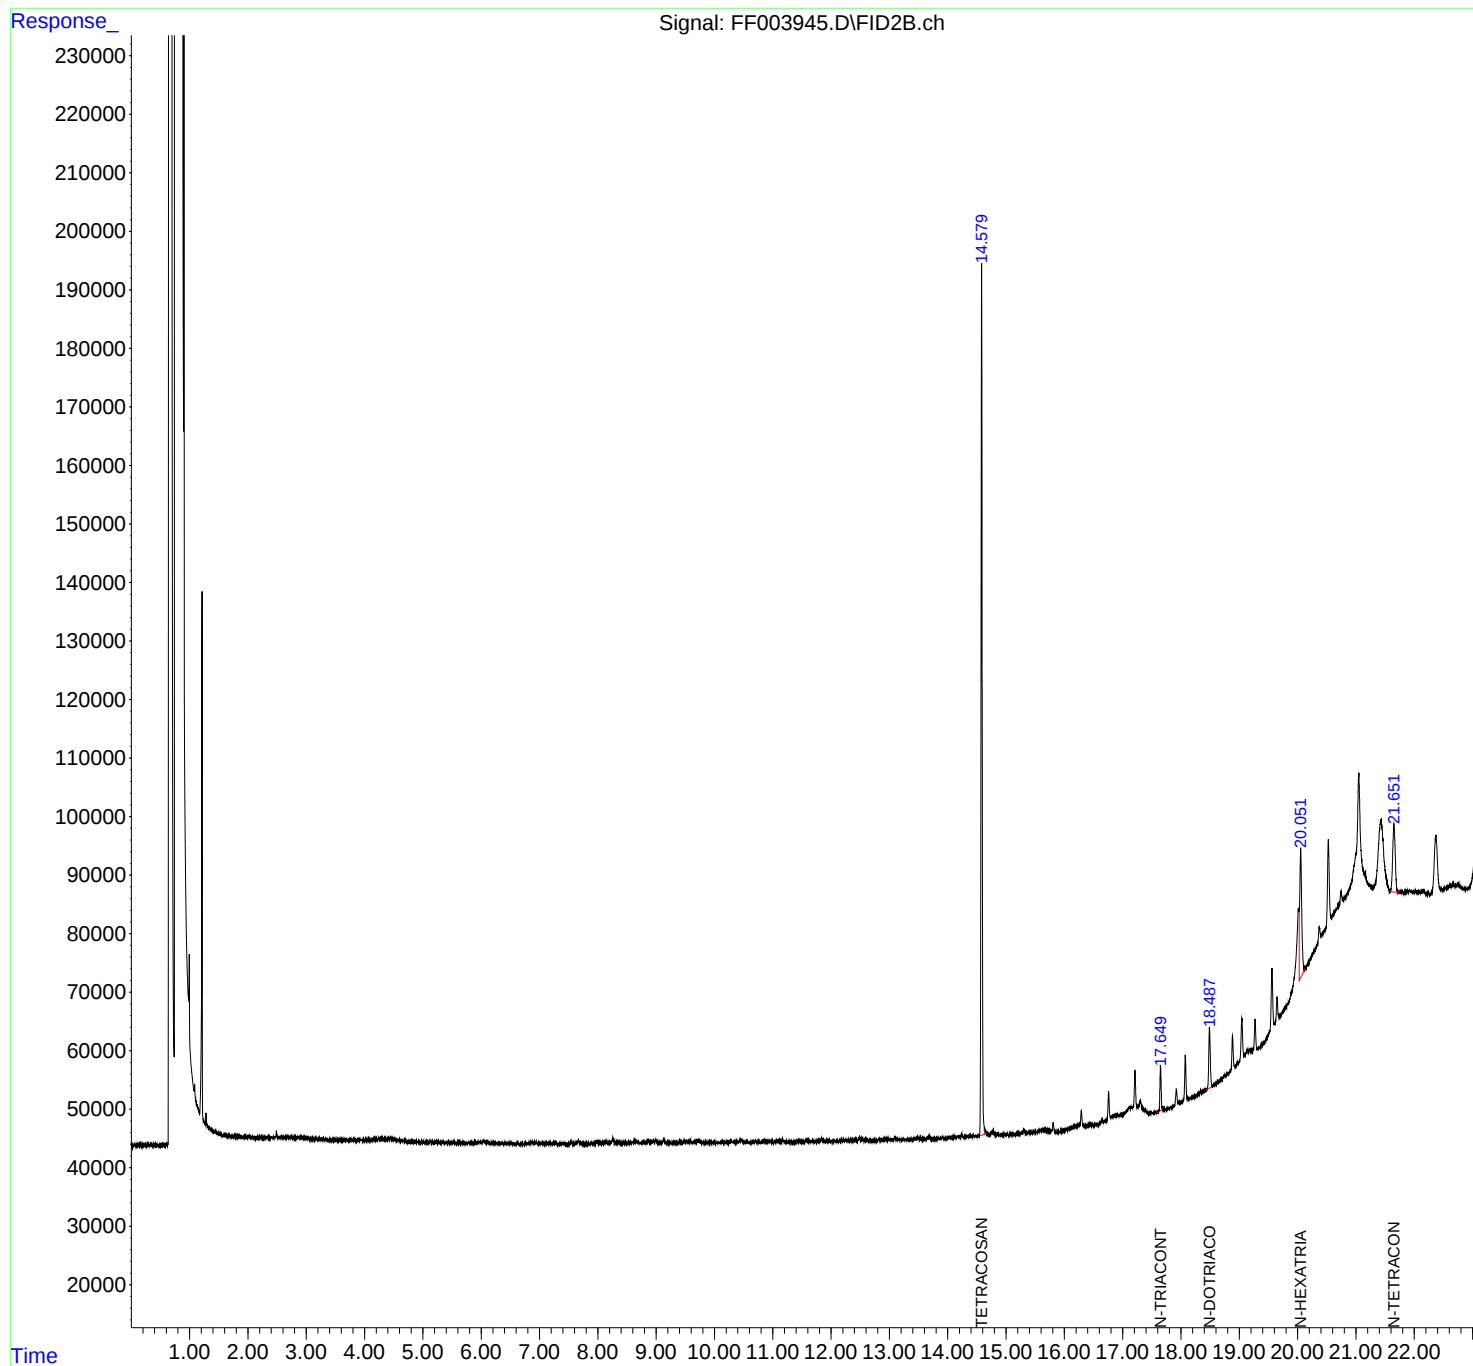


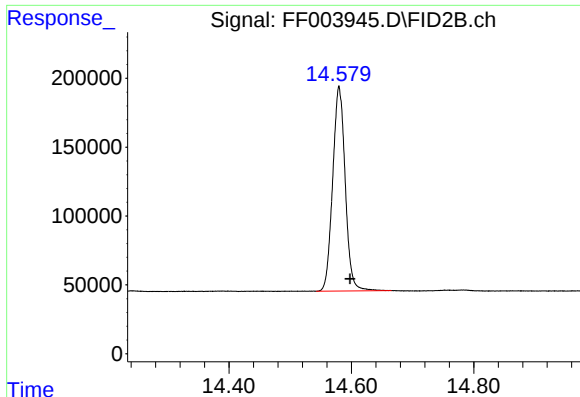

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.580 min
Delta R.T.: -0.018 min
Response: 2115845
Conc: 15.20 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK

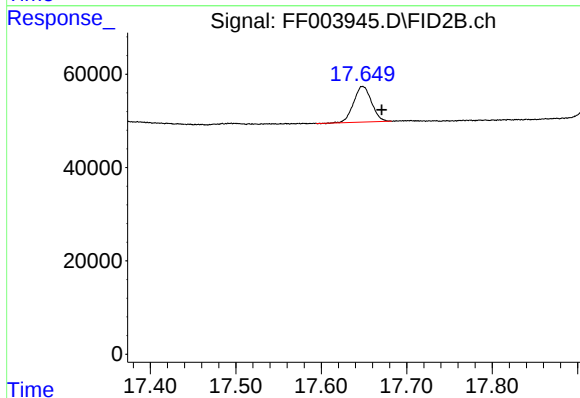


#13 N-TRIACONTANE

R.T.: 17.648 min
Delta R.T.: -0.022 min
Response: 111154
Conc: 0.76 ug/ml

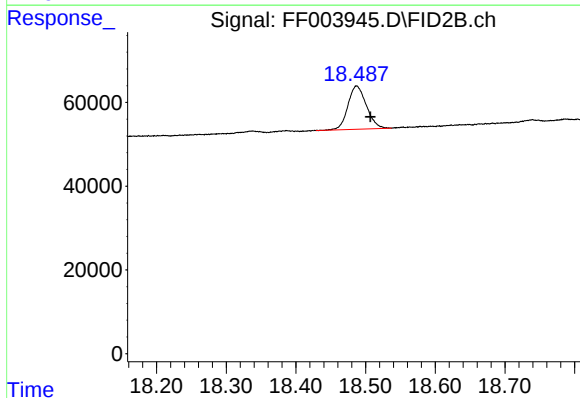


#14 N-DOTRIACONTANE

R.T.: 18.487 min
Delta R.T.: -0.020 min
Response: 189720
Conc: 1.33 ug/ml

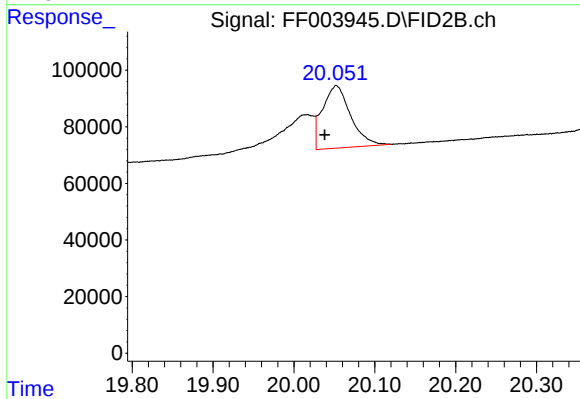

#16 N-HEXATRIACONTANE

R.T.: 20.052 min
Delta R.T.: 0.015 min
Response: 530187
Conc: 4.06 ug/ml

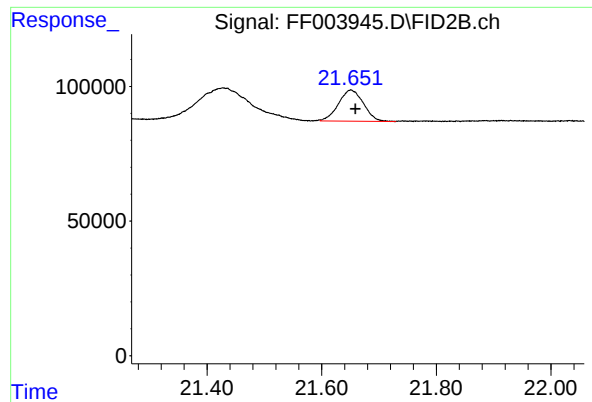

#18 N-TETRACONTANE

R.T.: 21.651 min
Delta R.T.: -0.008 min
Response: 349824
Conc: 2.81 ug/ml

Instrument :
FID_F
ClientSampleId :
I.BLK