

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
 Data File : FF010108.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2022 09:56
 Operator : AJ\MA
 Sample : MECL2
 Misc :
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 01:19:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
14) N-DOTRIACONTANE	18.602	180670	1.237 ug/ml
15) N-TETRATRIACONTANE	19.378	15476	0.113 ug/ml
16) N-HEXATRIACONTANE	20.155	384558	3.093 ug/ml
18) N-TETRACONTANE	21.813	920771	8.973 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
Data File : FF010108.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2022 09:56
Operator : AJ\MA
Sample : MECL2
Misc :
ALS Vial : 51 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 01:19:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

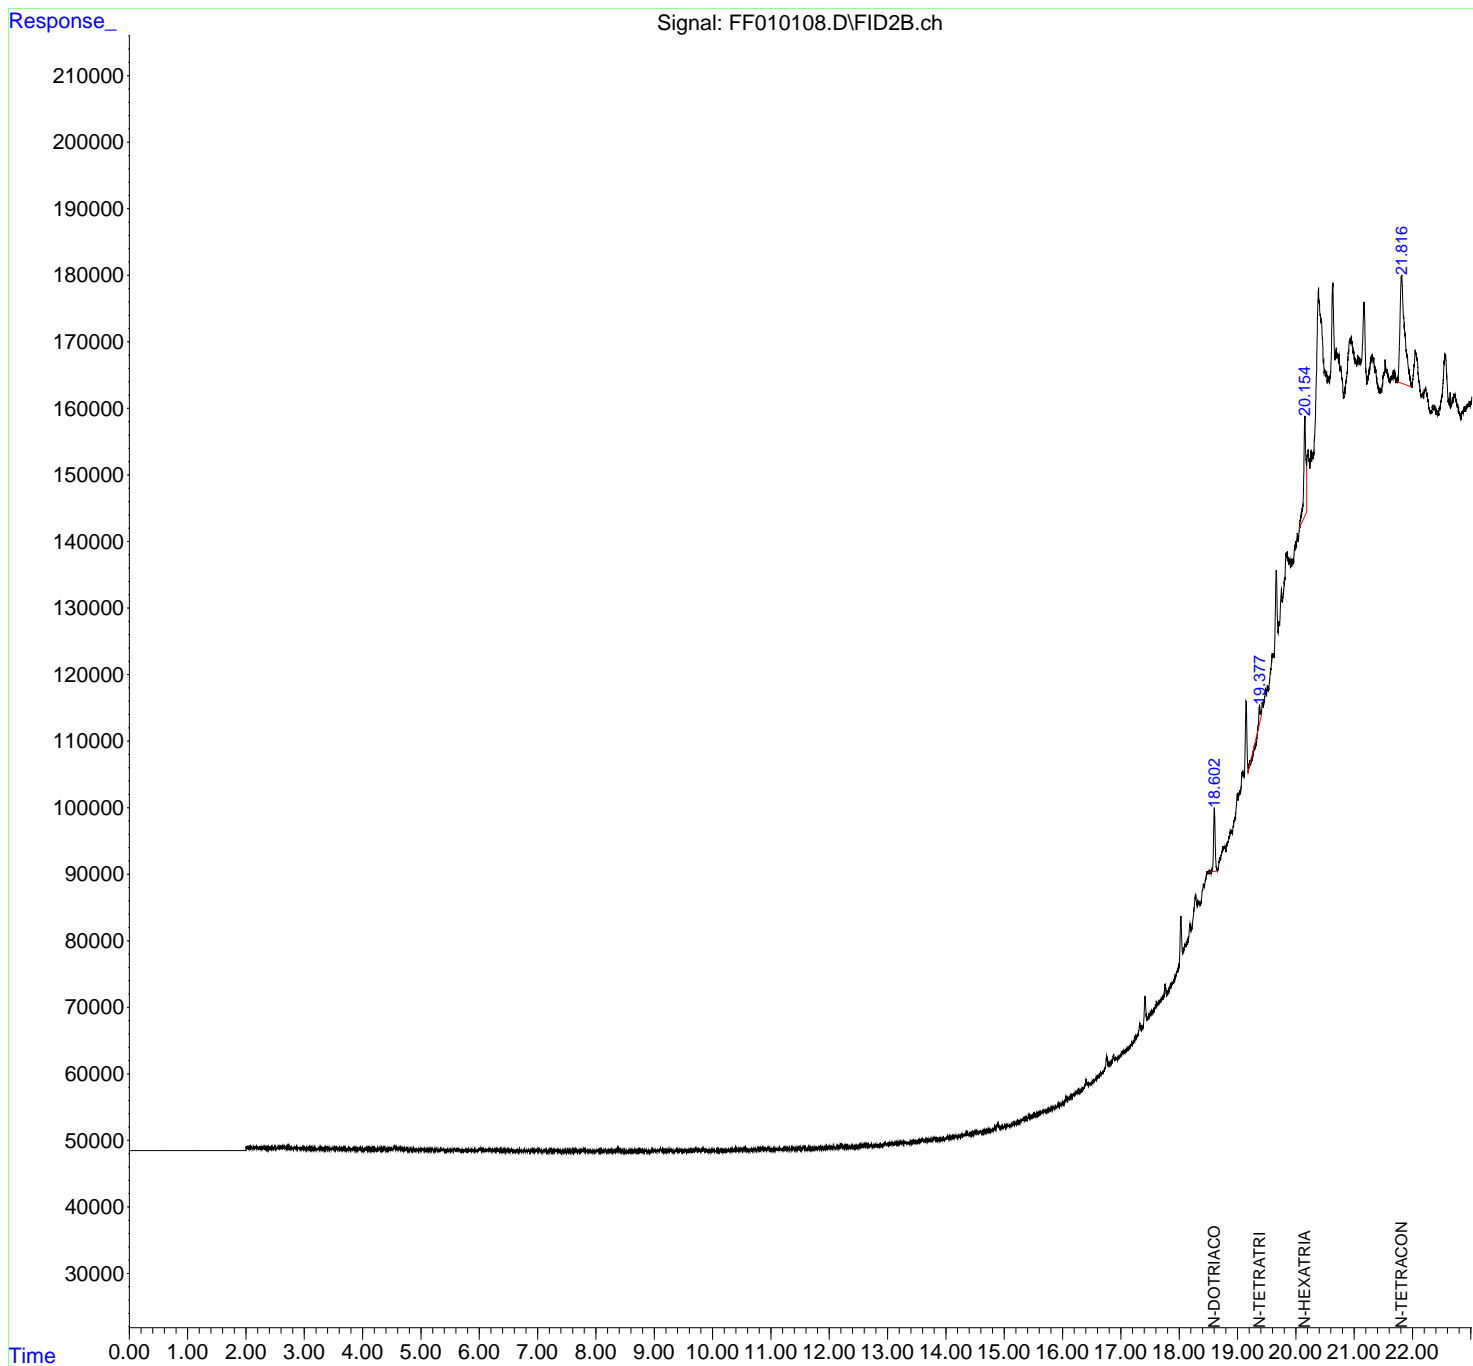


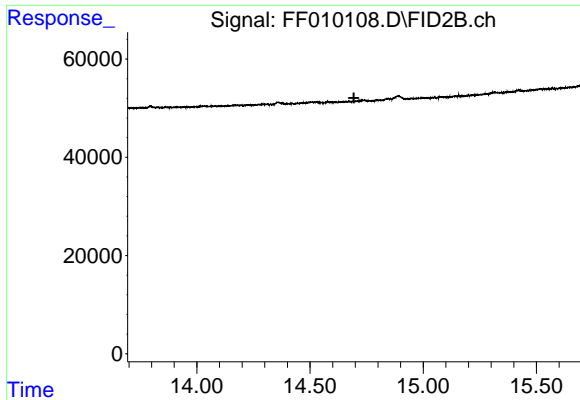

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
 Exp R.T.: 14.694 min
 Response: 0
 Conc: N.D.

Instrument :
 FID_F
 ClientSampleId :

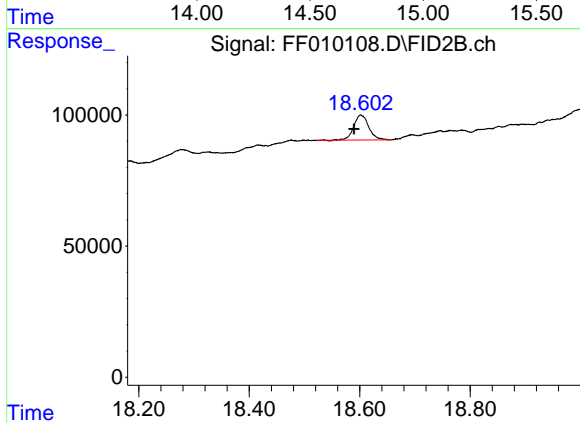


#14 N-DOTRIACONTANE

R.T.: 18.602 min
 Delta R.T.: 0.012 min
 Response: 180670
 Conc: 1.24 ug/ml

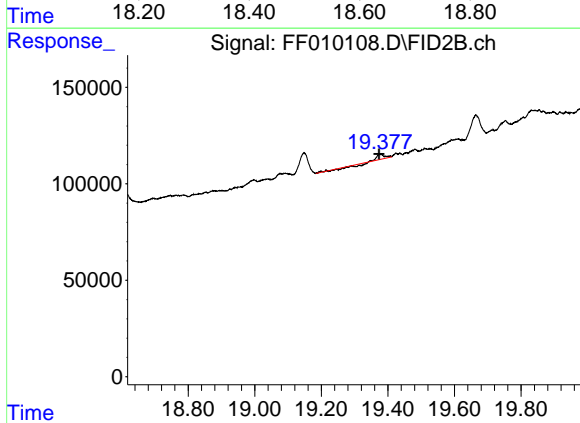


#15 N-TETRATRIACONTANE

R.T.: 19.378 min
 Delta R.T.: 0.004 min
 Response: 15476
 Conc: 0.11 ug/ml

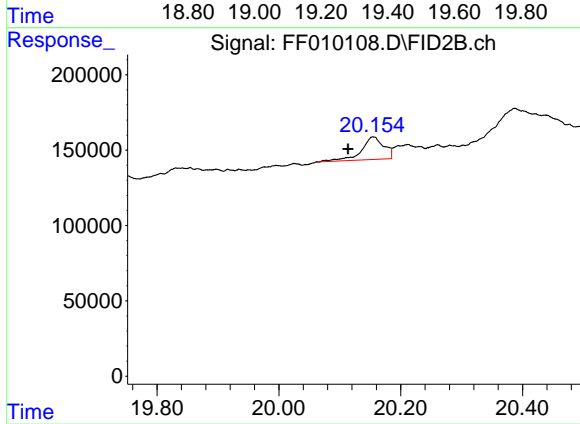

#16 N-HEXATRIACONTANE

R.T.: 20.155 min
 Delta R.T.: 0.041 min
 Response: 384558
 Conc: 3.09 ug/ml

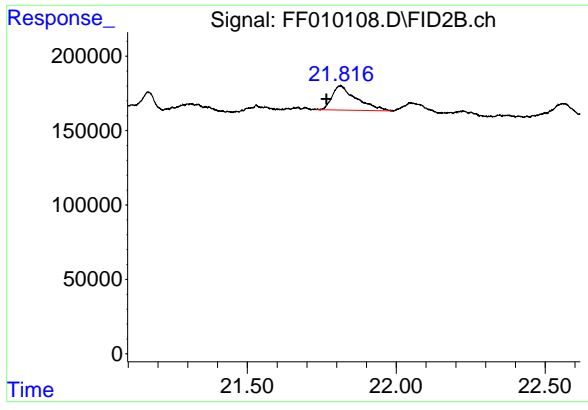

#18 N-TETRACONTANE

R.T.: 21.813 min
Delta R.T.: 0.048 min
Response: 920771
Conc: 8.97 ug/ml

Instrument :
FID_F
ClientSampleId :