

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
Data File : FF010111.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2022 11:40
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 01:20:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

3)	N-DODECANE	6.445	2805332	16.314 ug/ml
12)	N-OCTACOSANE	16.873	2505737	15.656 ug/ml
14)	N-DOTRIACONTANE	18.604	387770	2.655 ug/ml
15)	N-TETRATRIACONTANE	19.379	48113	0.351 ug/ml
16)	N-HEXATRIACONTANE	20.156	583857	4.696 ug/ml
18)	N-TETRACONTANE	21.804	722010	7.036 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
Data File : FF010111.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2022 11:40
Operator : AJ\MA
Sample : RT MARKER
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 01:20:20 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

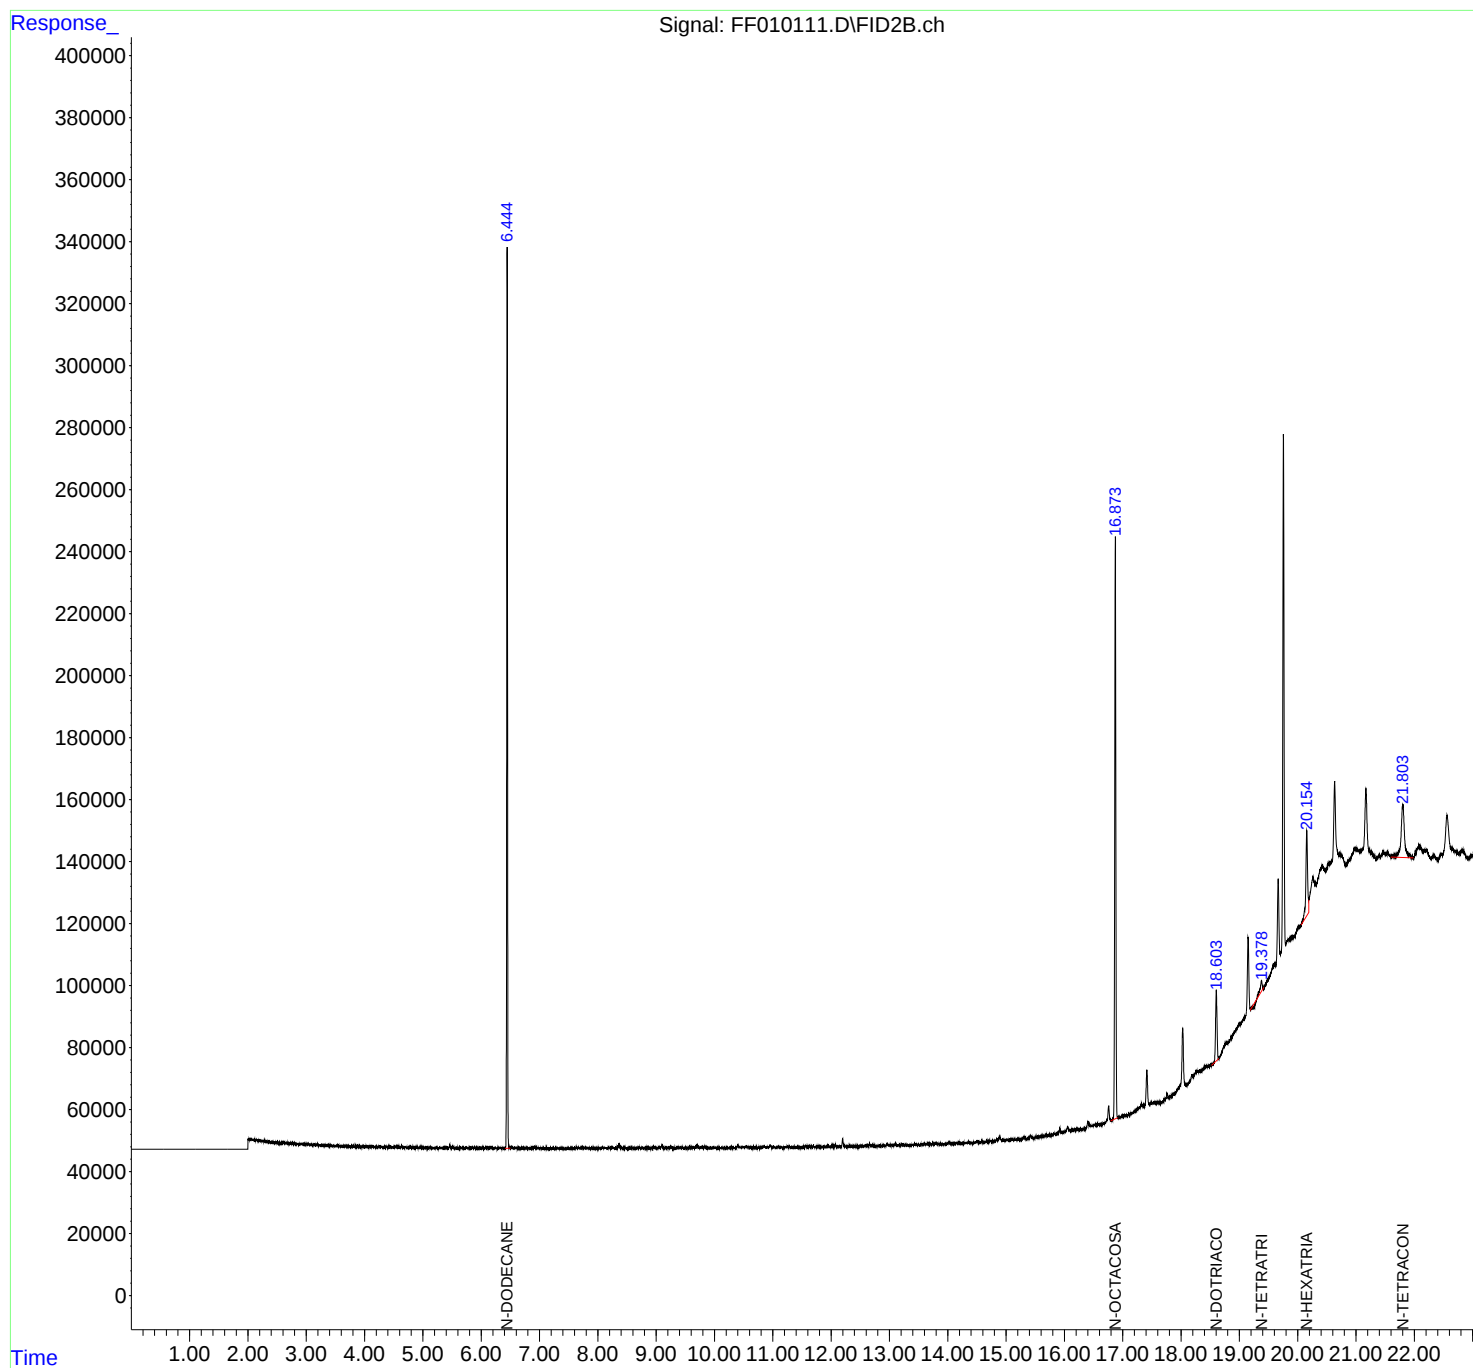


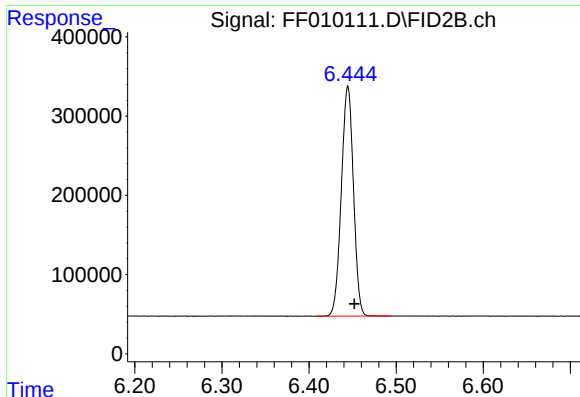

#3 N-DODECANE


R.T.: 6.445 min
Delta R.T.: -0.008 min
Response: 2805332
Conc: 16.31 ug/ml

Instrument :
FID_F
ClientSampleId :

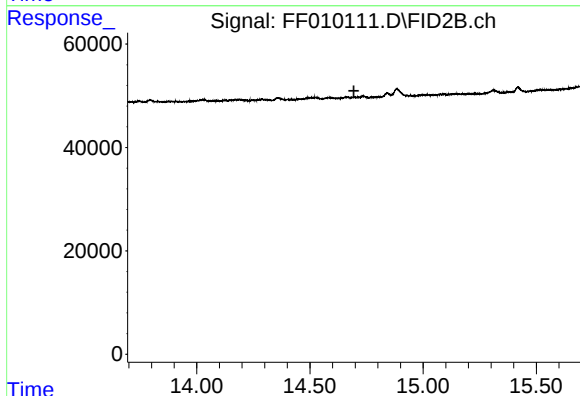


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.694 min
Response: 0
Conc: N.D.

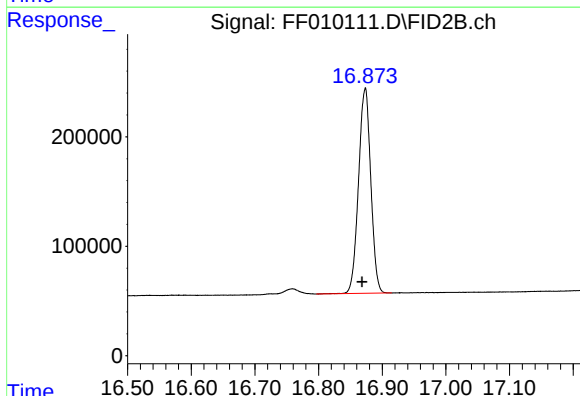


#12 N-OCTACOSANE

R.T.: 16.873 min
Delta R.T.: 0.004 min
Response: 2505737
Conc: 15.66 ug/ml

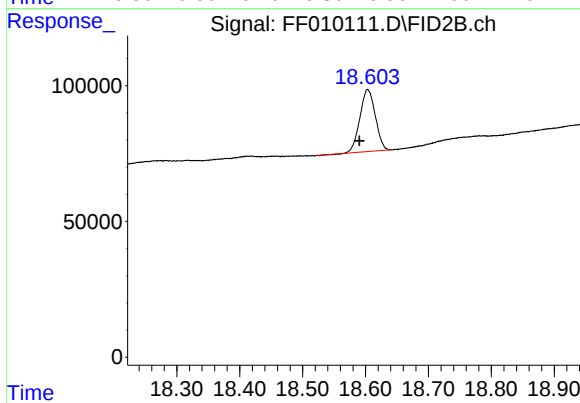

#14 N-DOTRIACONTANE


R.T.: 18.604 min
Delta R.T.: 0.013 min
Response: 387770
Conc: 2.66 ug/ml

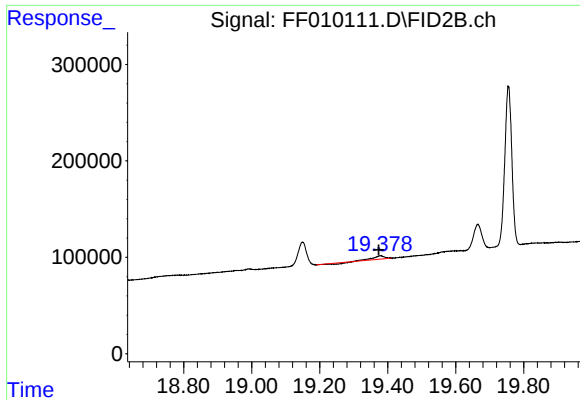

#15 N-TETRATRIACONTANE


R.T.: 19.379 min
Delta R.T.: 0.005 min
Response: 48113
Conc: 0.35 ug/ml

Instrument :
FID_F
ClientSampleId :

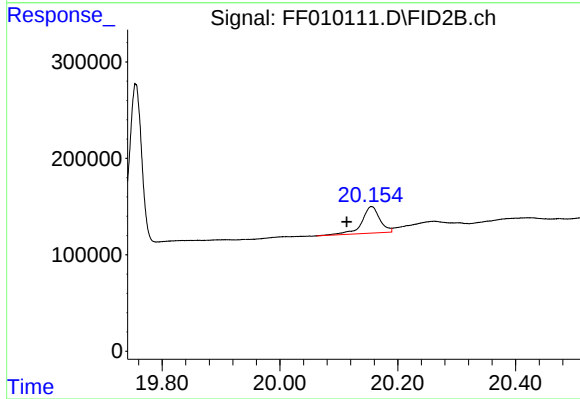

#16 N-HEXATRIACONTANE

R.T.: 20.156 min
Delta R.T.: 0.042 min
Response: 583857
Conc: 4.70 ug/ml

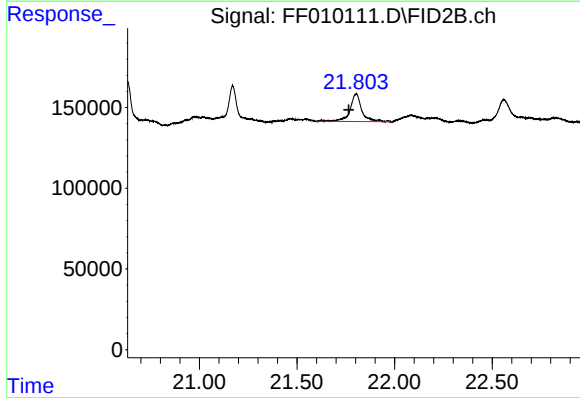

#18 N-TETRACONTANE

R.T.: 21.804 min
Delta R.T.: 0.038 min
Response: 722010
Conc: 7.04 ug/ml