

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
 Data File : FF010115.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2022 17:11
 Operator : AJ\MA
 Sample : N1974-03 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 01:21:11 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.696	236935	1.580 ug/ml
Target Compounds			
7) N-EICOSANE	12.545f	87427	0.503 ug/ml
8) N-DOCOSANE	13.827	173628	1.016 ug/ml
10) N-TETRACOSANE	14.881	628067	3.719 ug/ml
12) N-OCTACOSANE	16.882	216219	1.351 ug/ml
14) N-DOTRIACONTANE	18.603	177696	1.217 ug/ml
15) N-TETRATRIACONTANE	19.383	45399	0.331 ug/ml
16) N-HEXATRIACONTANE	20.154	190106	1.529 ug/ml
18) N-TETRACONTANE	21.721	237836	2.318 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
Data File : FF010115.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2022 17:11
Operator : AJ\MA
Sample : N1974-03 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 01:21:11 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

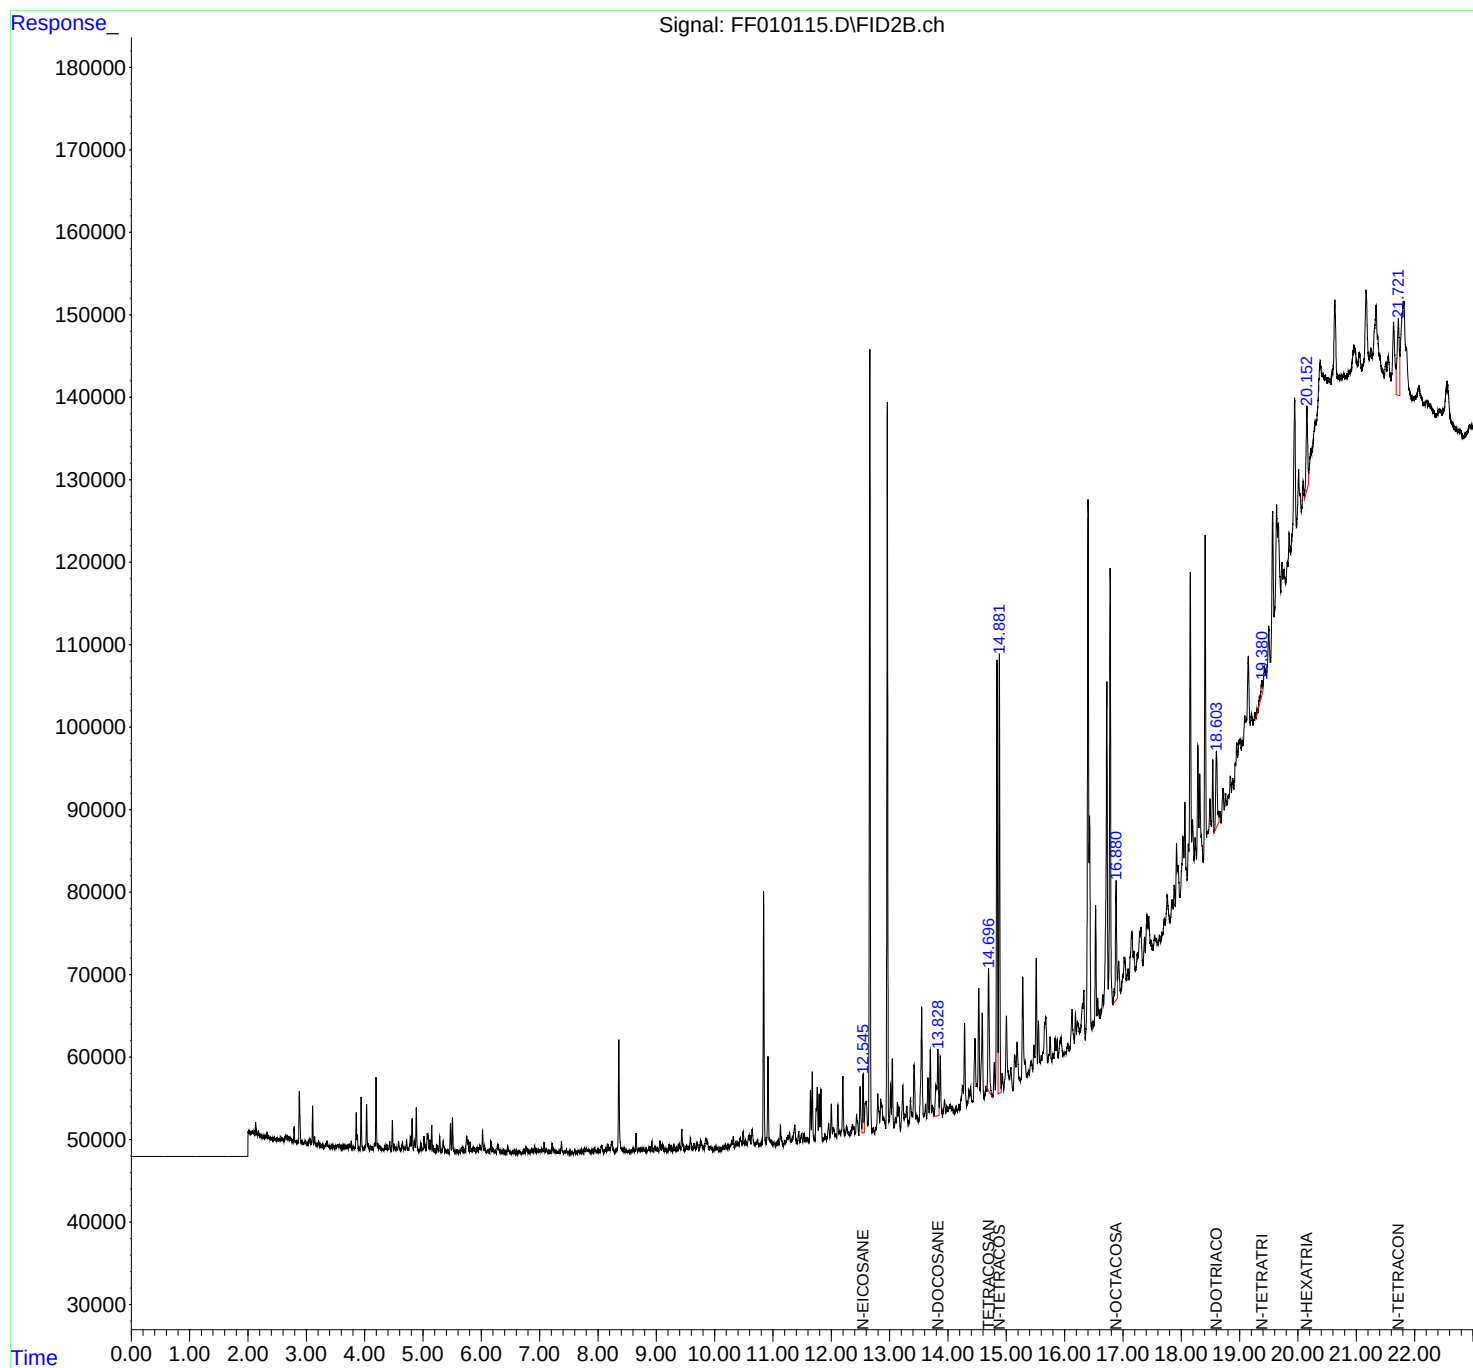


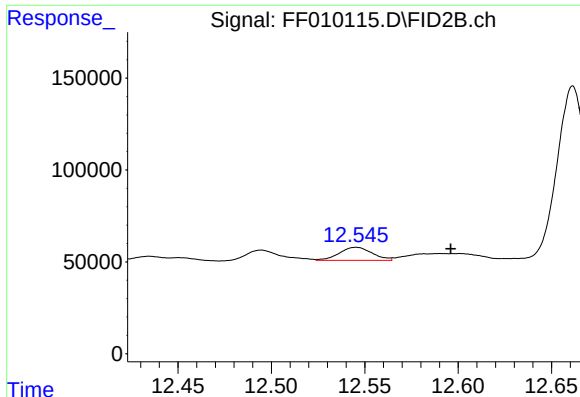

#7 N-EICOSANE


R.T.: 12.545 min
Delta R.T.: -0.051 min
Response: 87427
Conc: 0.50 ug/ml

Instrument :
FID_F
ClientSampleId :

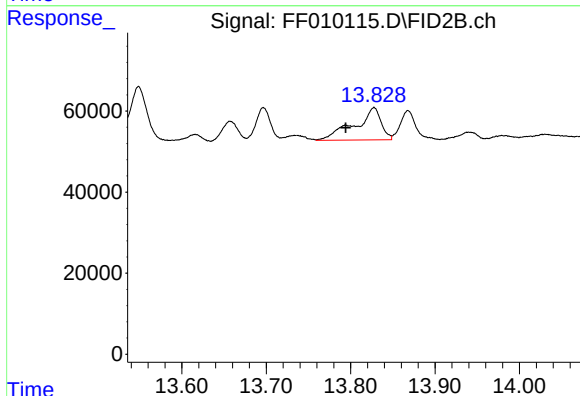


#8 N-DOCOSANE

R.T.: 13.827 min
Delta R.T.: 0.033 min
Response: 173628
Conc: 1.02 ug/ml

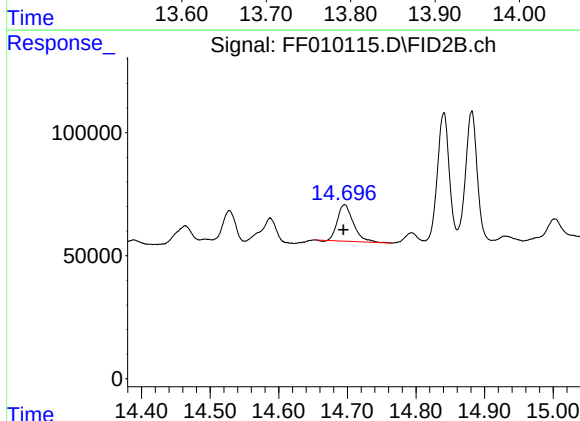


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.696 min
Delta R.T.: 0.002 min
Response: 236935
Conc: 1.58 ug/ml

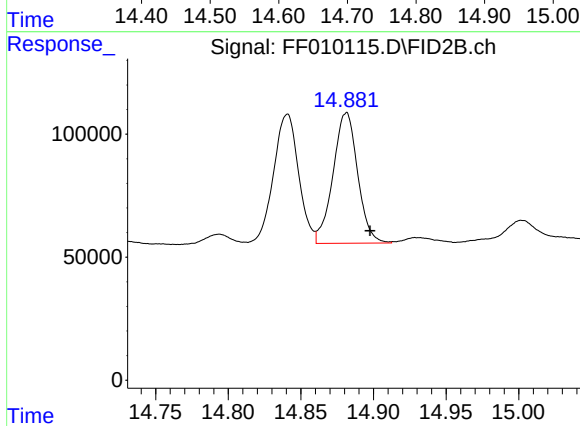

#10 N-TETRACOSANE


R.T.: 14.881 min
Delta R.T.: -0.016 min
Response: 628067
Conc: 3.72 ug/ml

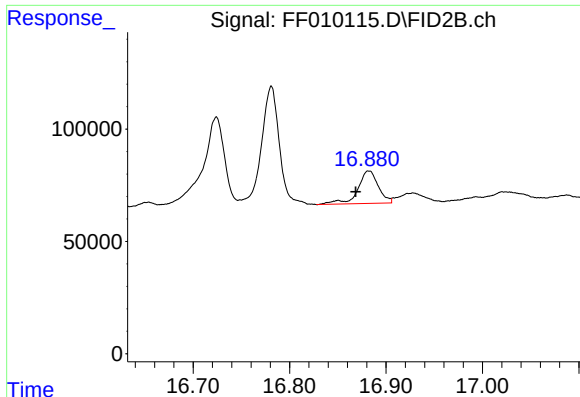

#12 N-OCTACOSANE


R.T.: 16.882 min
Delta R.T.: 0.014 min
Response: 216219
Conc: 1.35 ug/ml

Instrument :
FID_F
ClientSampleId :

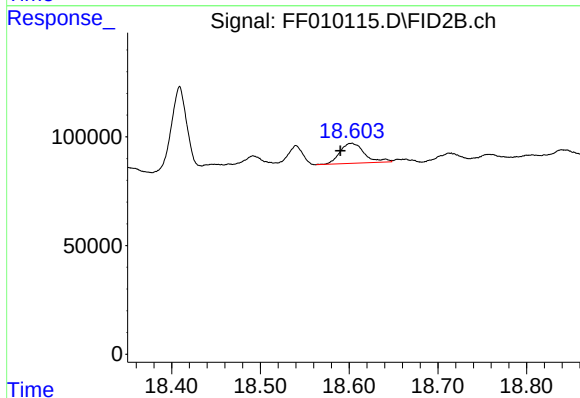


#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: 0.012 min
Response: 177696
Conc: 1.22 ug/ml

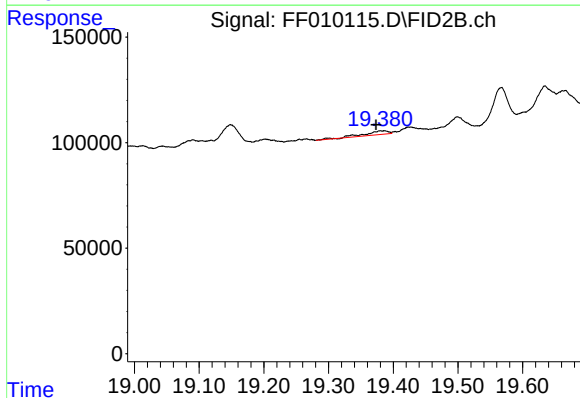


#15 N-TETRATRIACONTANE

R.T.: 19.383 min
Delta R.T.: 0.010 min
Response: 45399
Conc: 0.33 ug/ml

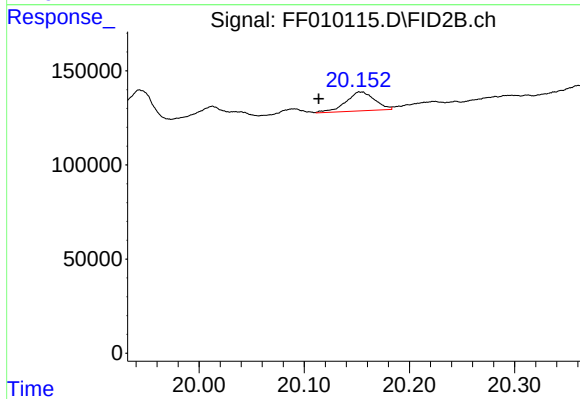

#16 N-HEXATRIACONTANE

R.T.: 20.154 min
Delta R.T.: 0.040 min
Response: 190106
Conc: 1.53 ug/ml

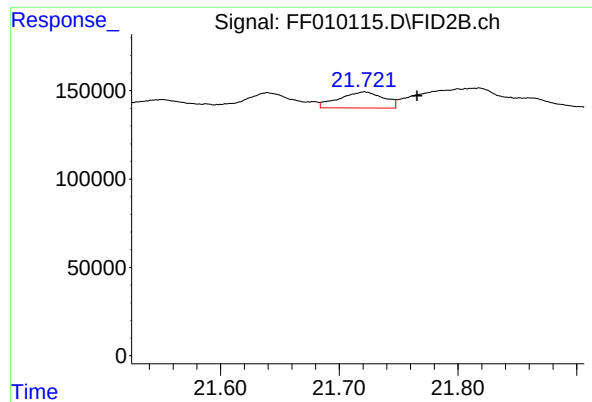

#18 N-TETRACONTANE

R.T.: 21.721 min
Delta R.T.: -0.044 min
Response: 237836
Conc: 2.32 ug/ml

Instrument :

FID_F

ClientSampleId :