

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
 Data File : FF010117.D
 Signal(s) : FID2B.ch
 Acq On : 21 Mar 2022 18:12
 Operator : AJ\MA
 Sample : N1974-06 10X
 Misc :
 ALS Vial : 60 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 22 01:21:41 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
 Quant Title :
 QLast Update : Thu Mar 10 12:46:01 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.695	272815	1.819 ug/ml
Target Compounds			
5) N-HEXADECANE	9.858	96151	0.552 ug/ml
7) N-EICOSANE	12.546f	129661	0.747 ug/ml
8) N-DOCOSANE	13.826	267139	1.562 ug/ml
10) N-TETRACOSANE	14.881	1049308	6.213 ug/ml
12) N-OCTACOSANE	16.882	312081	1.950 ug/ml
14) N-DOTRIACONTANE	18.603	1029021	7.046 ug/ml
15) N-TETRATRIACONTANE	19.379	74788	0.546 ug/ml
16) N-HEXATRIACONTANE	20.153	1399118	11.252 ug/ml
18) N-TETRACONTANE	21.802	2003097	19.521 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032122\
Data File : FF010117.D
Signal(s) : FID2B.ch
Acq On : 21 Mar 2022 18:12
Operator : AJ\MA
Sample : N1974-06 10X
Misc :
ALS Vial : 60 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 22 01:21:41 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031022.M
Quant Title :
QLast Update : Thu Mar 10 12:46:01 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

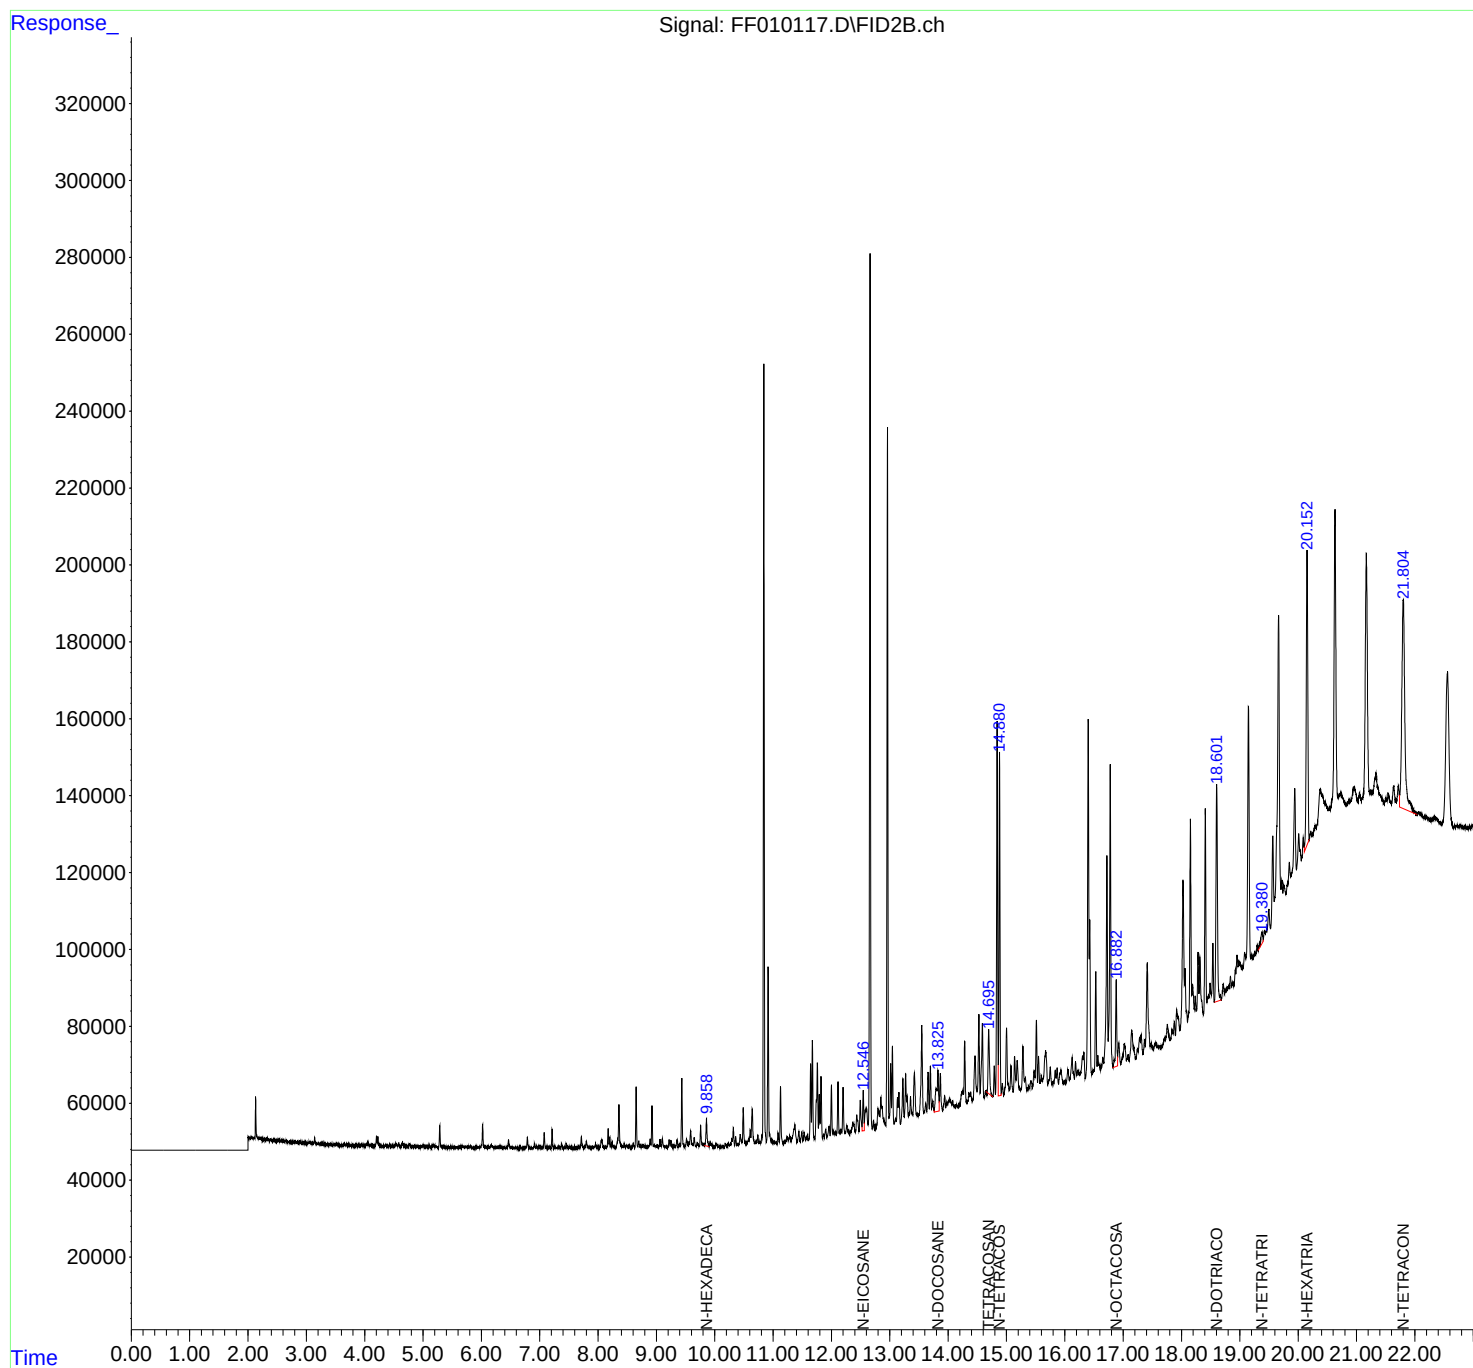


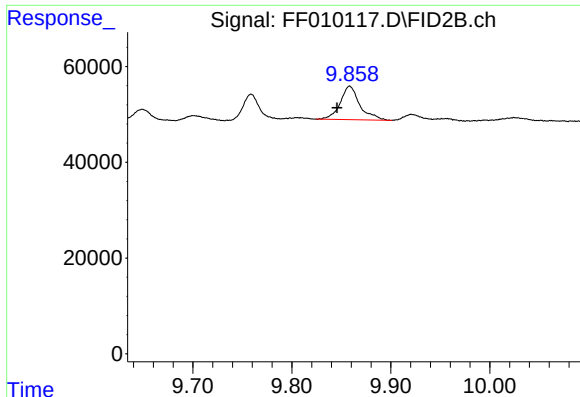

#5 N-HEXADECANE


R.T.: 9.858 min
Delta R.T.: 0.013 min
Response: 96151
Conc: 0.55 ug/ml

Instrument :
FID_F
ClientSampleId :

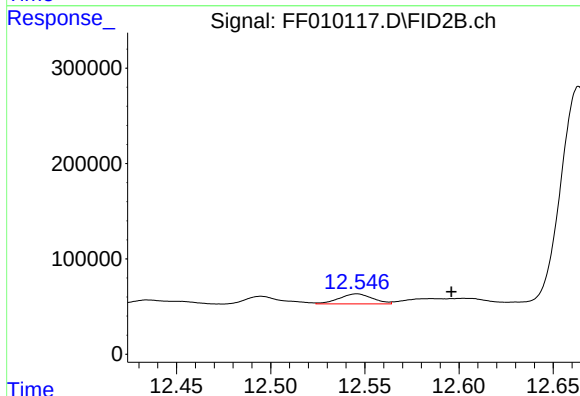


#7 N-EICOSANE

R.T.: 12.546 min
Delta R.T.: -0.050 min
Response: 129661
Conc: 0.75 ug/ml

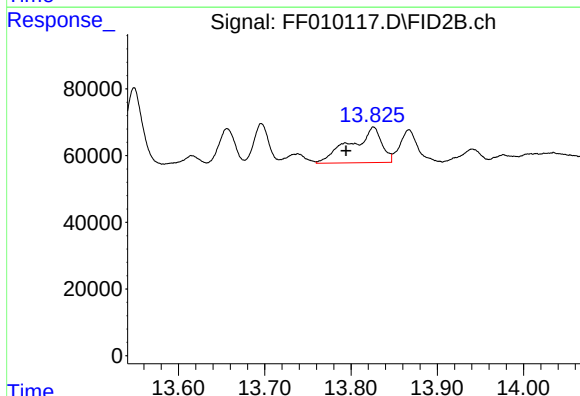


#8 N-DOCOSANE

R.T.: 13.826 min
Delta R.T.: 0.032 min
Response: 267139
Conc: 1.56 ug/ml

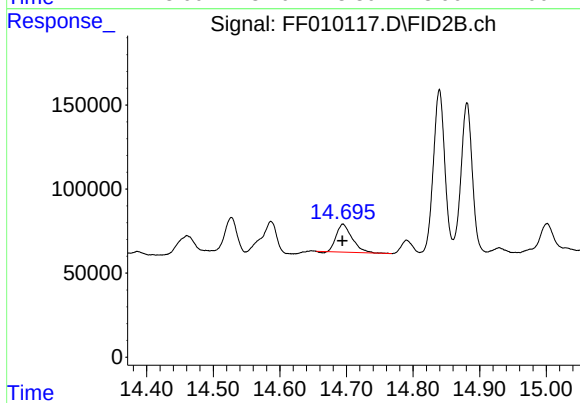

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 14.695 min
Delta R.T.: 0.000 min
Response: 272815
Conc: 1.82 ug/ml

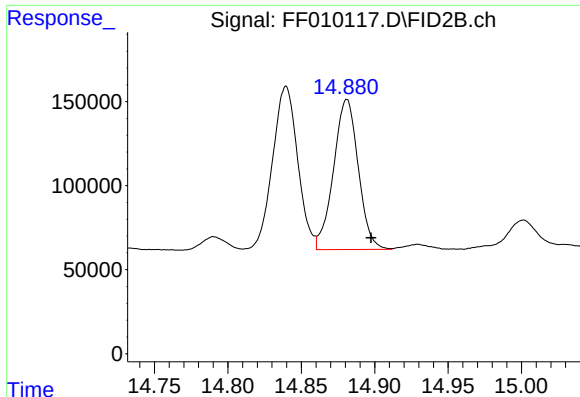

#10 N-TETRACOSANE


R.T.: 14.881 min
Delta R.T.: -0.017 min
Response: 1049308
Conc: 6.21 ug/ml

Instrument :
FID_F
ClientSampleId :

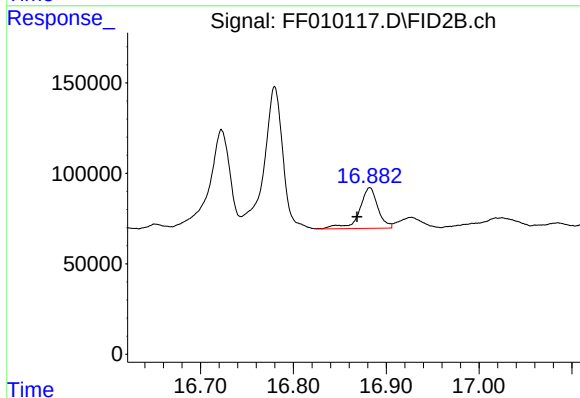


#12 N-OCTACOSANE

R.T.: 16.882 min
Delta R.T.: 0.014 min
Response: 312081
Conc: 1.95 ug/ml

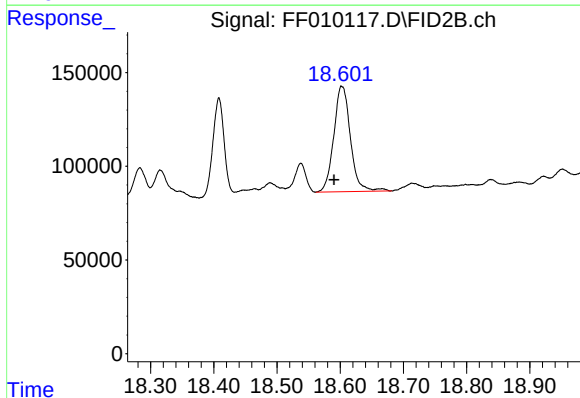


#14 N-DOTRIACONTANE

R.T.: 18.603 min
Delta R.T.: 0.013 min
Response: 1029021
Conc: 7.05 ug/ml

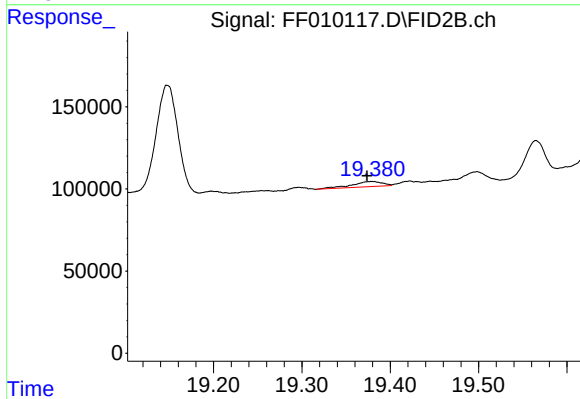

#15 N-TETRATRIACONTANE

R.T.: 19.379 min
Delta R.T.: 0.005 min
Response: 74788
Conc: 0.55 ug/ml

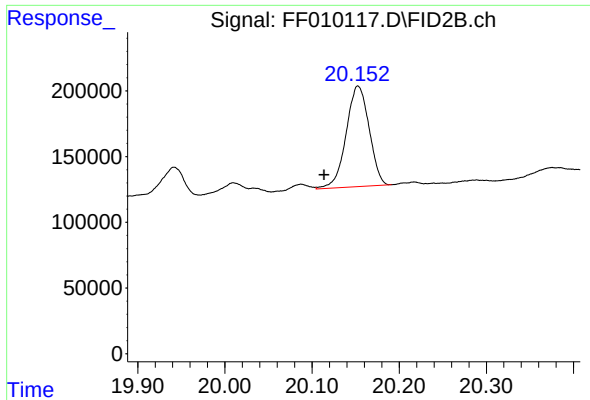


#16 N-HEXATRIACONTANE

R.T.: 20.153 min
Delta R.T.: 0.039 min
Response: 1399118
Conc: 11.25 ug/ml

Instrument :

FID_F

ClientSampleId :

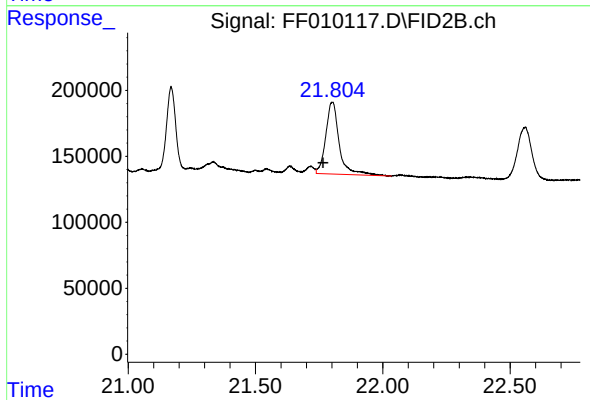

#18 N-TETRACONTANE

R.T.: 21.802 min
Delta R.T.: 0.036 min
Response: 2003097
Conc: 19.52 ug/ml