

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032323\
 Data File : FF012342.D
 Signal(s) : FID2B.ch
 Acq On : 23 Mar 2023 19:37
 Operator : YP\AJ
 Sample : 02021-07 20X
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 24 01:03:55 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
 Quant Title :
 QLast Update : Wed Mar 15 18:07:23 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.029	137408	1.228 ug/ml
Target Compounds			
7) N-EICOSANE	12.933	116895	0.879 ug/ml
8) N-DOCOSANE	14.135	78821	0.620 ug/ml
10) N-TETRACOSANE	15.229	1488734	11.938 ug/ml
11) N-HEXACOSANE	16.230	35763	0.299 ug/ml
12) N-OCTACOSANE	17.198	46749	0.406 ug/ml
13) N-TRIACONTANE	18.090	219833	1.998 ug/ml
14) N-DOTRIACONTANE	18.937	41997	0.405 ug/ml
15) N-TETRATRIACONTANE	19.702	329211	3.480 ug/ml
16) N-HEXATRIACONTANE	20.442	1585971	18.103 ug/ml
18) N-TETRACONTANE	22.102	187707	2.298 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032323\
Data File : FF012342.D
Signal(s) : FID2B.ch
Acq On : 23 Mar 2023 19:37
Operator : YP\AJ
Sample : 02021-07 20X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 24 01:03:55 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

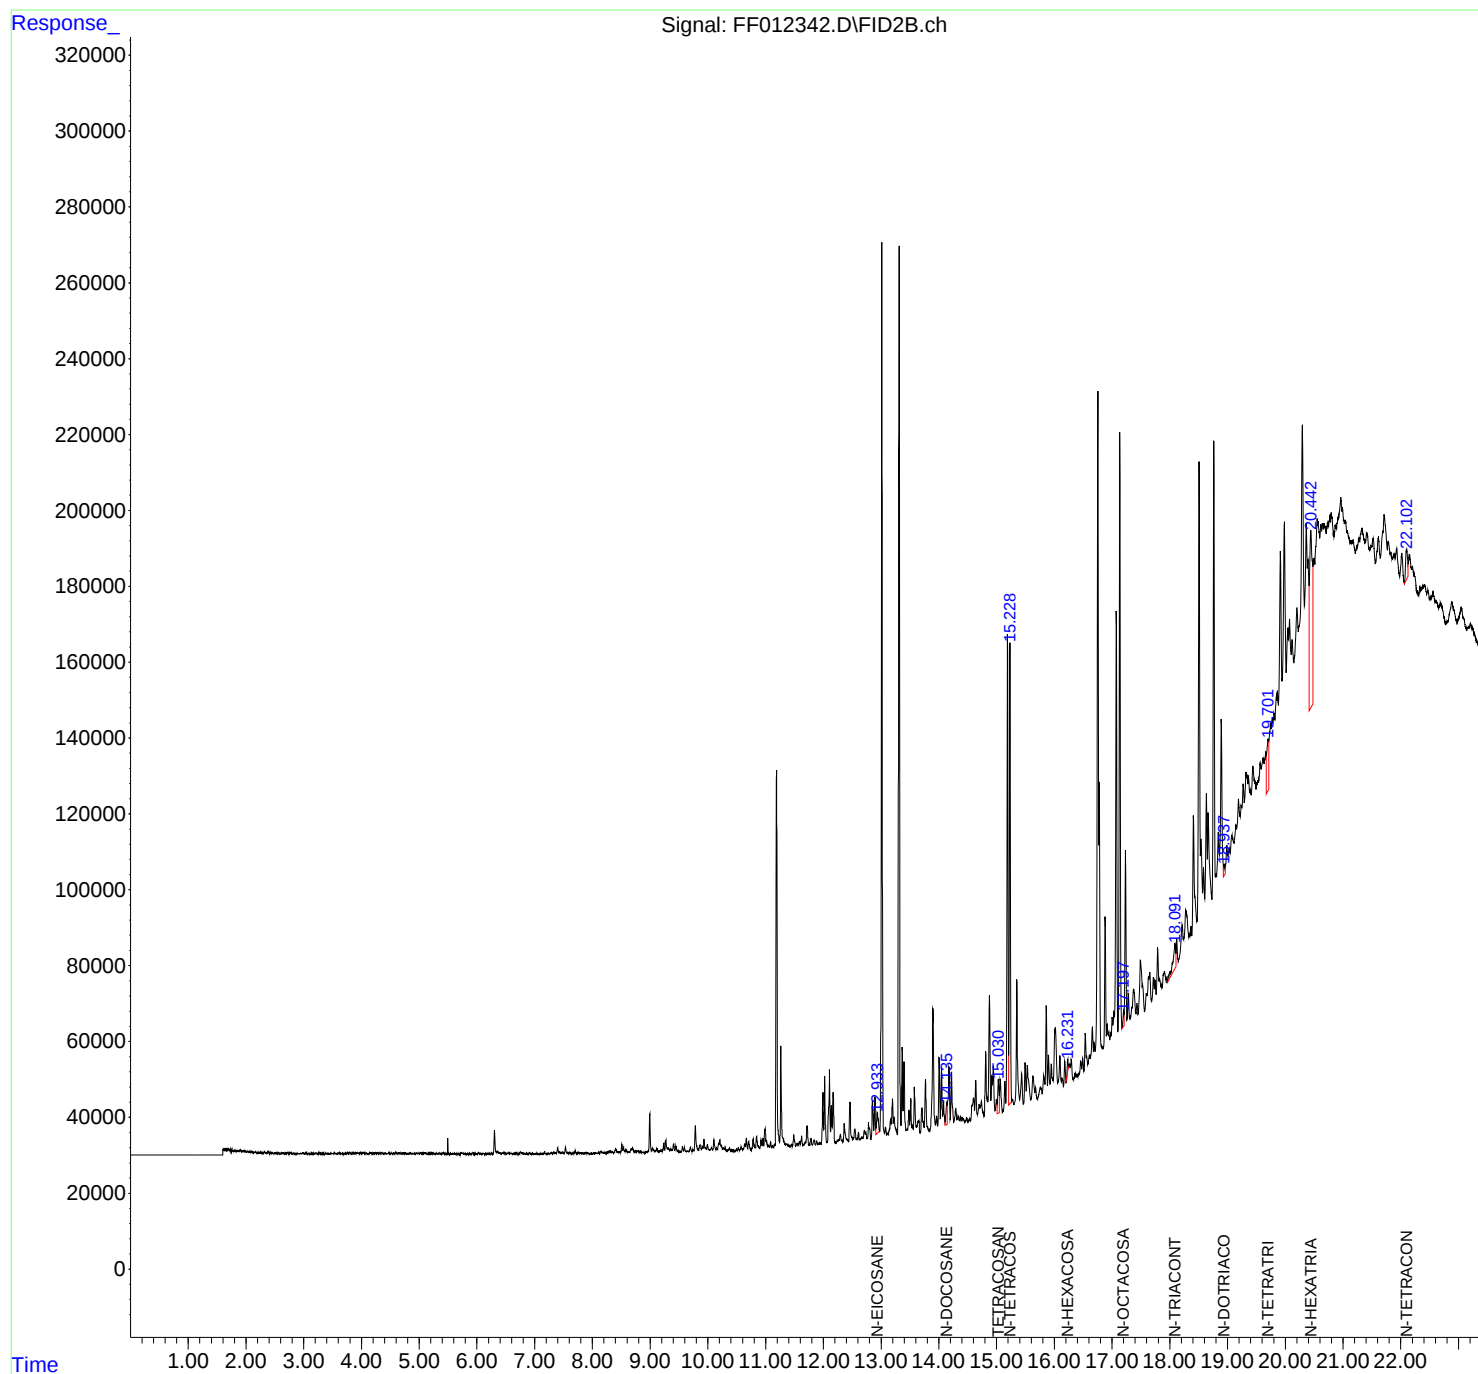


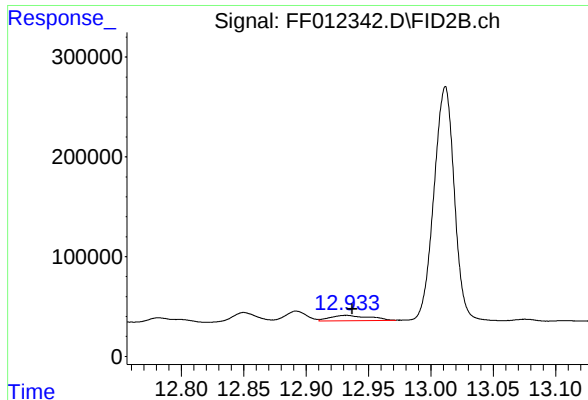

#7 N-EICOSANE


R.T.: 12.933 min
Delta R.T.: -0.005 min
Response: 116895
Conc: 0.88 ug/ml

Instrument :
FID_F
ClientSampleId :

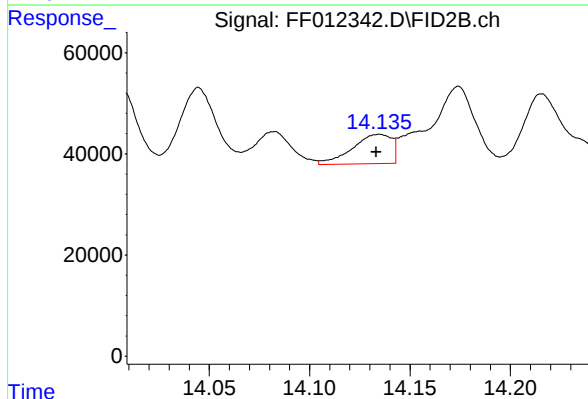


#8 N-DOCOSANE

R.T.: 14.135 min
Delta R.T.: 0.001 min
Response: 78821
Conc: 0.62 ug/ml

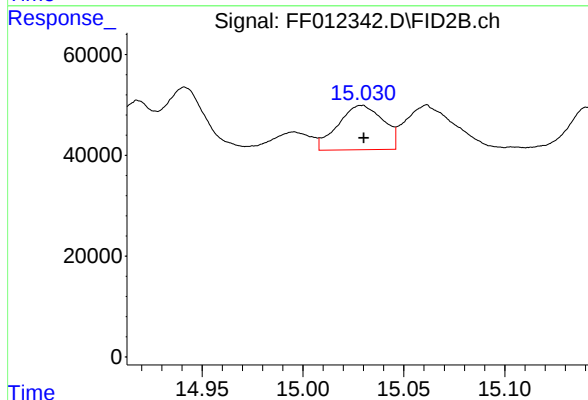


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.029 min
Delta R.T.: -0.001 min
Response: 137408
Conc: 1.23 ug/ml

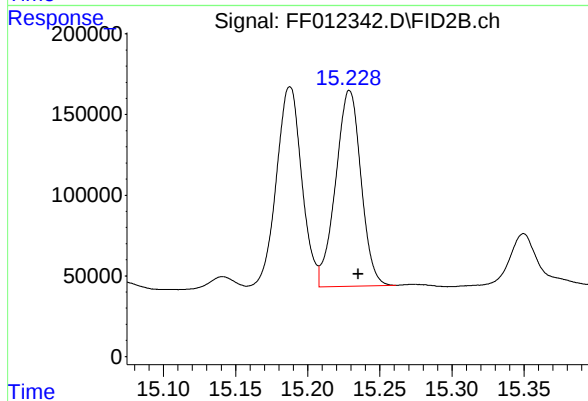

#10 N-TETRACOSANE


R.T.: 15.229 min
Delta R.T.: -0.006 min
Response: 1488734
Conc: 11.94 ug/ml

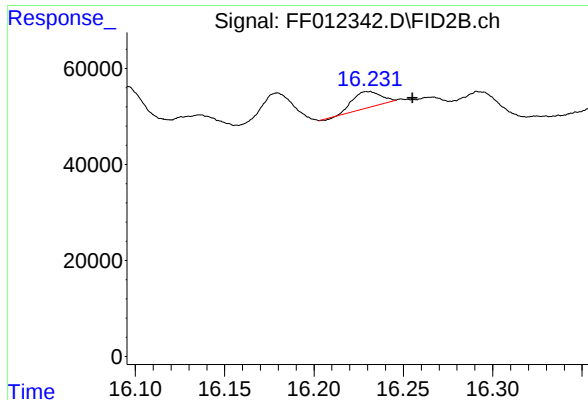

#11 N-HEXACOSANE


R.T.: 16.230 min
Delta R.T.: -0.025 min
Response: 35763
Conc: 0.30 ug/ml

Instrument :
FID_F
ClientSampleId :

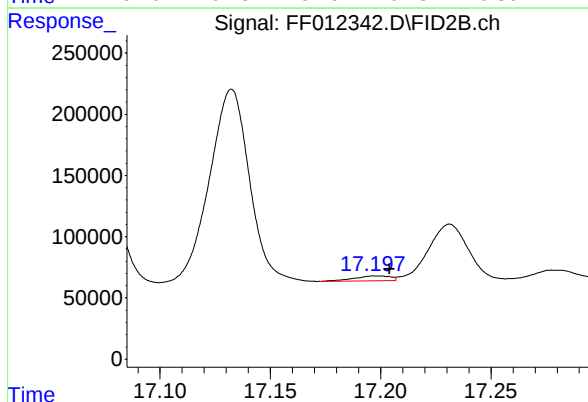


#12 N-OCTACOSANE

R.T.: 17.198 min
Delta R.T.: -0.006 min
Response: 46749
Conc: 0.41 ug/ml

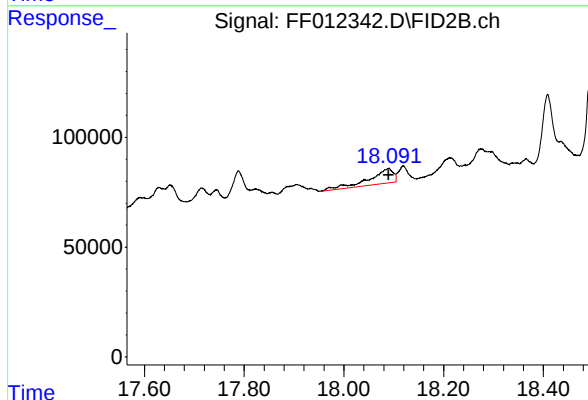


#13 N-TRIACONTANE

R.T.: 18.090 min
Delta R.T.: 0.000 min
Response: 219833
Conc: 2.00 ug/ml

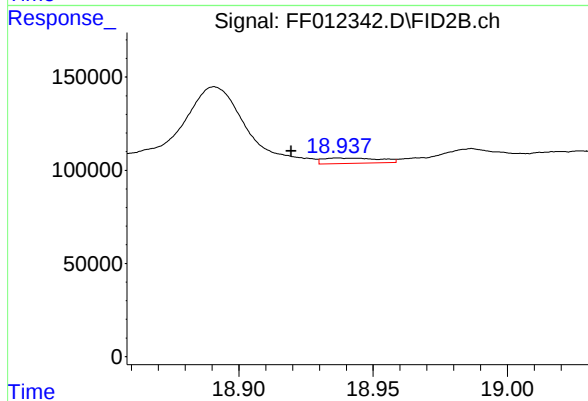

#14 N-DOTRIACONTANE


R.T.: 18.937 min
Delta R.T.: 0.018 min
Response: 41997
Conc: 0.40 ug/ml

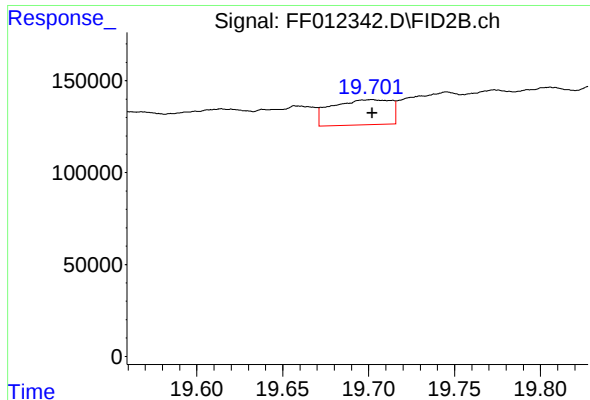

#15 N-TETRATRIACONTANE


R.T.: 19.702 min
Delta R.T.: 0.000 min
Response: 329211
Conc: 3.48 ug/ml

Instrument :
FID_F
ClientSampleId :

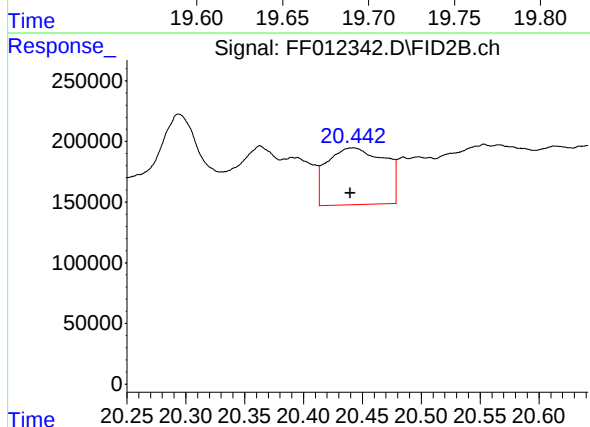

#16 N-HEXATRIACONTANE

R.T.: 20.442 min
Delta R.T.: 0.002 min
Response: 1585971
Conc: 18.10 ug/ml

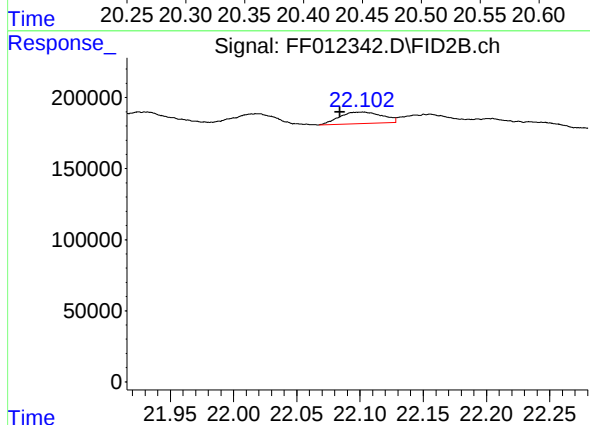

#18 N-TETRACONTANE

R.T.: 22.102 min
Delta R.T.: 0.018 min
Response: 187707
Conc: 2.30 ug/ml