

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032420\
 Data File : FF006655.D
 Signal(s) : FID2B.ch
 Acq On : 24 Mar 2020 10:18
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 25 03:47:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.589	2250746	17.488 ug/ml
Target Compounds			
13) N-TRIACONTANE	17.638	93337	0.659 ug/ml
14) N-DOTRIACONTANE	18.466	104509	0.775 ug/ml
16) N-HEXATRIACONTANE	19.985	48445	0.527 ug/ml
17) N-OCTATRIACONTANE	20.700	396503	5.742 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032420\
Data File : FF006655.D
Signal(s) : FID2B.ch
Acq On : 24 Mar 2020 10:18
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 25 03:47:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

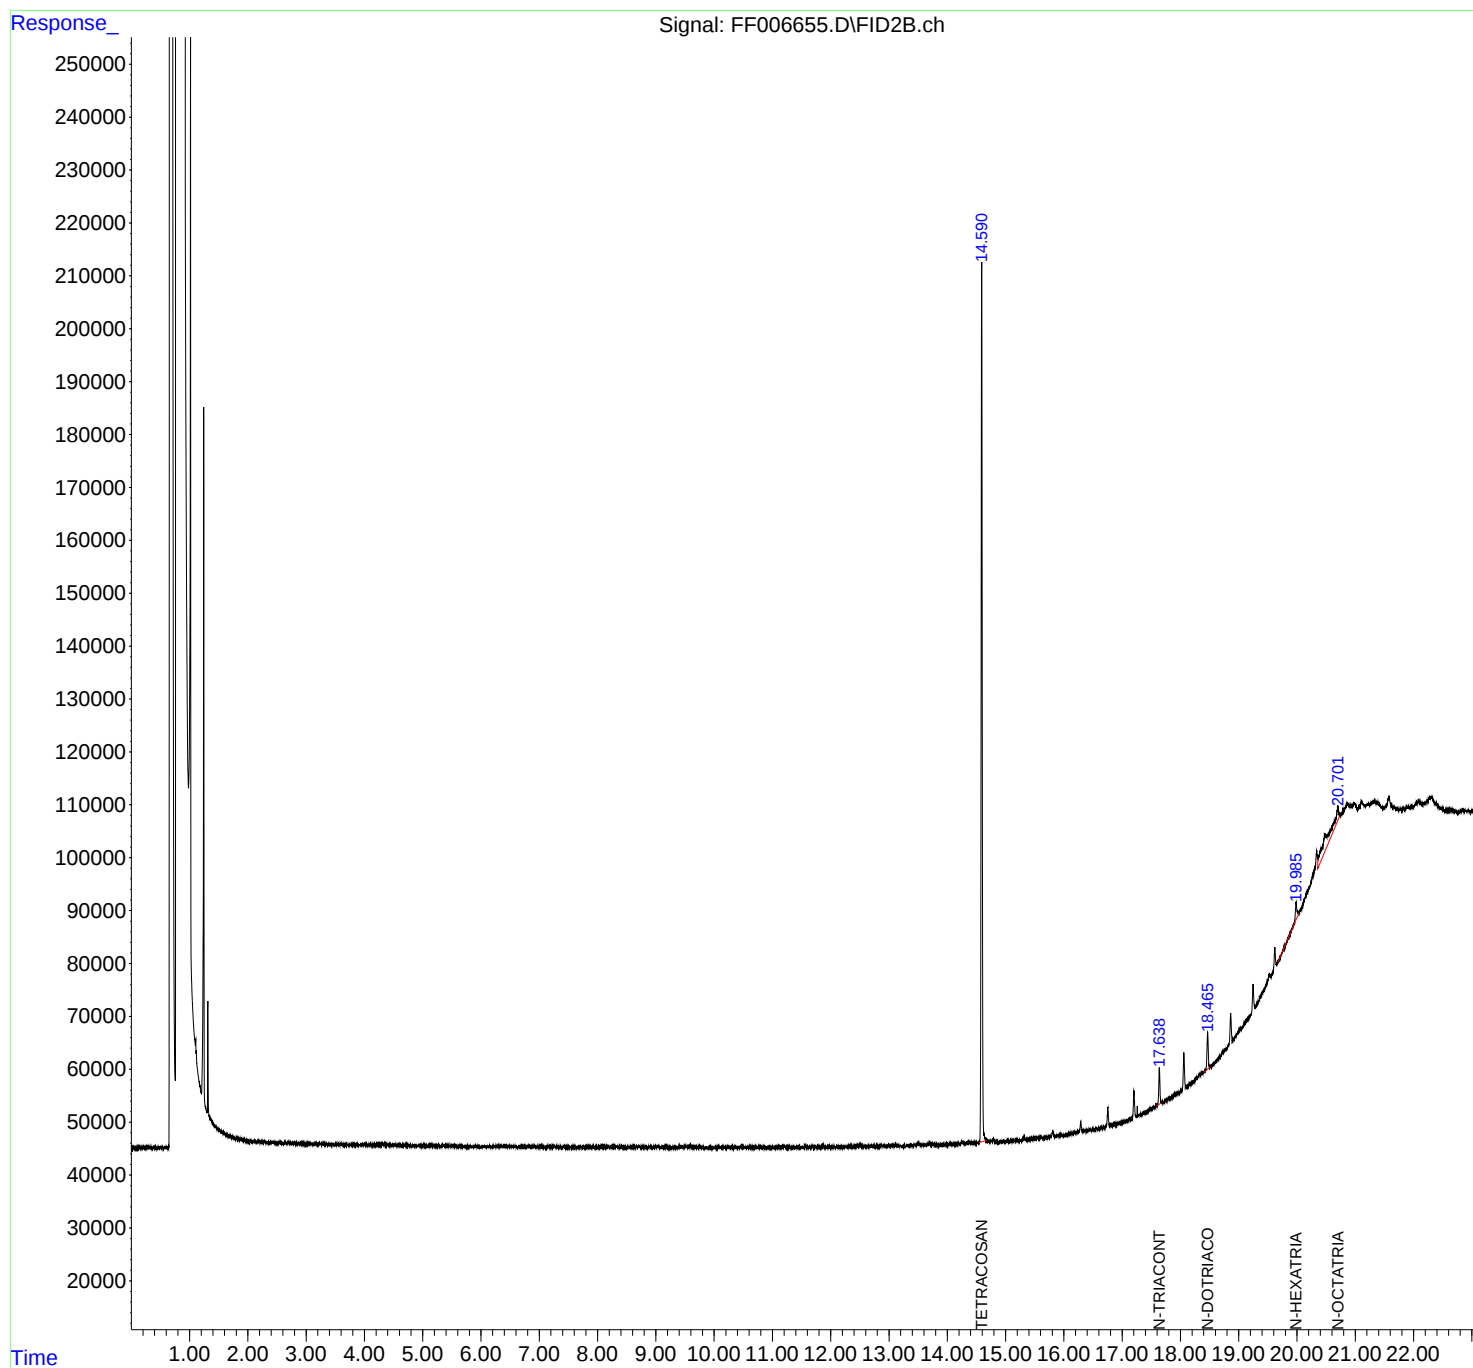

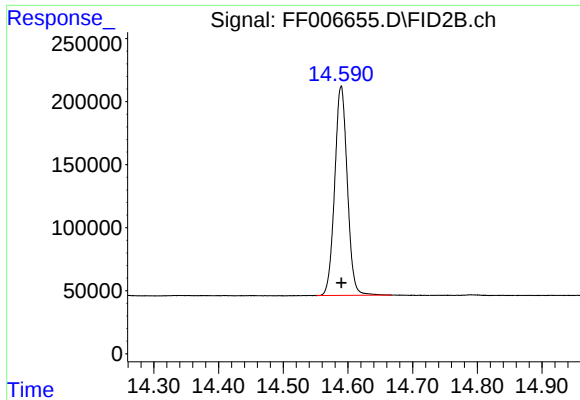


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.589 min
Delta R.T.: 0.000 min
Response: 2250746
Conc: 17.49 ug/ml

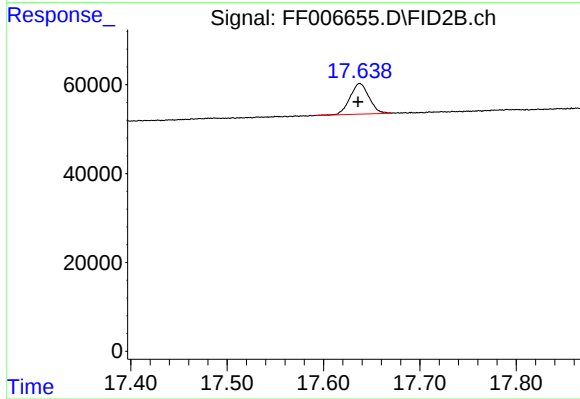


#13 N-TRIACONTANE

R.T.: 17.638 min
Delta R.T.: 0.002 min
Response: 93337
Conc: 0.66 ug/ml

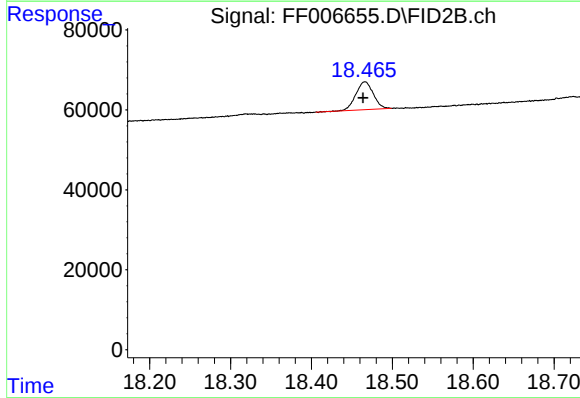


#14 N-DOTRIACONTANE

R.T.: 18.466 min
Delta R.T.: 0.002 min
Response: 104509
Conc: 0.78 ug/ml

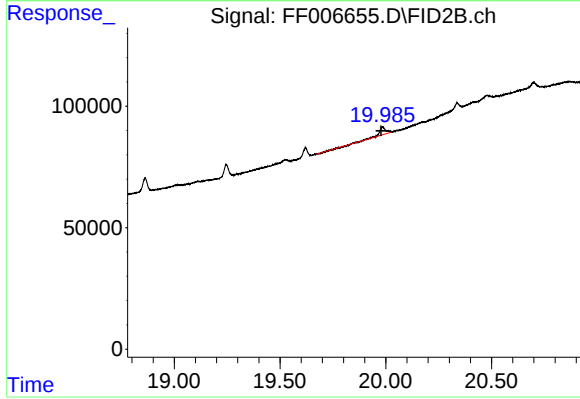

#16 N-HEXATRIACONTANE

R.T.: 19.985 min
Delta R.T.: 0.006 min
Response: 48445
Conc: 0.53 ug/ml

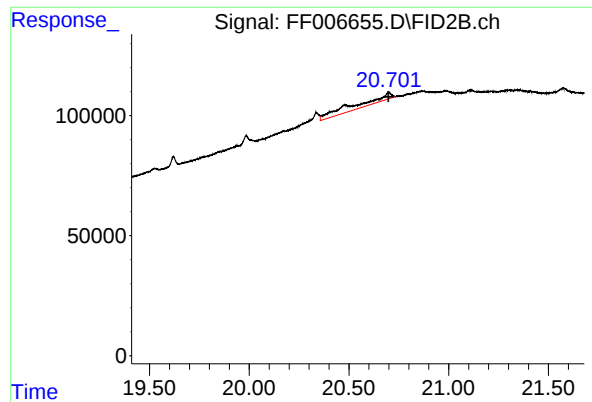

#17 N-OCTATRIACONTANE

R.T.: 20.700 min
Delta R.T.: 0.003 min
Response: 396503
Conc: 5.74 ug/ml