

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032423\
Data File : FF012352.D
Signal(s) : FID2B.ch
Acq On : 24 Mar 2023 15:08
Operator : YP\AJ
Sample : 02058-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CHAMBER-B-72-EAST

Integration File: autoint1.e
Quant Time: Mar 24 17:37:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	15.024	1544327	13.799 ug/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032423\
Data File : FF012352.D
Signal(s) : FID2B.ch
Acq On : 24 Mar 2023 15:08
Operator : YP\AJ
Sample : 02058-01
Misc :
ALS Vial : 63 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :
CHAMBER-B-72-EAST

Integration File: autoint1.e
Quant Time: Mar 24 17:37:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031623.M
Quant Title :
QLast Update : Wed Mar 15 18:07:23 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

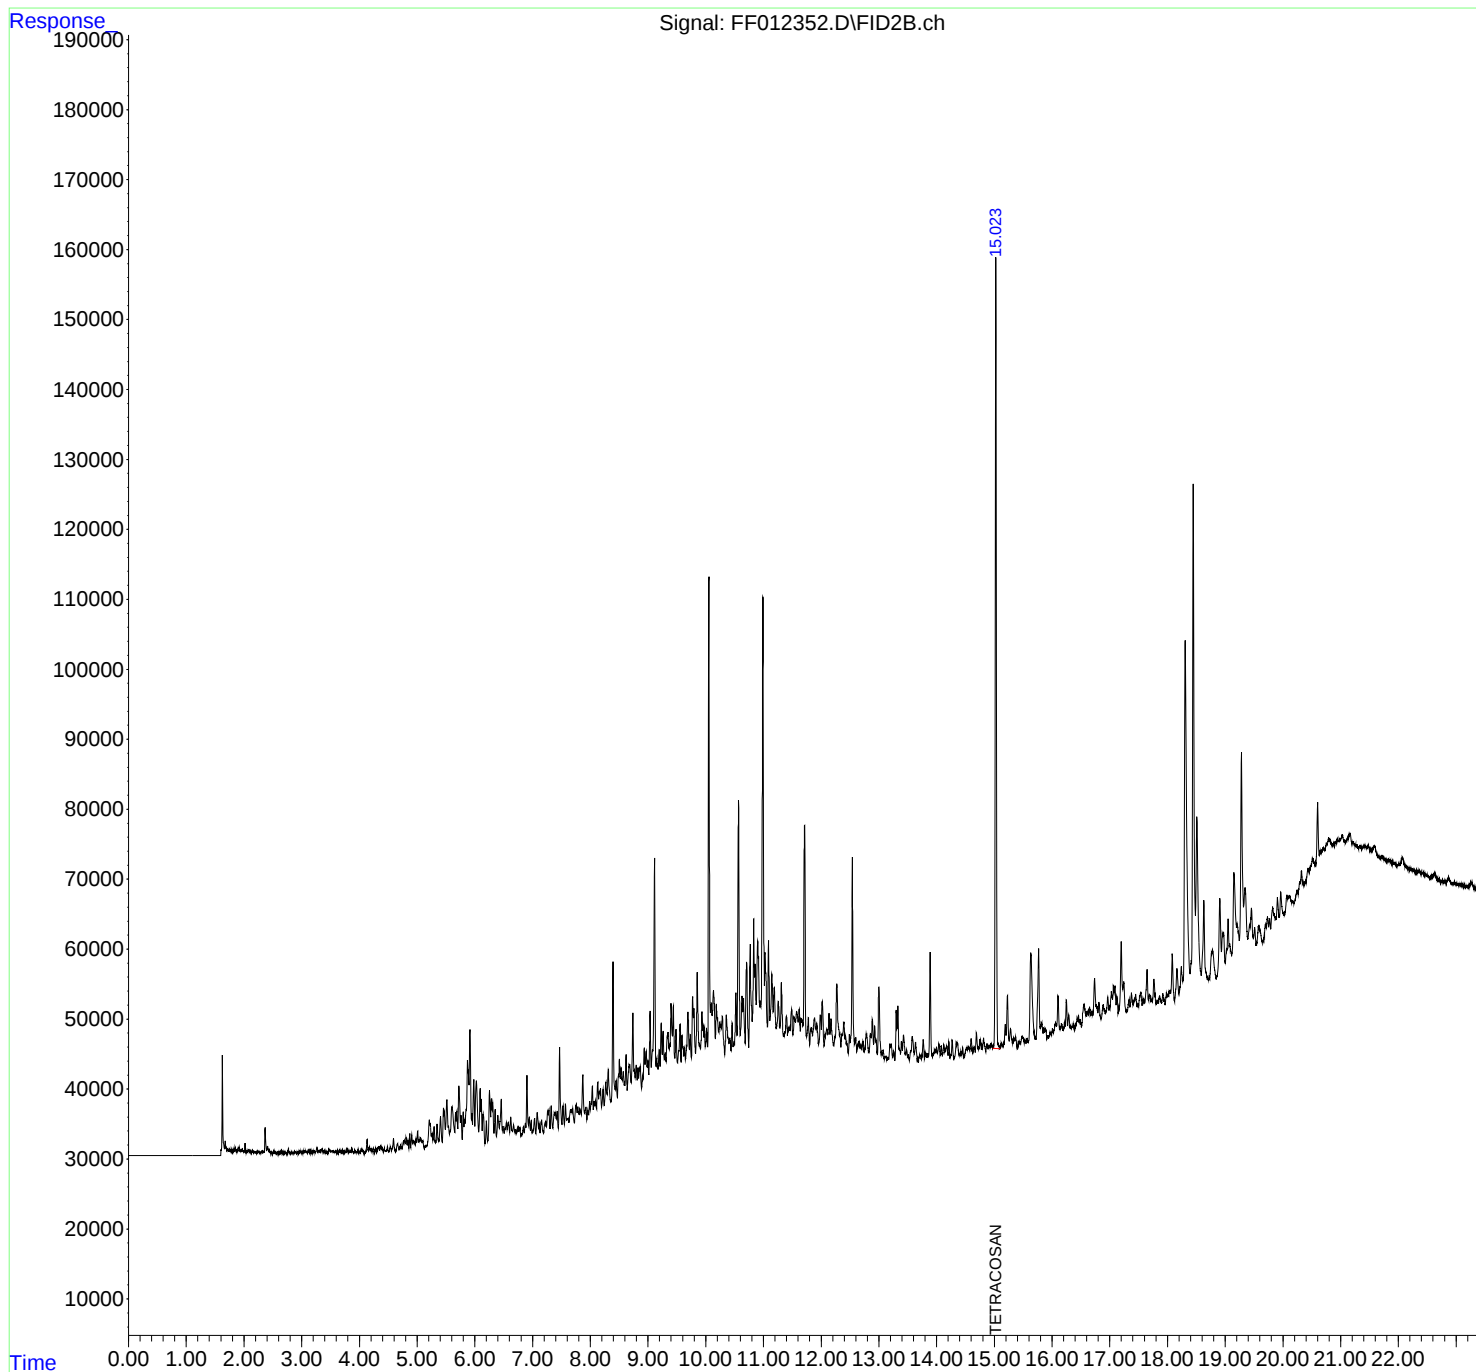

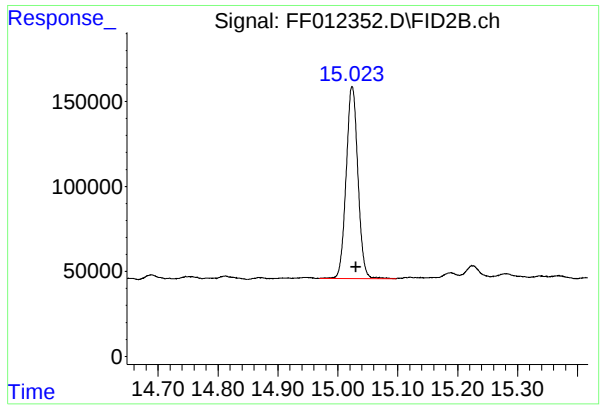

#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 15.024 min
Delta R.T.: -0.006 min
Response: 1544327
Conc: 13.80 ug/ml

Instrument :
FID_F
ClientSampleId :
CHAMBER-B-72-EAST