

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032519\  
Data File : FF003966.D  
Signal(s) : FID2B.ch  
Acq On : 25 Mar 2019 09:26  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Mar 25 15:06:06 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units  |
|-----------------------------|--------|----------|-------------|
| -----                       |        |          |             |
| System Monitoring Compounds |        |          |             |
| Target Compounds            |        |          |             |
| 16) N-HEXATRIACONTANE       | 20.046 | 358303   | 2.746 ug/ml |
| 18) N-TETRACONTANE          | 21.640 | 438992   | 3.529 ug/ml |
| -----                       |        |          |             |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032519\  
Data File : FF003966.D  
Signal(s) : FID2B.ch  
Acq On : 25 Mar 2019 09:26  
Operator : AJ\SJ  
Sample : MECL2  
Misc :  
ALS Vial : 51 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Mar 25 15:06:06 2019  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF030119.M  
Quant Title :  
QLast Update : Mon Mar 04 08:35:38 2019  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

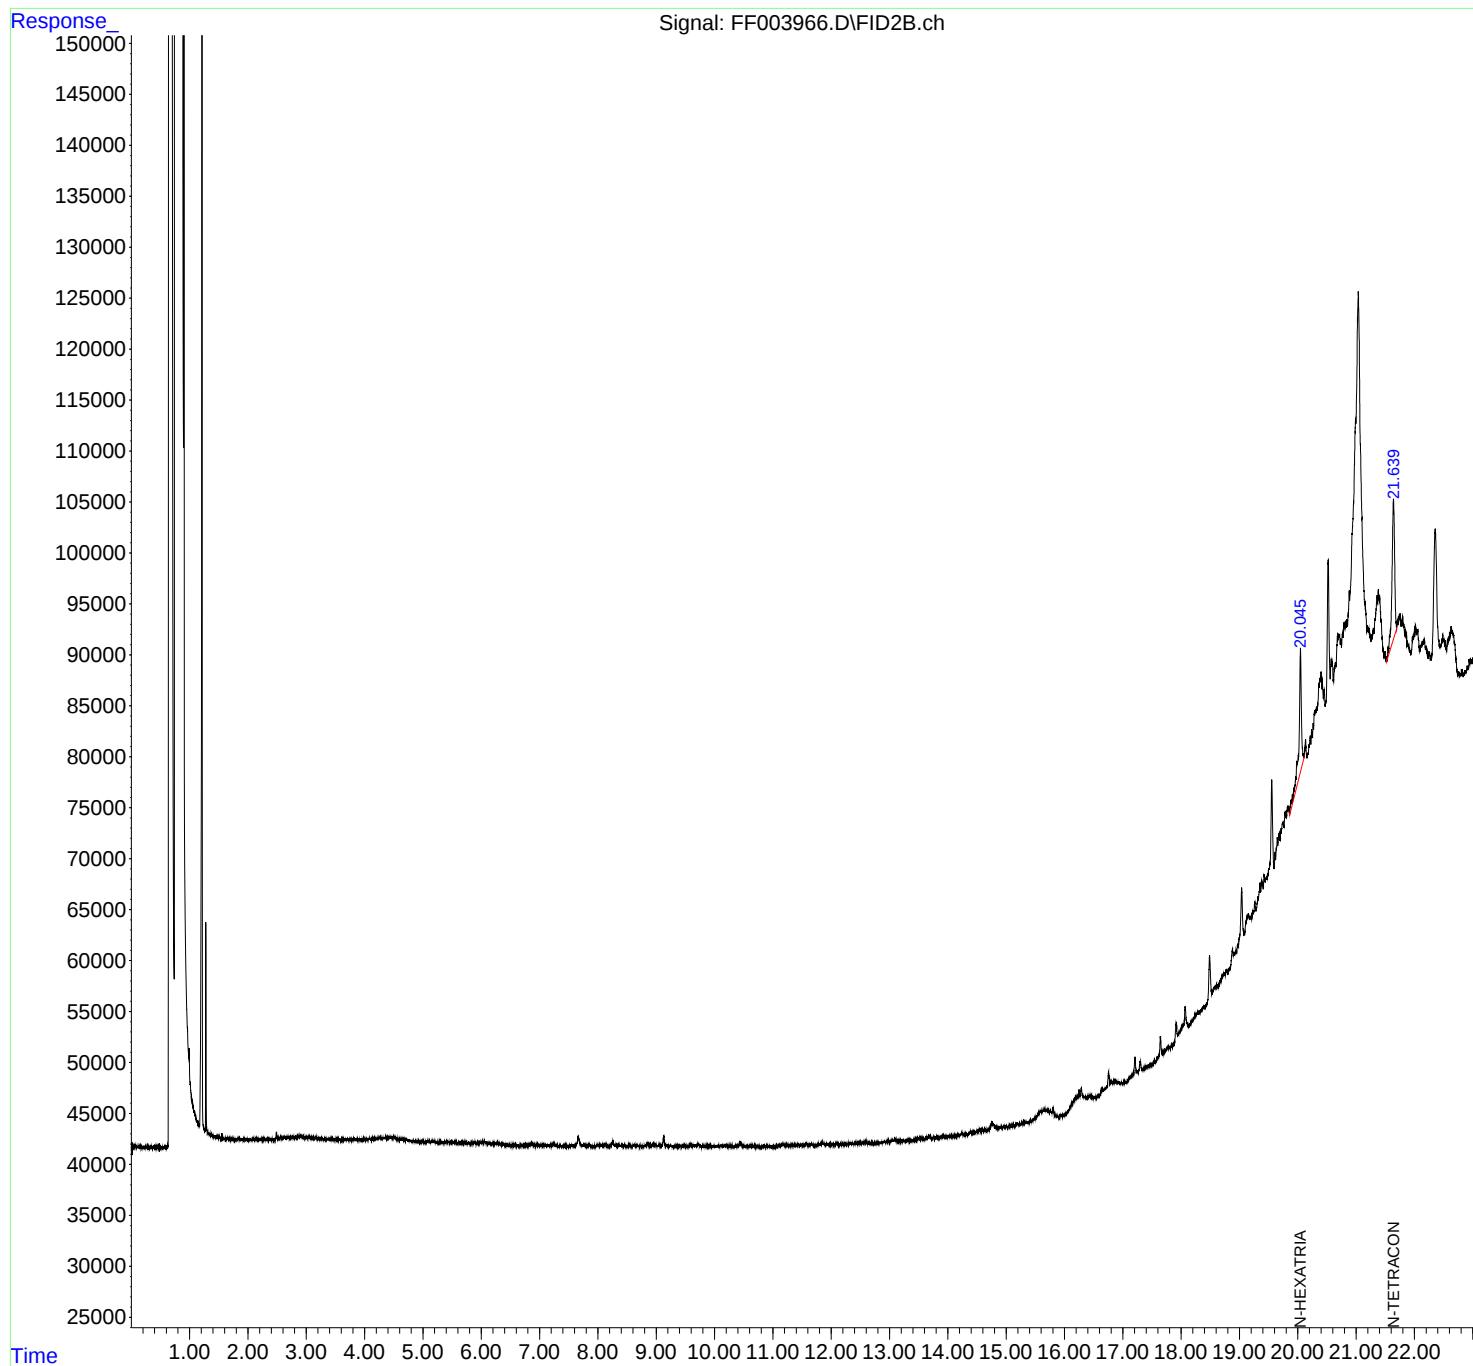

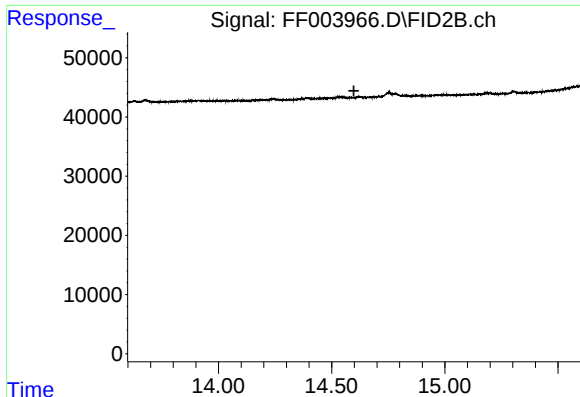


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.598 min  
Response: 0  
Conc: N.D.

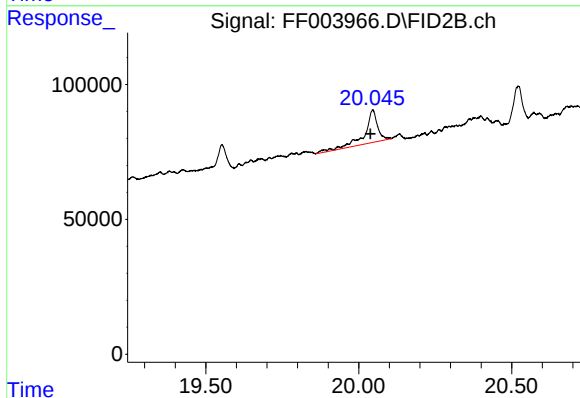

#16 N-HEXATRIACONTANE

R.T.: 20.046 min  
Delta R.T.: 0.008 min  
Response: 358303  
Conc: 2.75 ug/ml

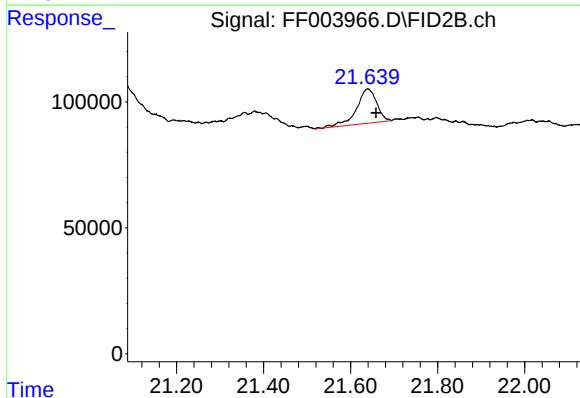

#18 N-TETRACONTANE

R.T.: 21.640 min  
Delta R.T.: -0.019 min  
Response: 438992  
Conc: 3.53 ug/ml