

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
 Data File : FF003983.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2019 14:45
 Operator : AJ\SJ
 Sample : K1693-15 10X
 Misc :
 ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 27 00:59:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.573	277878	1.996 ug/ml
Target Compounds			
7) N-EICOSANE	12.472	134240	0.821 ug/ml
8) N-DOCOSANE	13.699	89407	0.554 ug/ml
10) N-TETRACOSANE	14.755	874149	5.525 ug/ml
11) N-HEXACOSANE	15.801	128441	0.832 ug/ml
12) N-OCTACOSANE	16.767	388886	2.573 ug/ml
13) N-TRIACONTANE	17.639	241255	1.640 ug/ml
14) N-DOTRIACONTANE	18.473	232758	1.637 ug/ml
15) N-TETRATRIACONTANE	19.272	196513	1.468 ug/ml
16) N-HEXATRIACONTANE	20.028	79141	0.607 ug/ml
18) N-TETRACONTANE	21.628	431442	3.468 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
Data File : FF003983.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2019 14:45
Operator : AJ\SJ
Sample : K1693-15 10X
Misc :
ALS Vial : 58 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 00:59:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

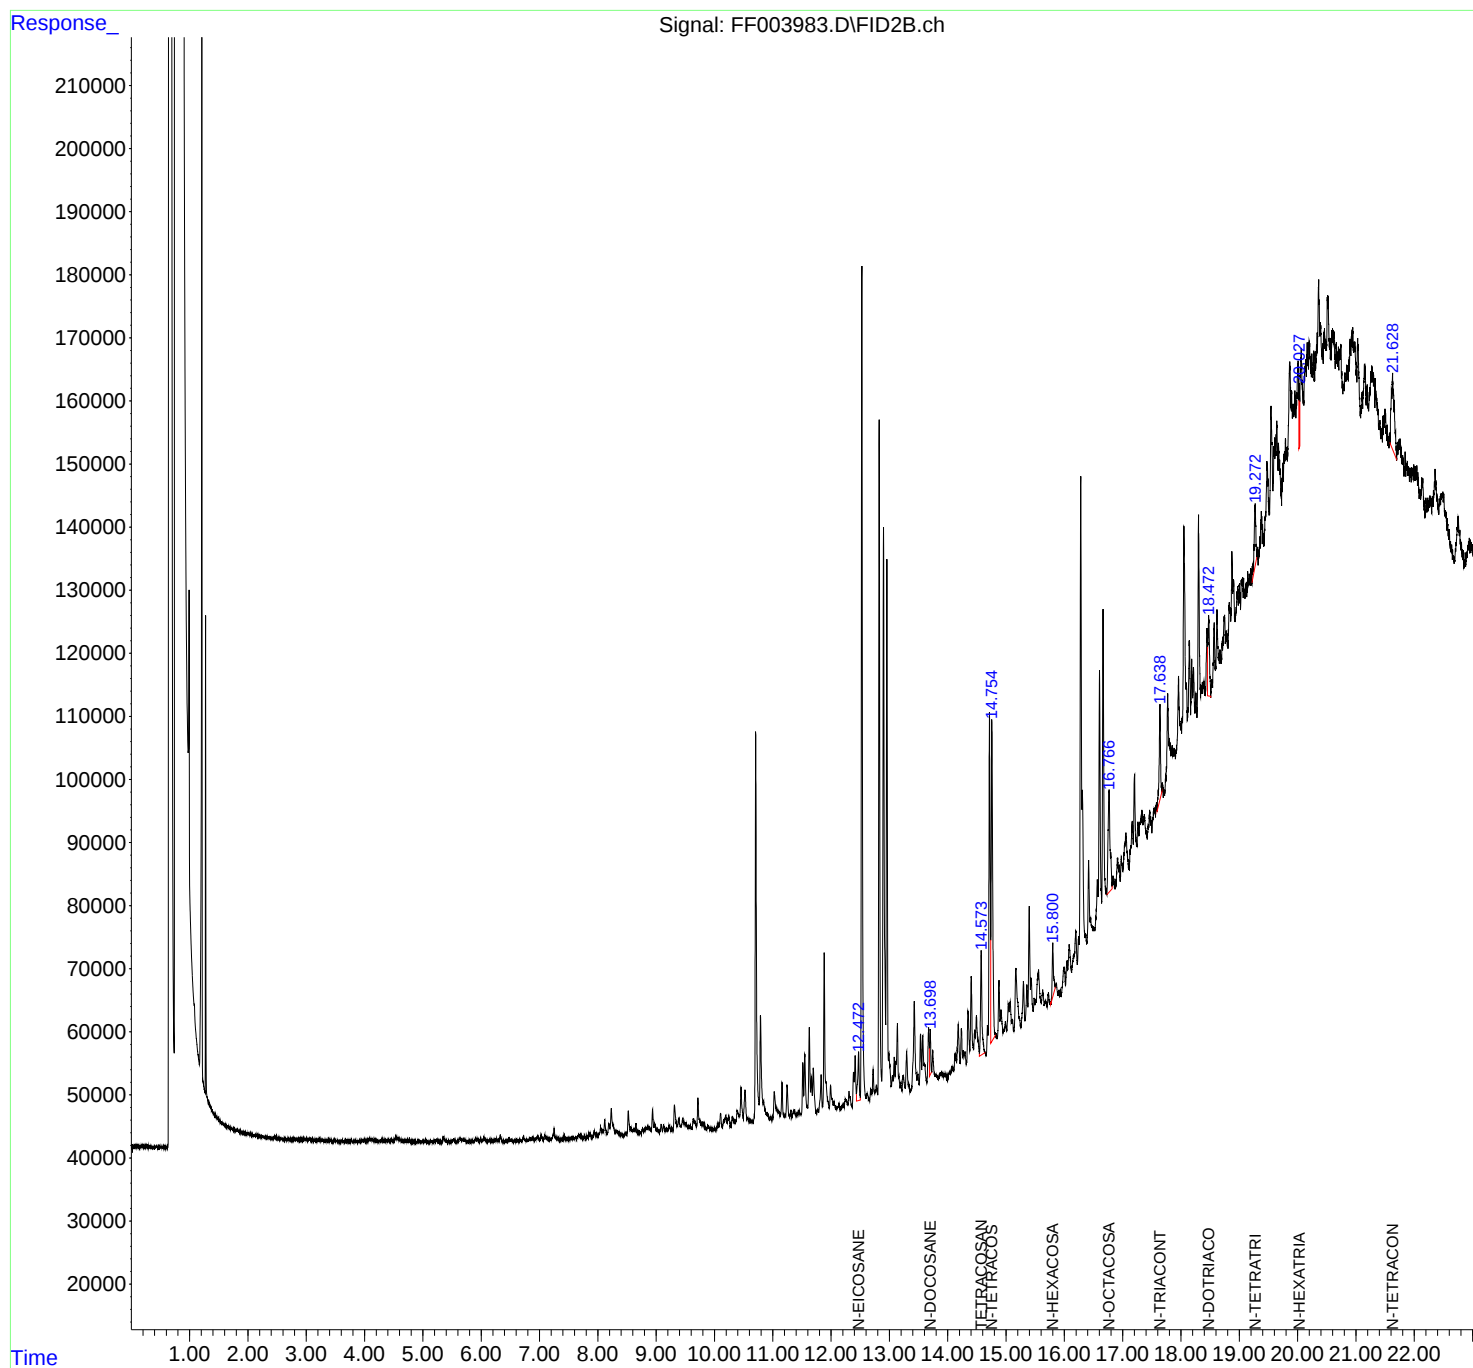

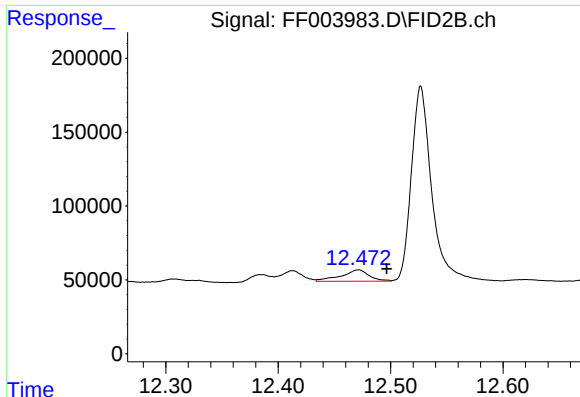


#7 N-EICOSANE

R.T.: 12.472 min
Delta R.T.: -0.025 min
Response: 134240
Conc: 0.82 ug/ml

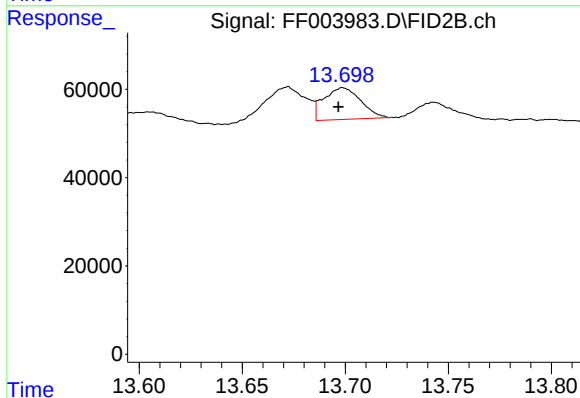


#8 N-DOCOSANE

R.T.: 13.699 min
Delta R.T.: 0.002 min
Response: 89407
Conc: 0.55 ug/ml

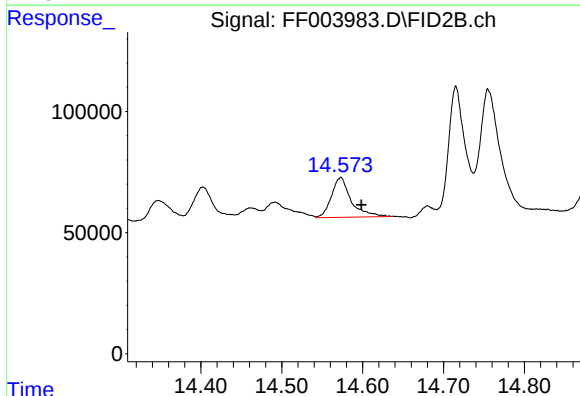


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.573 min
Delta R.T.: -0.025 min
Response: 277878
Conc: 2.00 ug/ml

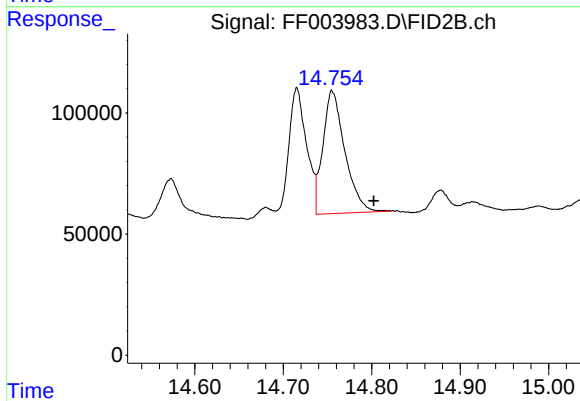


#10 N-TETRACOSANE

R.T.: 14.755 min
Delta R.T.: -0.047 min
Response: 874149
Conc: 5.52 ug/ml

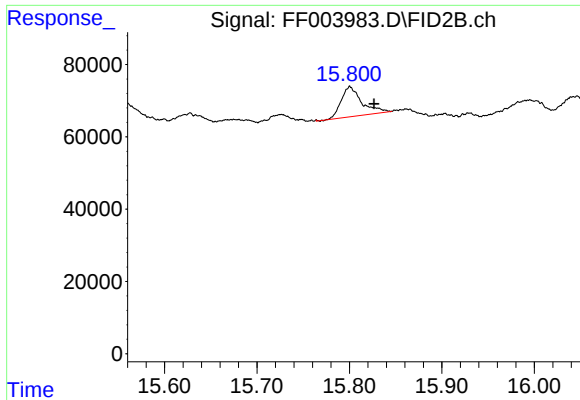


#11 N-HEXACOSANE

R.T.: 15.801 min
Delta R.T.: -0.026 min
Response: 128441
Conc: 0.83 ug/ml

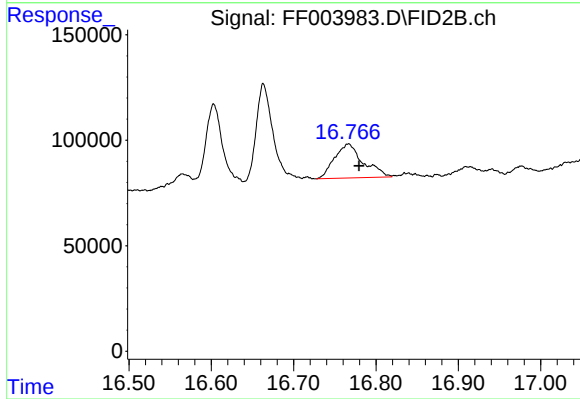


#12 N-OCTACOSANE

R.T.: 16.767 min
Delta R.T.: -0.013 min
Response: 388886
Conc: 2.57 ug/ml

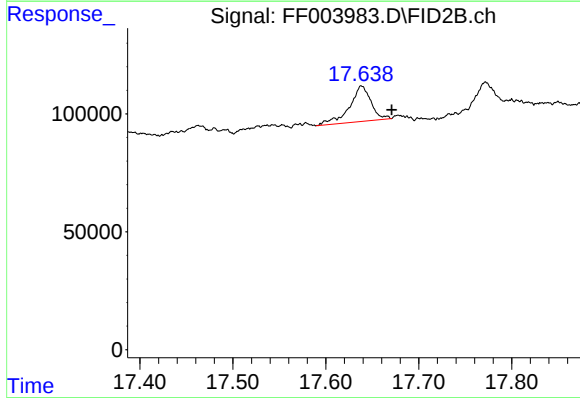


#13 N-TRIACONTANE

R.T.: 17.639 min
Delta R.T.: -0.032 min
Response: 241255
Conc: 1.64 ug/ml

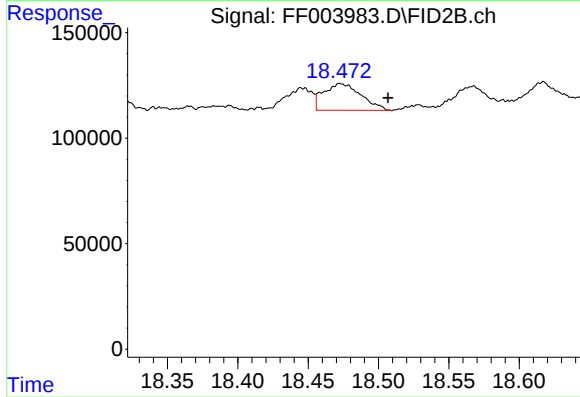

#14 N-DOTRIACONTANE

R.T.: 18.473 min
Delta R.T.: -0.034 min
Response: 232758
Conc: 1.64 ug/ml

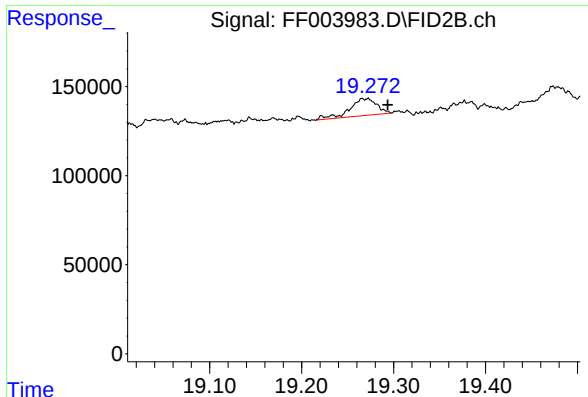


#15 N-TETRATRIACONTANE

R.T.: 19.272 min

Delta R.T.: -0.022 min

Response: 196513

Conc: 1.47 ug/ml

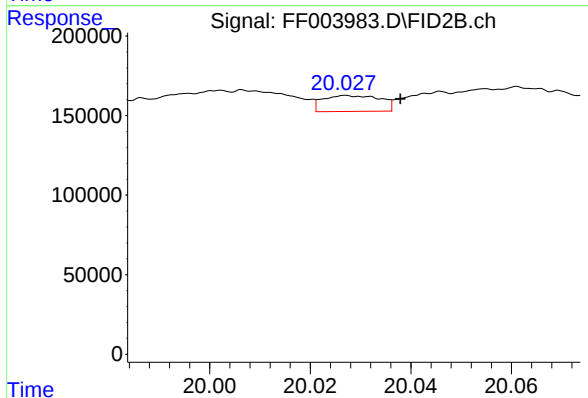


#16 N-HEXATRIACONTANE

R.T.: 20.028 min

Delta R.T.: -0.010 min

Response: 79141

Conc: 0.61 ug/ml

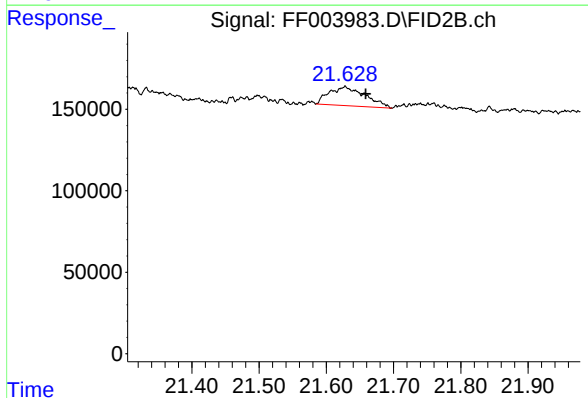

#18 N-TETRACONTANE

R.T.: 21.628 min

Delta R.T.: -0.031 min

Response: 431442

Conc: 3.47 ug/ml