

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
 Data File : FF003986.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2019 16:17
 Operator : AJ\SJ
 Sample : K2061-01
 Misc :
 ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 27 01:00:25 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.573	1912703	13.738 ug/ml
Target Compounds			
4) N-TETRADECANE	8.178	551860	3.442 ug/ml
10) N-TETRACOSANE	14.775	143703	0.908 ug/ml
11) N-HEXACOSANE	15.799	406617	2.635 ug/ml
12) N-OCTACOSANE	16.751	913600	6.046 ug/ml
13) N-TRIACONTANE	17.640	1115893	7.586 ug/ml
14) N-DOTRIACONTANE	18.474	774410	5.446 ug/ml
15) N-TETRATRIACONTANE	19.262	146927	1.097 ug/ml
16) N-HEXATRIACONTANE	20.041	309932	2.375 ug/ml
18) N-TETRACONTANE	21.639	560337	4.504 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
Data File : FF003986.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2019 16:17
Operator : AJ\SJ
Sample : K2061-01
Misc :
ALS Vial : 61 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 01:00:25 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

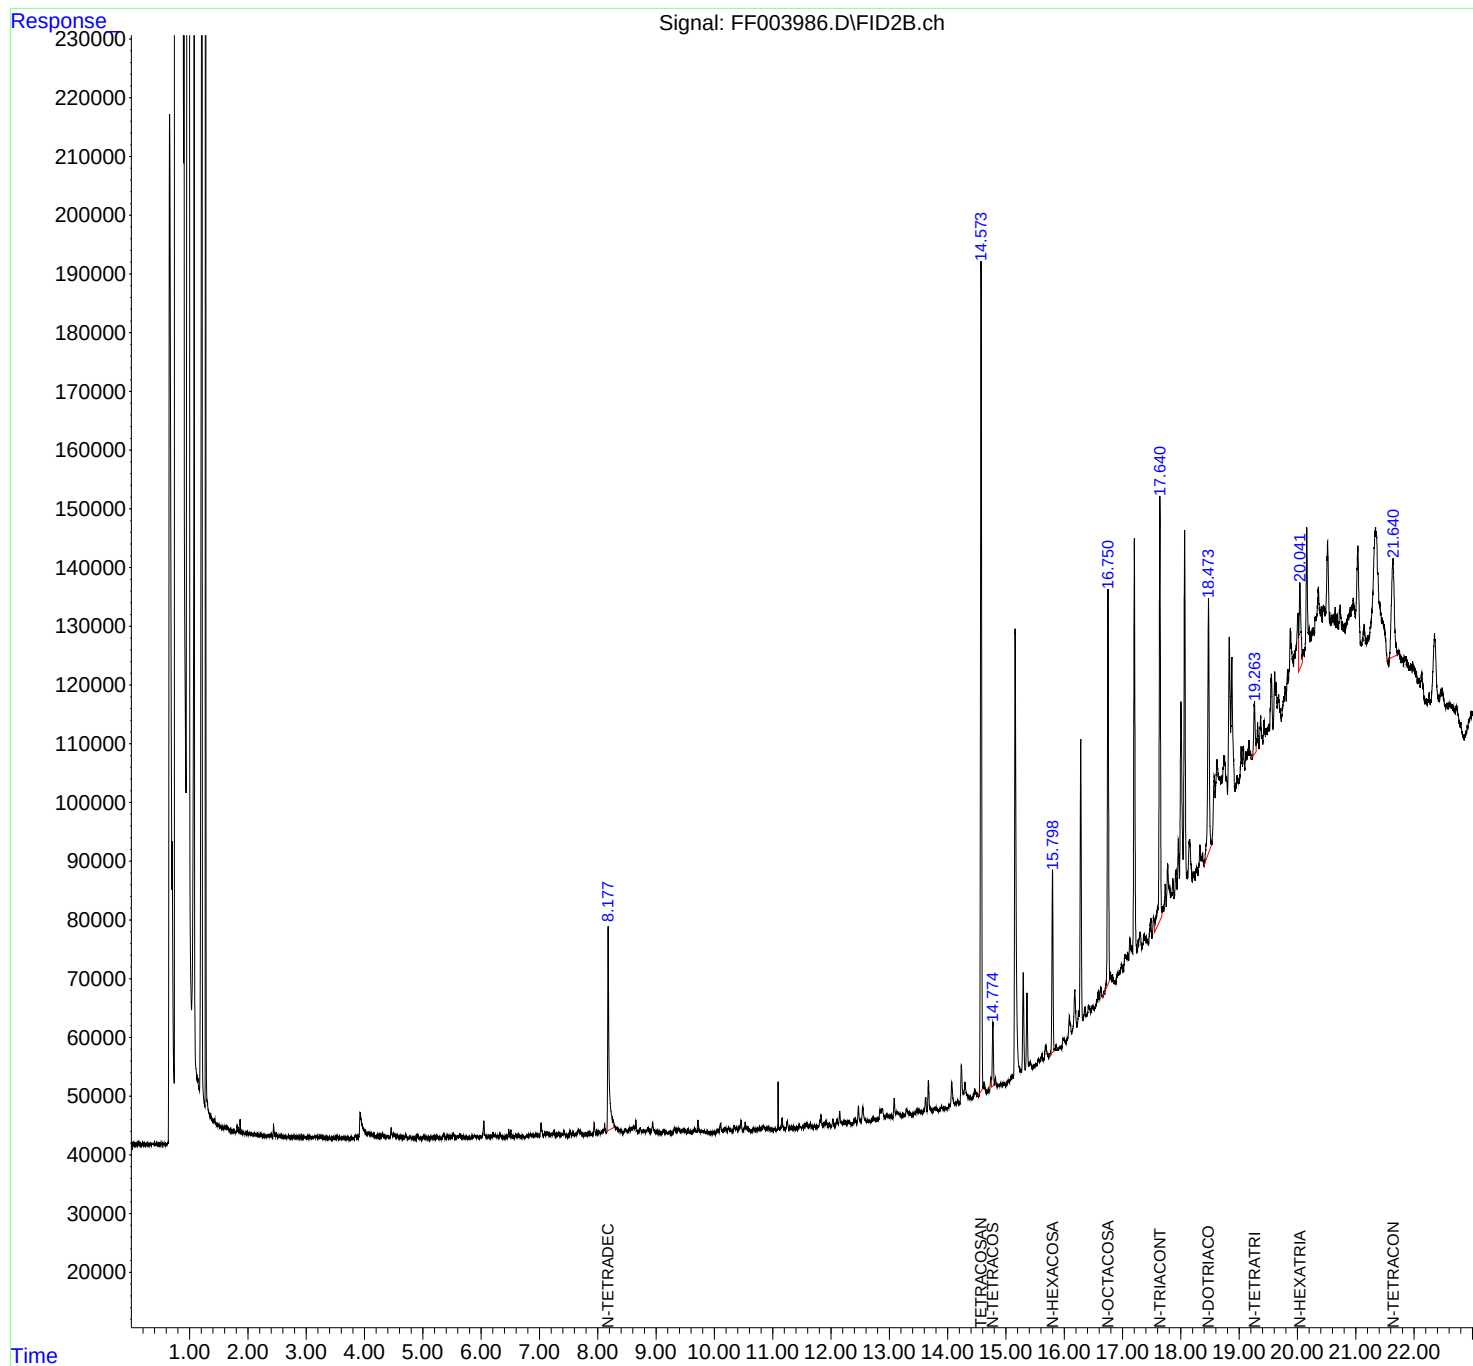

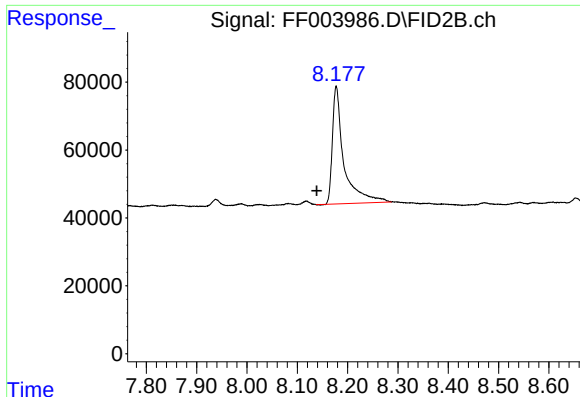


#4 N-TETRADECANE

R.T.: 8.178 min
Delta R.T.: 0.039 min
Response: 551860
Conc: 3.44 ug/ml

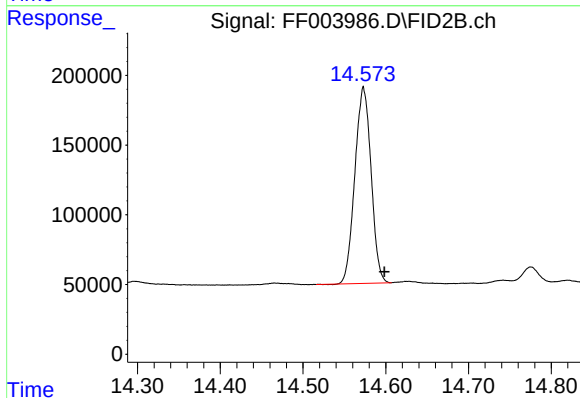


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.573 min
Delta R.T.: -0.025 min
Response: 1912703
Conc: 13.74 ug/ml

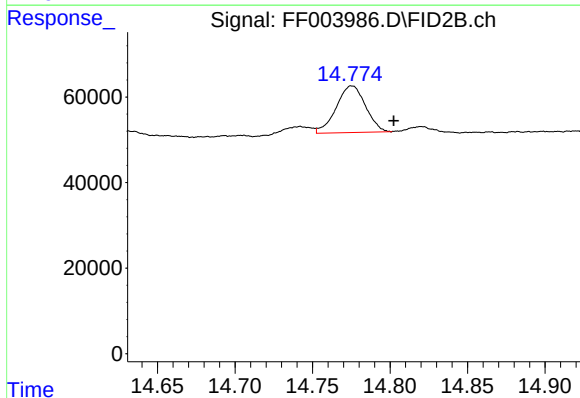


#10 N-TETRACOSANE

R.T.: 14.775 min
Delta R.T.: -0.027 min
Response: 143703
Conc: 0.91 ug/ml

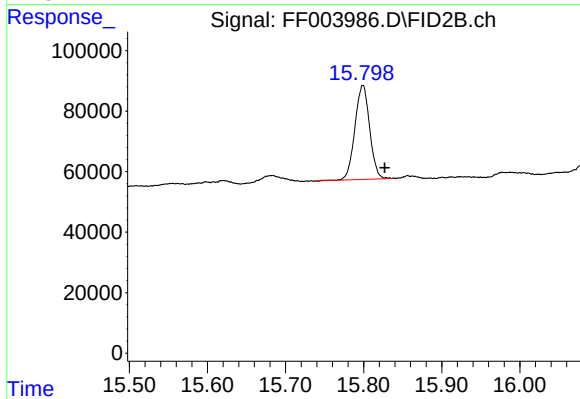


#11 N-HEXACOSANE

R.T.: 15.799 min
Delta R.T.: -0.028 min
Response: 406617
Conc: 2.63 ug/ml

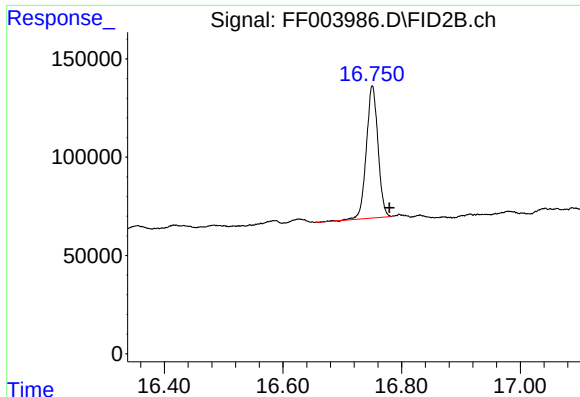


#12 N-OCTACOSANE

R.T.: 16.751 min
Delta R.T.: -0.029 min
Response: 913600
Conc: 6.05 ug/ml

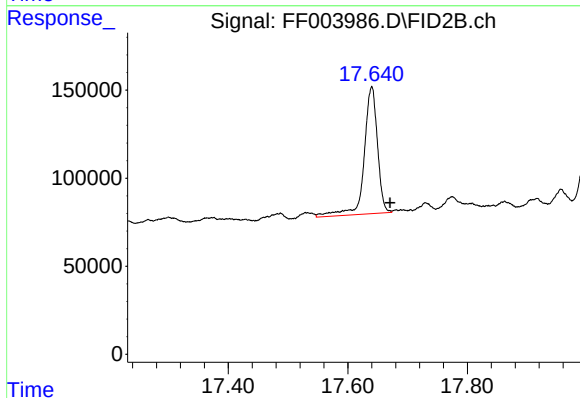


#13 N-TRIACONTANE

R.T.: 17.640 min
Delta R.T.: -0.031 min
Response: 1115893
Conc: 7.59 ug/ml

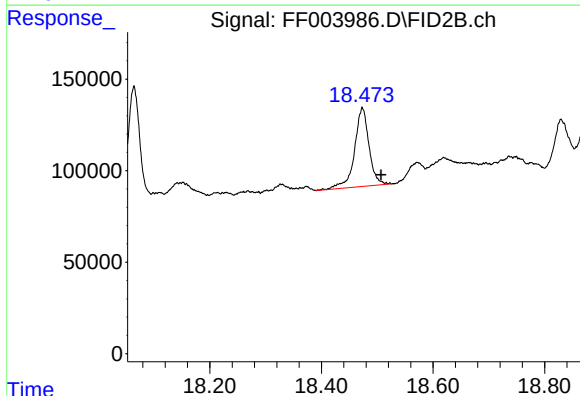


#14 N-DOTRIACONTANE

R.T.: 18.474 min
Delta R.T.: -0.033 min
Response: 774410
Conc: 5.45 ug/ml

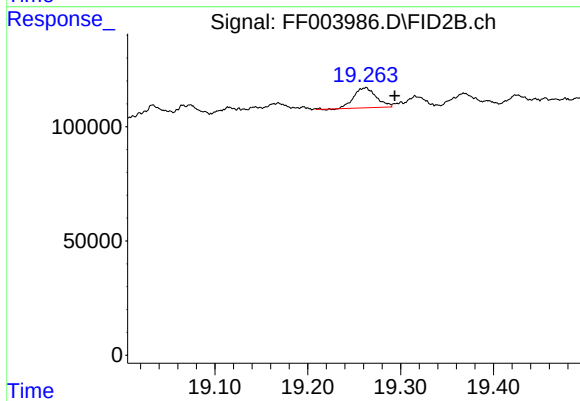


#15 N-TETRATRIACONTANE

R.T.: 19.262 min
Delta R.T.: -0.031 min
Response: 146927
Conc: 1.10 ug/ml

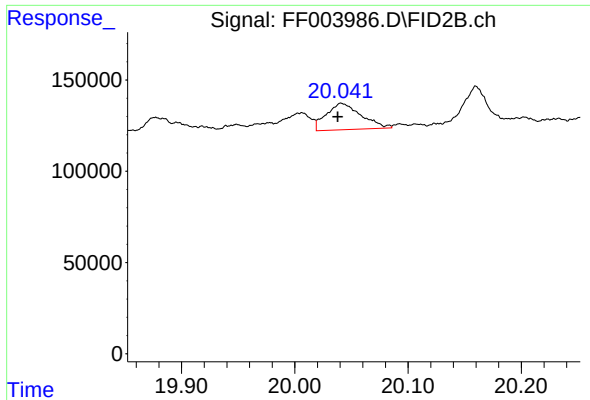

#16 N-HEXATRIACONTANE

R.T.: 20.041 min
Delta R.T.: 0.003 min
Response: 309932
Conc: 2.38 ug/ml

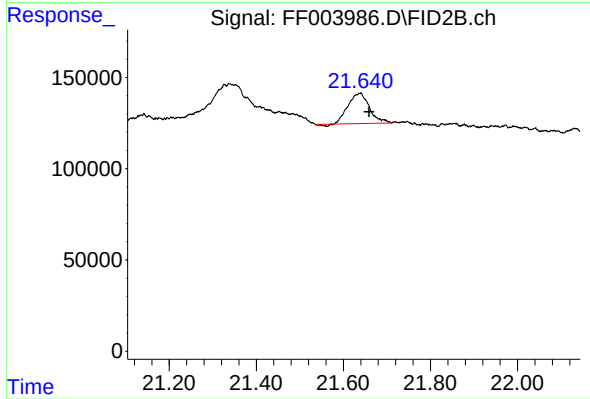

#18 N-TETRACONTANE

R.T.: 21.639 min
Delta R.T.: -0.020 min
Response: 560337
Conc: 4.50 ug/ml