

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
 Data File : FF003991.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2019 18:50
 Operator : AJ\SJ
 Sample : K2091-01 20X
 Misc :
 ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 27 01:01:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.575	111518	0.801 ug/ml
Target Compounds			
6) N-OCTADECANE	11.251f	199148	1.209 ug/ml
13) N-TRIACONTANE	17.639	71942	0.489 ug/ml
14) N-DOTRIACONTANE	18.475	198483	1.396 ug/ml
15) N-TETRATRIACONTANE	19.304	125069	0.934 ug/ml
16) N-HEXATRIACONTANE	20.039	543795	4.168 ug/ml
17) N-OCTATRIACONTANE	20.775	149581	1.295 ug/ml
18) N-TETRACONTANE	21.629	313780	2.522 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
Data File : FF003991.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2019 18:50
Operator : AJ\SJ
Sample : K2091-01 20X
Misc :
ALS Vial : 66 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 01:01:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

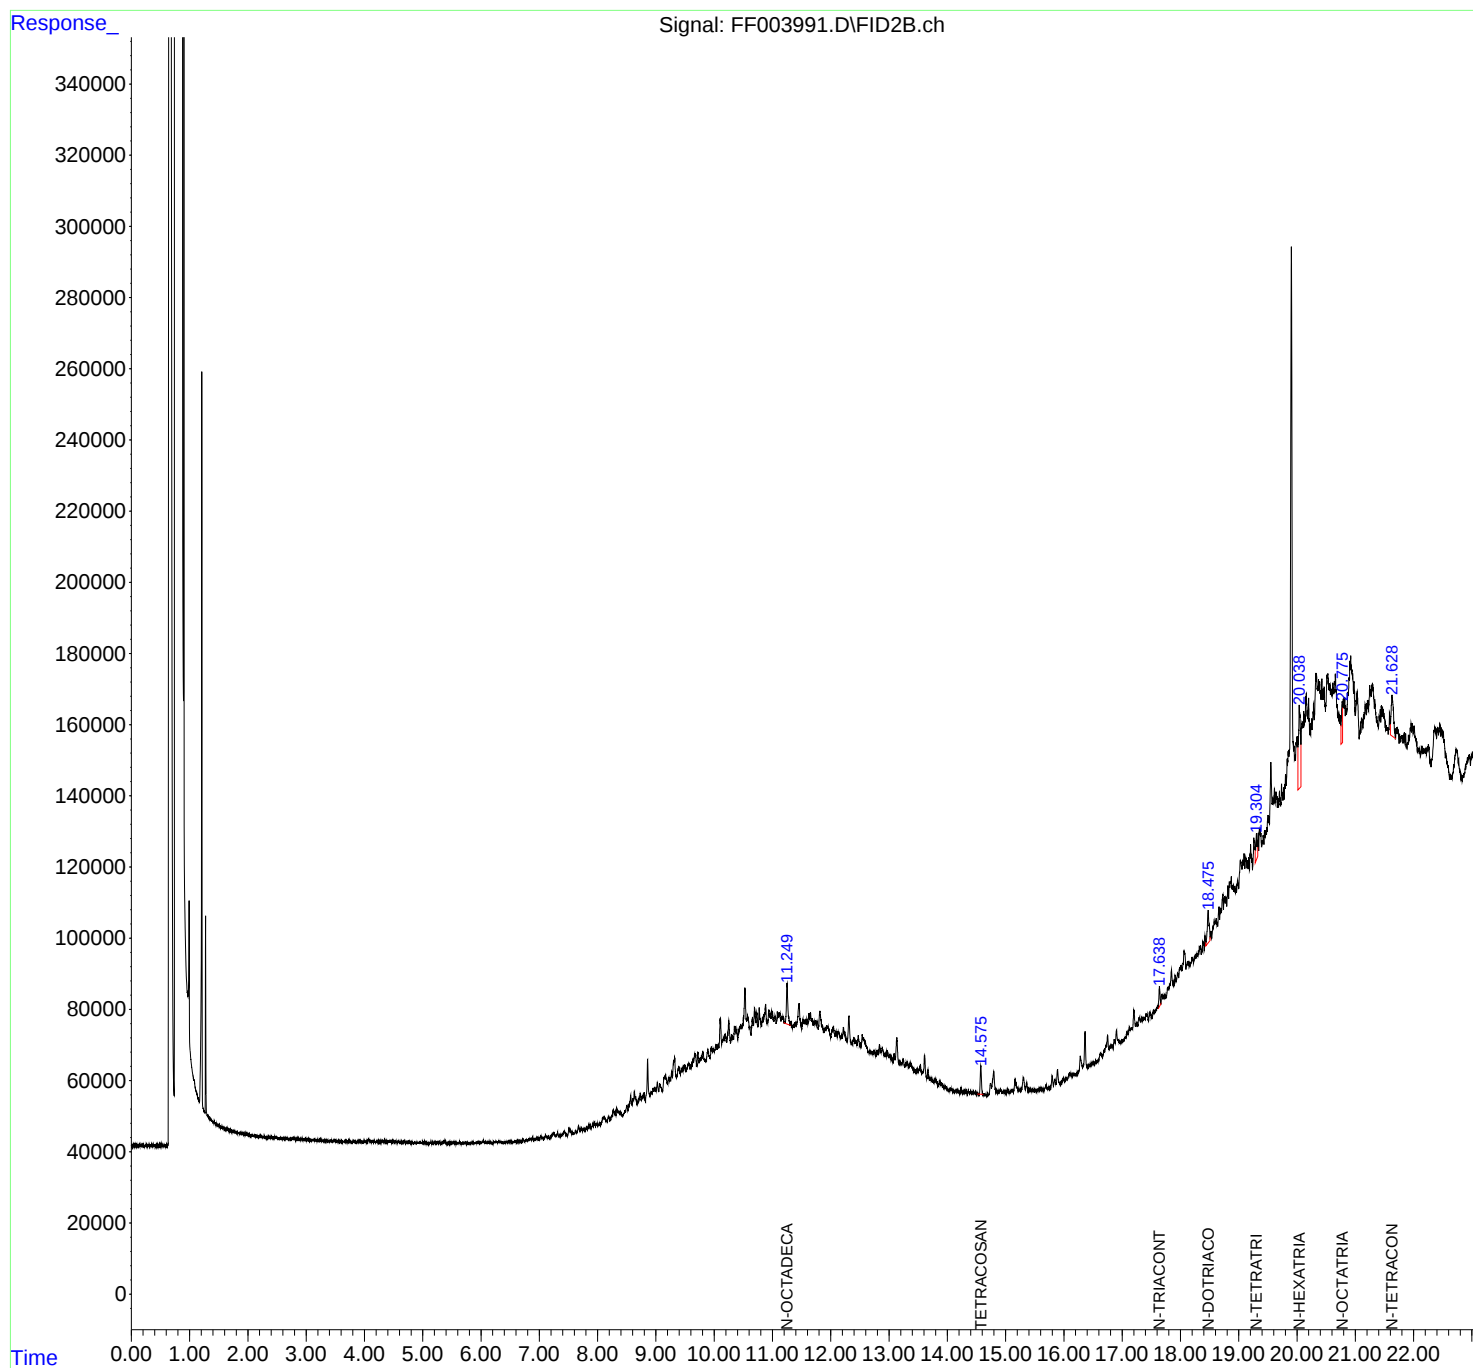

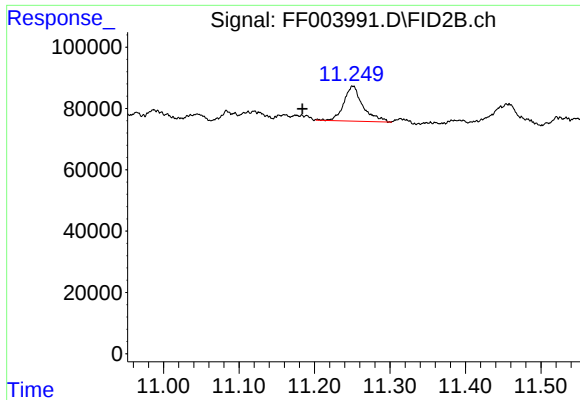


#6 N-OCTADECANE

R.T.: 11.251 min
Delta R.T.: 0.067 min
Response: 199148
Conc: 1.21 ug/ml

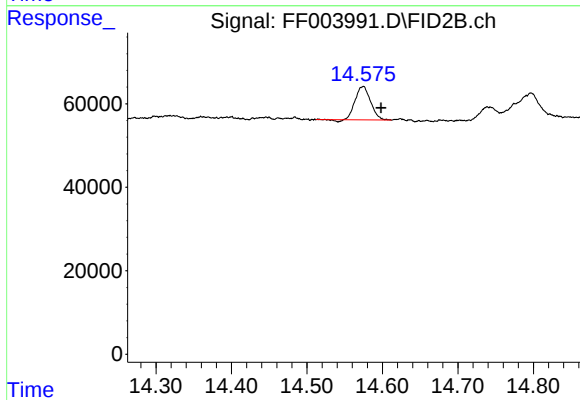


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.575 min
Delta R.T.: -0.024 min
Response: 111518
Conc: 0.80 ug/ml

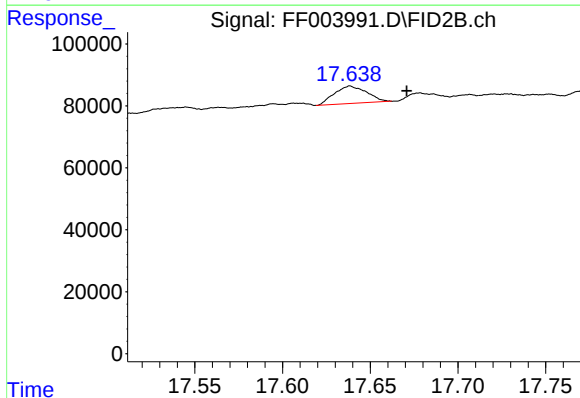


#13 N-TRIACONTANE

R.T.: 17.639 min
Delta R.T.: -0.032 min
Response: 71942
Conc: 0.49 ug/ml

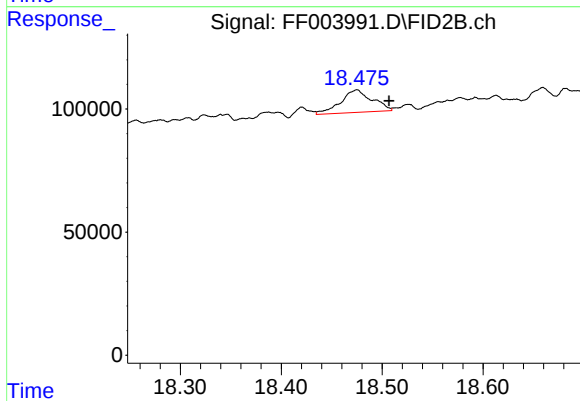

#14 N-DOTRIACONTANE

R.T.: 18.475 min
Delta R.T.: -0.032 min
Response: 198483
Conc: 1.40 ug/ml

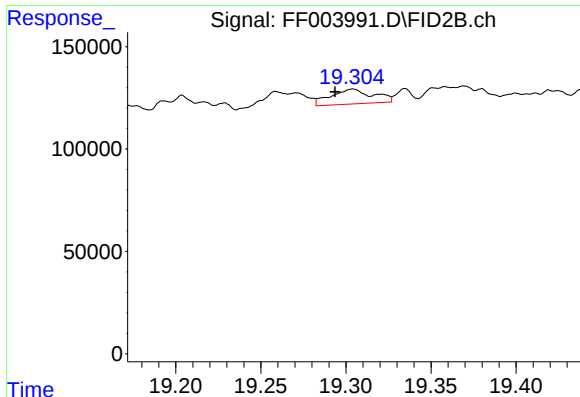


#15 N-TETRATRIACONTANE

R.T.: 19.304 min

Delta R.T.: 0.010 min

Response: 125069

Conc: 0.93 ug/ml

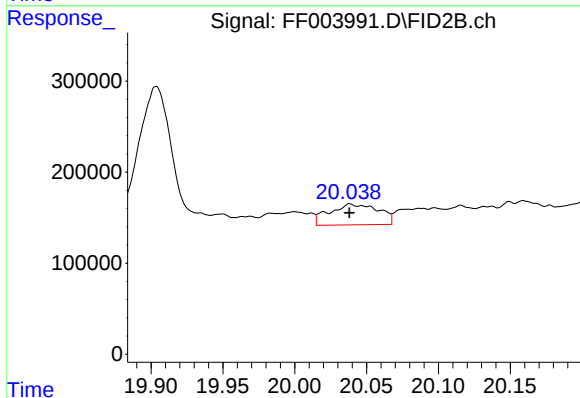


#16 N-HEXATRIACONTANE

R.T.: 20.039 min

Delta R.T.: 0.000 min

Response: 543795

Conc: 4.17 ug/ml

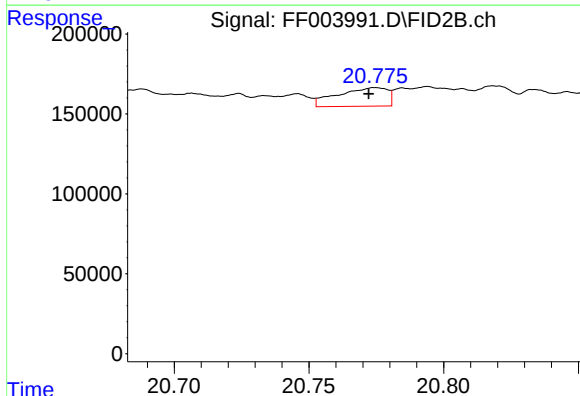


#17 N-OCTATRIACONTANE

R.T.: 20.775 min

Delta R.T.: 0.003 min

Response: 149581

Conc: 1.30 ug/ml

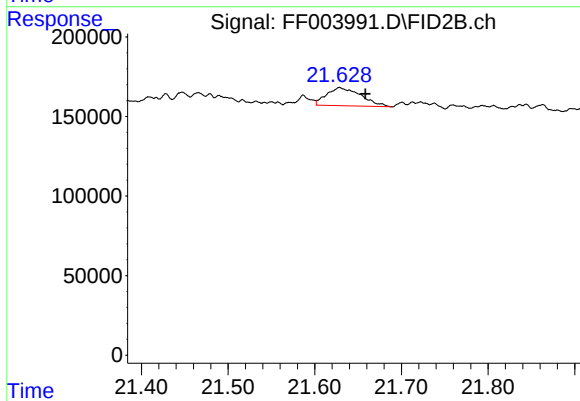

#18 N-TETRACONTANE

R.T.: 21.629 min

Delta R.T.: -0.030 min

Response: 313780

Conc: 2.52 ug/ml