

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
 Data File : FF003981.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2019 13:43
 Operator : AJ\SJ
 Sample : PB118272BS
 Misc :
 ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 27 00:59:01 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.571	1920888	13.797 ug/ml
Target Compounds			
2) N-DECANE	4.302	2564667	16.673 ug/ml
3) N-DODECANE	6.322	2640350	16.918 ug/ml
4) N-TETRADECANE	8.116	2627515	16.388 ug/ml
5) N-HEXADECANE	9.716	2599844	15.963 ug/ml
6) N-OCTADECANE	11.159	2557210	15.521 ug/ml
7) N-EICOSANE	12.470	2480211	15.161 ug/ml
8) N-DOCOSANE	13.670	2415042	14.964 ug/ml
10) N-TETRACOSANE	14.775	2361098	14.923 ug/ml
11) N-HEXACOSANE	15.798	2305221	14.936 ug/ml
12) N-OCTACOSANE	16.751	2286576	15.131 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
Data File : FF003981.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2019 13:43
Operator : AJ\SJ
Sample : PB118272BS
Misc :
ALS Vial : 56 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 00:59:01 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

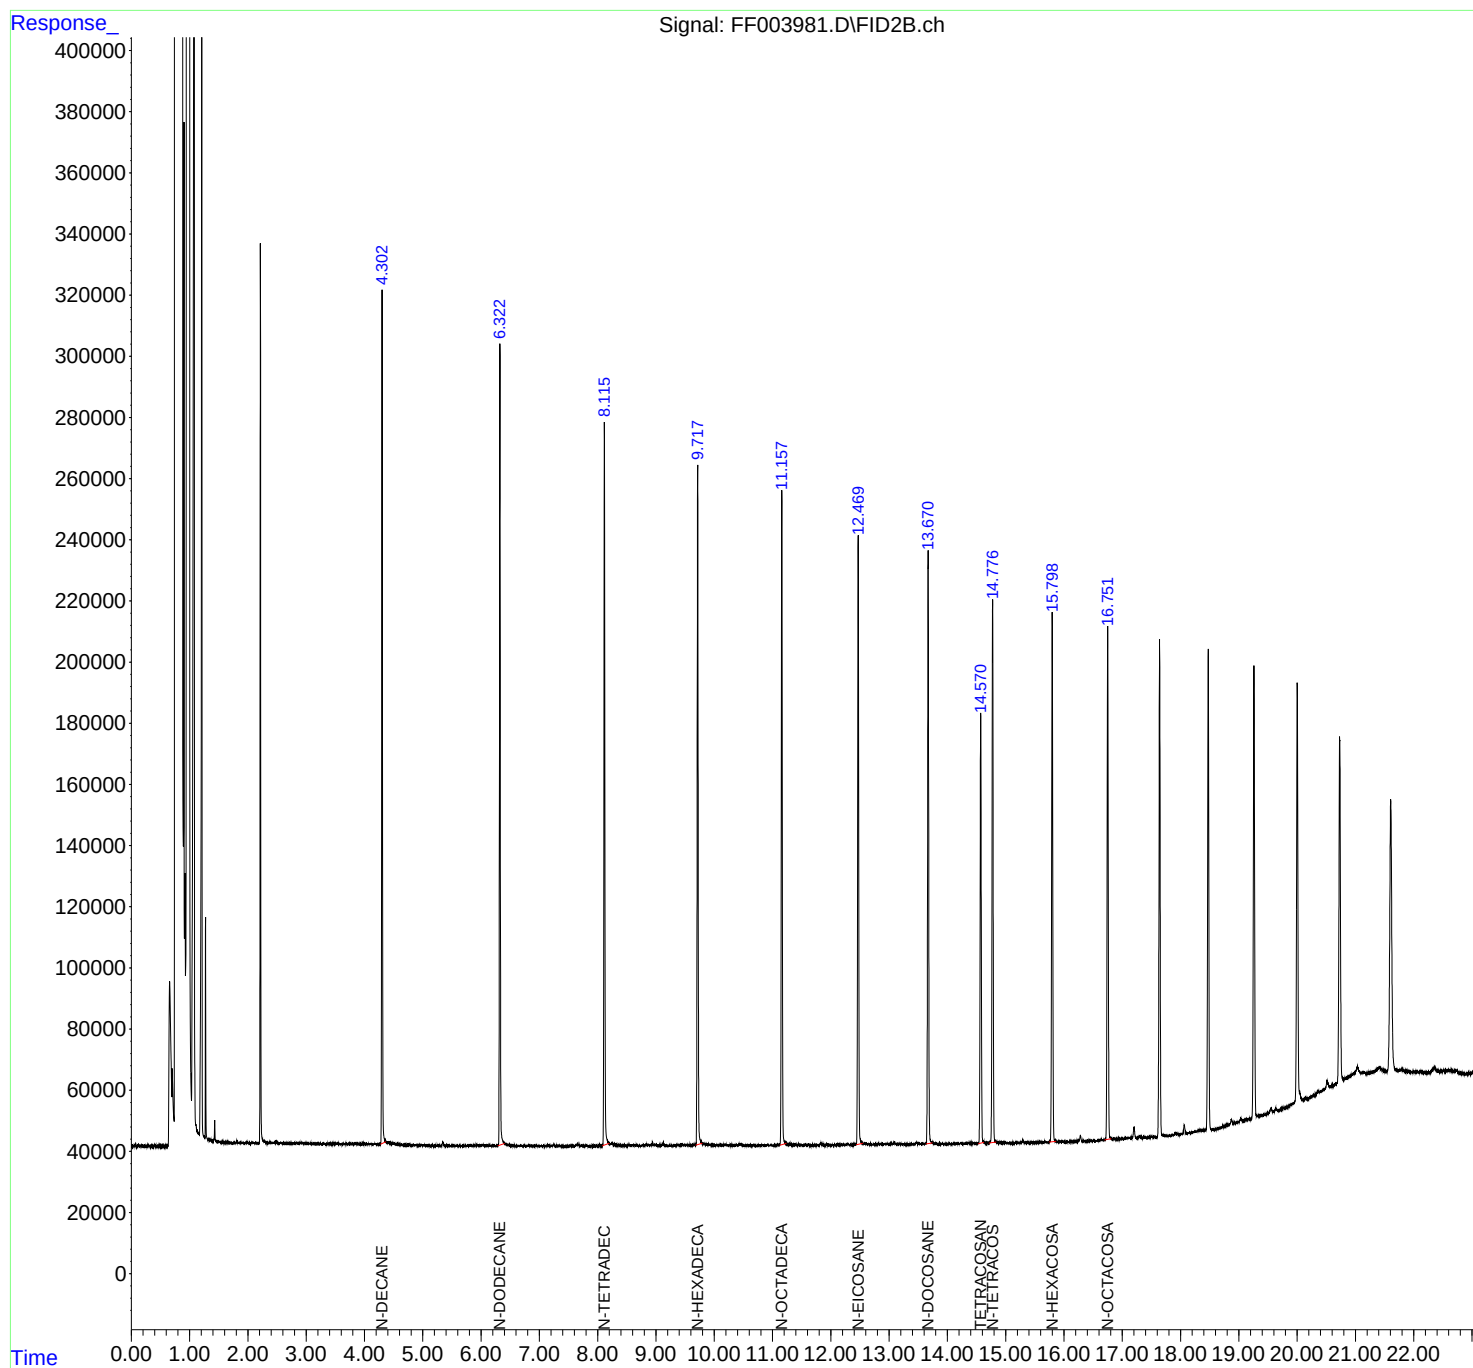

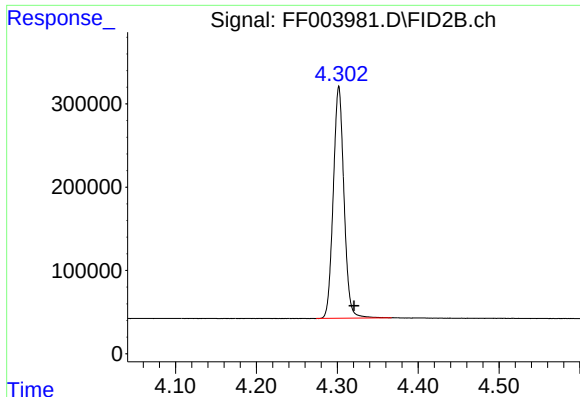


#2 N-DECANE

R.T.: 4.302 min
Delta R.T.: -0.019 min
Response: 2564667
Conc: 16.67 ug/ml

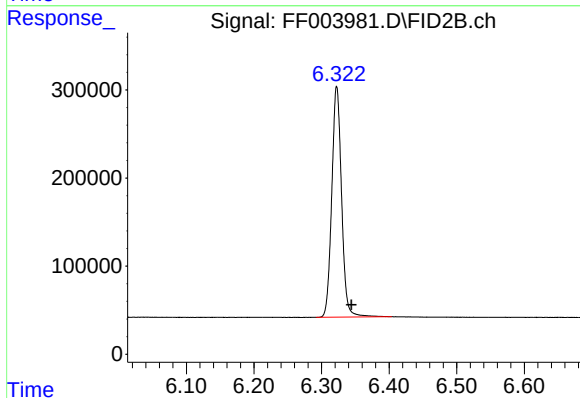


#3 N-DODECANE

R.T.: 6.322 min
Delta R.T.: -0.022 min
Response: 2640350
Conc: 16.92 ug/ml

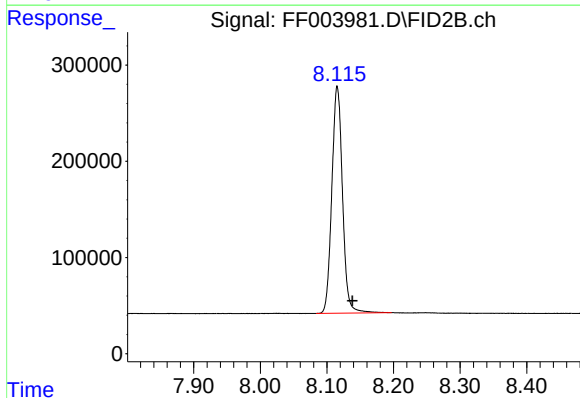


#4 N-TETRADECANE

R.T.: 8.116 min
Delta R.T.: -0.023 min
Response: 2627515
Conc: 16.39 ug/ml

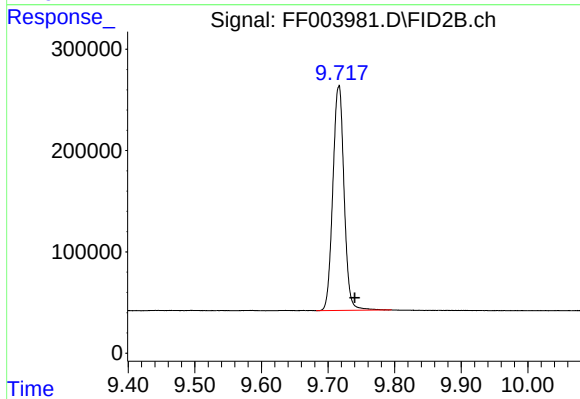


#5 N-HEXADECANE

R.T.: 9.716 min
Delta R.T.: -0.024 min
Response: 2599844
Conc: 15.96 ug/ml

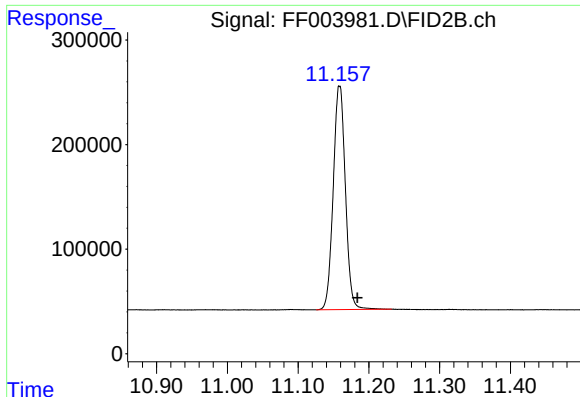


#6 N-OCTADECANE

R.T.: 11.159 min
Delta R.T.: -0.025 min
Response: 2557210
Conc: 15.52 ug/ml

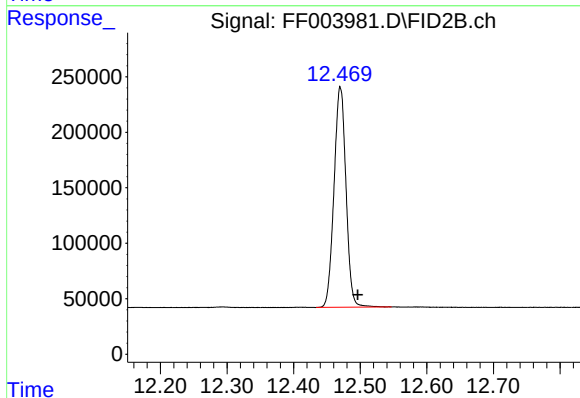


#7 N-EICOSANE

R.T.: 12.470 min
Delta R.T.: -0.026 min
Response: 2480211
Conc: 15.16 ug/ml

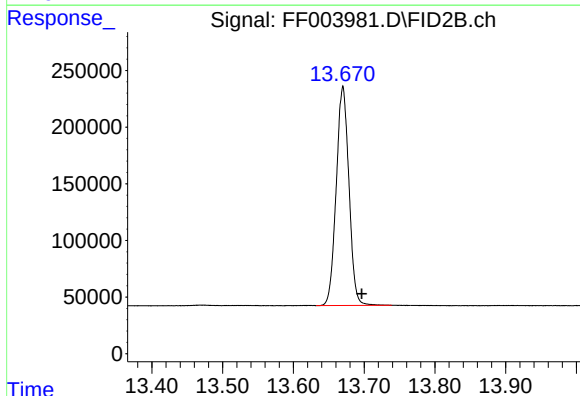


#8 N-DOCOSANE

R.T.: 13.670 min
Delta R.T.: -0.027 min
Response: 2415042
Conc: 14.96 ug/ml

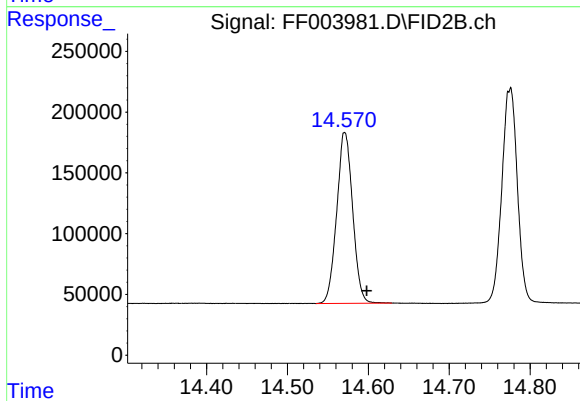


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.571 min
Delta R.T.: -0.027 min
Response: 1920888
Conc: 13.80 ug/ml

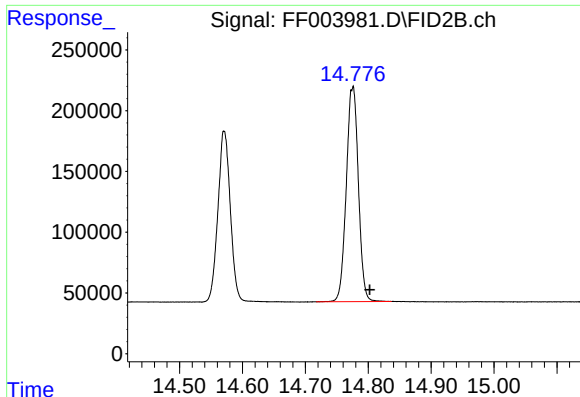


#10 N-TETRACOSANE

R.T.: 14.775 min
Delta R.T.: -0.027 min
Response: 2361098
Conc: 14.92 ug/ml

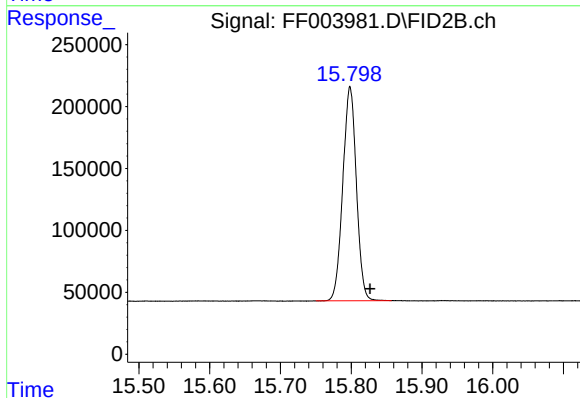

#11 N-HEXACOSANE

R.T.: 15.798 min
Delta R.T.: -0.028 min
Response: 2305221
Conc: 14.94 ug/ml

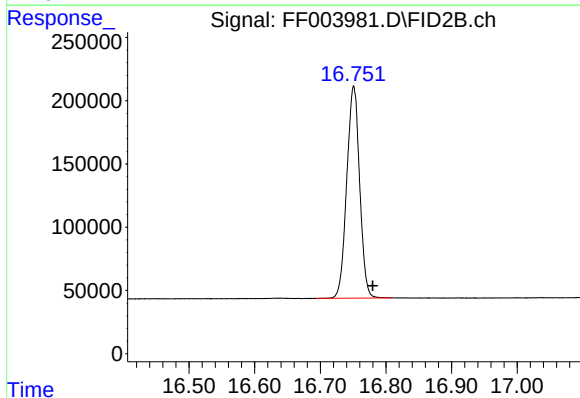

#12 N-OCTACOSANE

R.T.: 16.751 min
Delta R.T.: -0.029 min
Response: 2286576
Conc: 15.13 ug/ml