

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
 Data File : FF003988.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2019 17:18
 Operator : AJ\SJ
 Sample : K2061-02MS
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 27 01:00:56 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
 Quant Title :
 QLast Update : Mon Mar 04 08:35:38 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.573	1752767	12.589 ug/ml
Target Compounds			
2) N-DECANE	4.306	1780020	11.572 ug/ml
3) N-DODECANE	6.326	1923312	12.324 ug/ml
4) N-TETRADECANE	8.117	1986779	12.391 ug/ml
5) N-HEXADECANE	9.718	1979316	12.153 ug/ml
6) N-OCTADECANE	11.160	1963651	11.919 ug/ml
7) N-EICOSANE	12.471	1899236	11.610 ug/ml
8) N-DOCOSANE	13.672	1901113	11.780 ug/ml
10) N-TETRACOSANE	14.776	1916066	12.110 ug/mlm
11) N-HEXACOSANE	15.800	2276061	14.747 ug/ml
12) N-OCTACOSANE	16.752	2955222	19.556 ug/mlm


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032619\
Data File : FF003988.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2019 17:18
Operator : AJ\SJ
Sample : K2061-02MS
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 01:00:56 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF030119.M
Quant Title :
QLast Update : Mon Mar 04 08:35:38 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

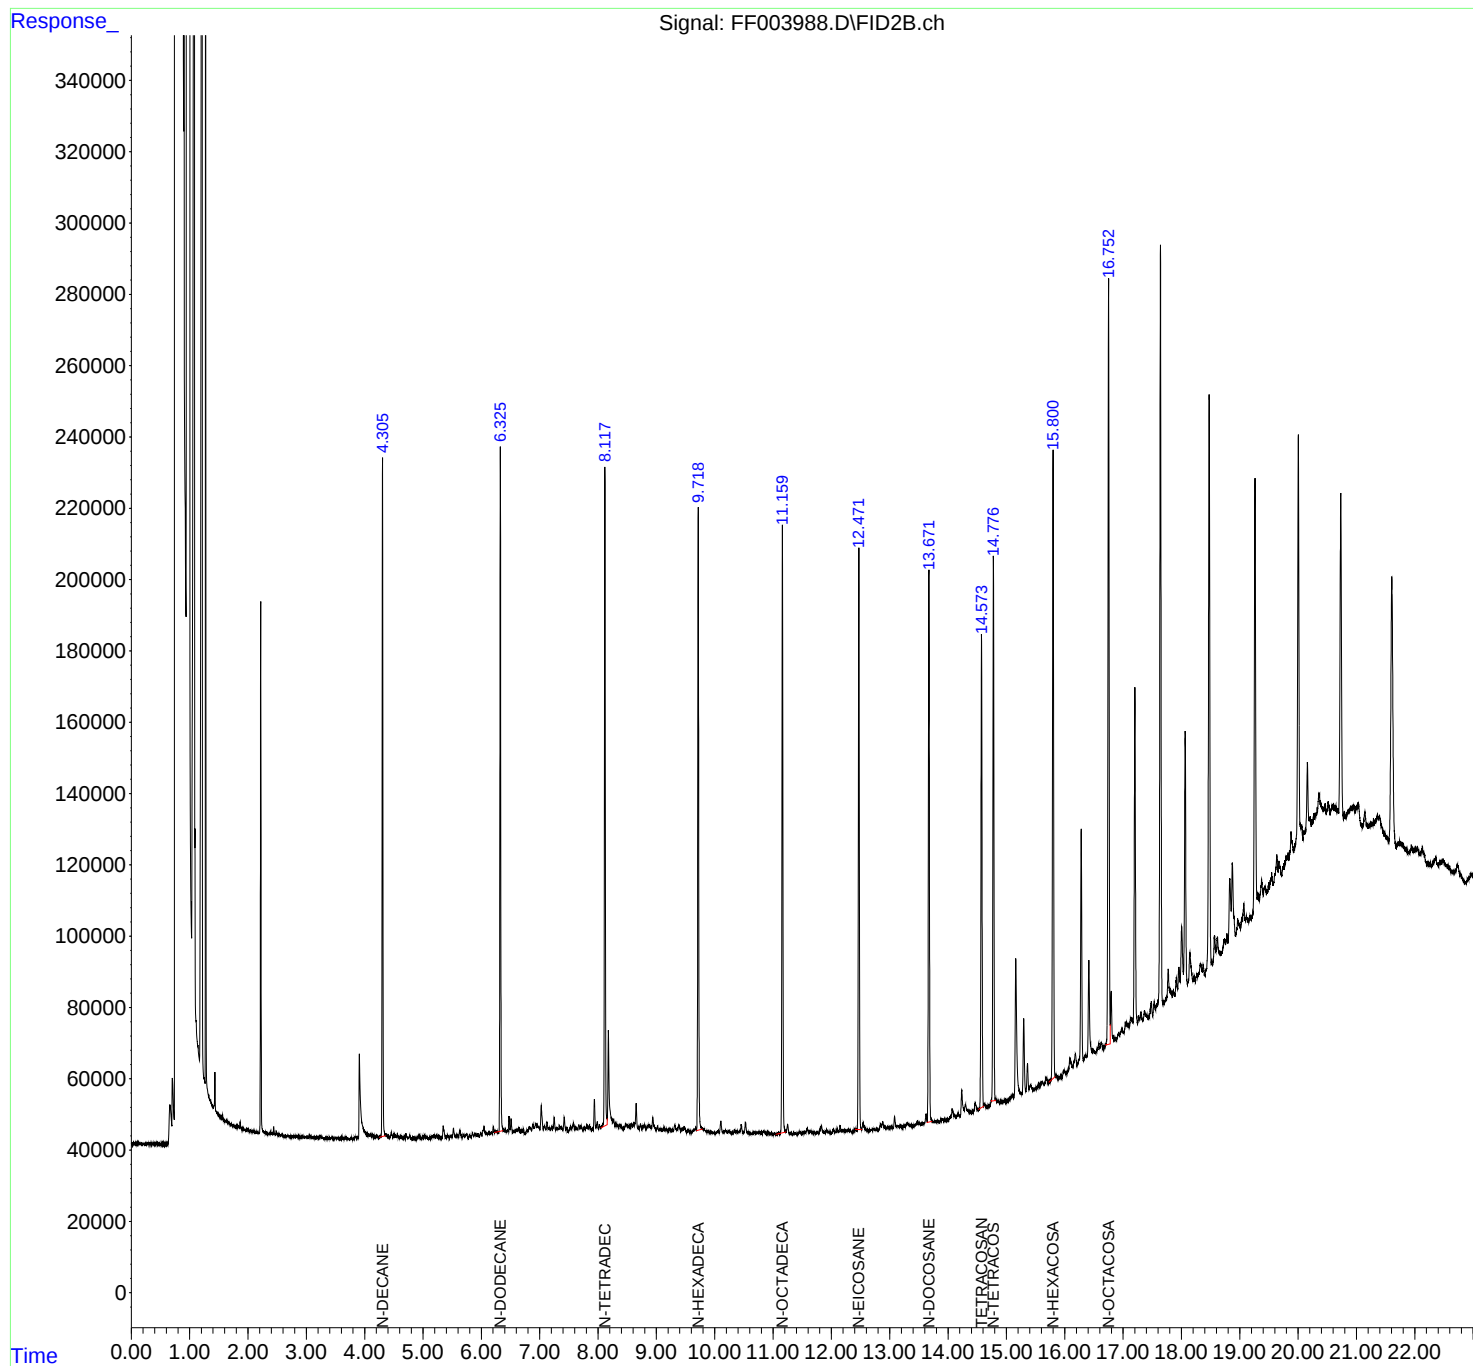

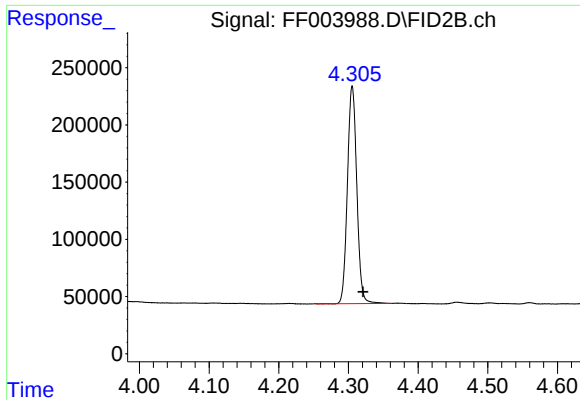


#2 N-DECANE

R.T.: 4.306 min
Delta R.T.: -0.015 min
Response: 1780020
Conc: 11.57 ug/ml

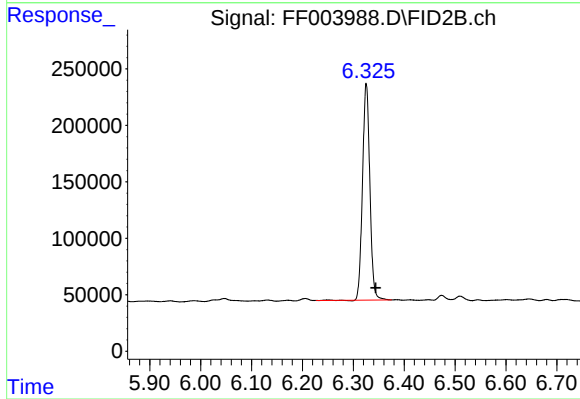


#3 N-DODECANE

R.T.: 6.326 min
Delta R.T.: -0.019 min
Response: 1923312
Conc: 12.32 ug/ml

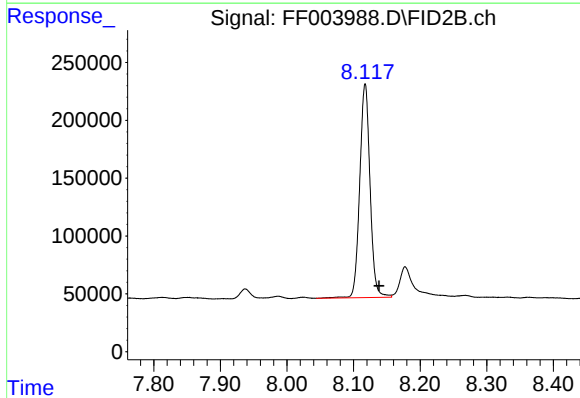


#4 N-TETRADECANE

R.T.: 8.117 min
Delta R.T.: -0.021 min
Response: 1986779
Conc: 12.39 ug/ml

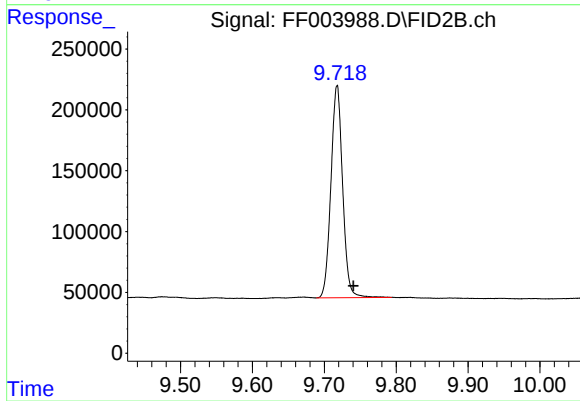


#5 N-HEXADECANE

R.T.: 9.718 min
Delta R.T.: -0.022 min
Response: 1979316
Conc: 12.15 ug/ml

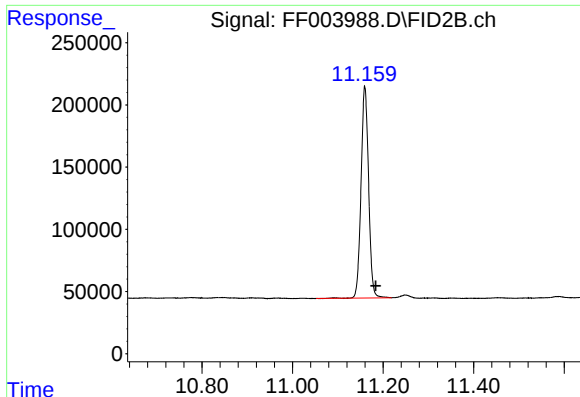


#6 N-OCTADECANE

R.T.: 11.160 min
Delta R.T.: -0.024 min
Response: 1963651
Conc: 11.92 ug/ml

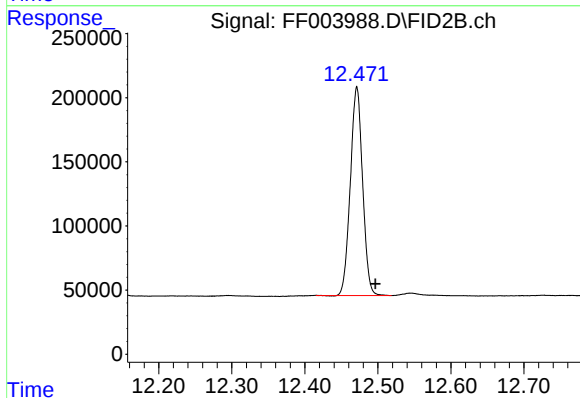


#7 N-EICOSANE

R.T.: 12.471 min
Delta R.T.: -0.025 min
Response: 1899236
Conc: 11.61 ug/ml

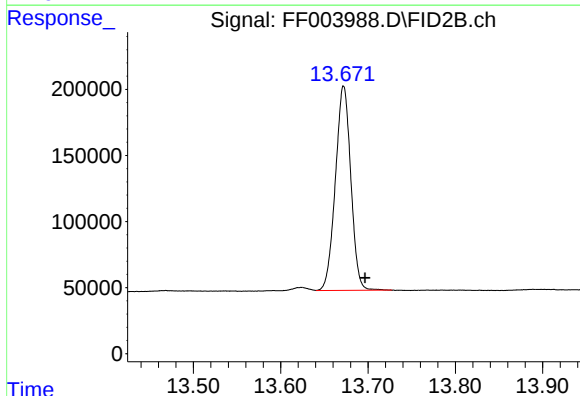


#8 N-DOCOSANE

R.T.: 13.672 min
Delta R.T.: -0.025 min
Response: 1901113
Conc: 11.78 ug/ml

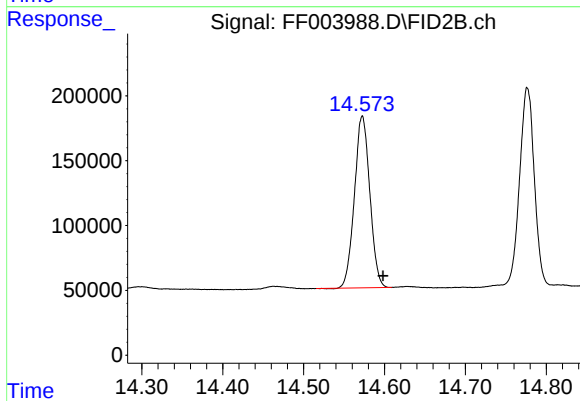


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.573 min
Delta R.T.: -0.026 min
Response: 1752767
Conc: 12.59 ug/ml

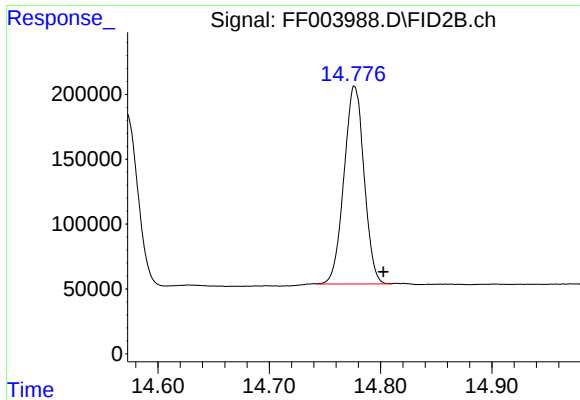


#10 N-TETRACOSANE

R.T.: 14.776 min
Delta R.T.: -0.027 min
Response: 1916066
Conc: 12.11 ug/ml m

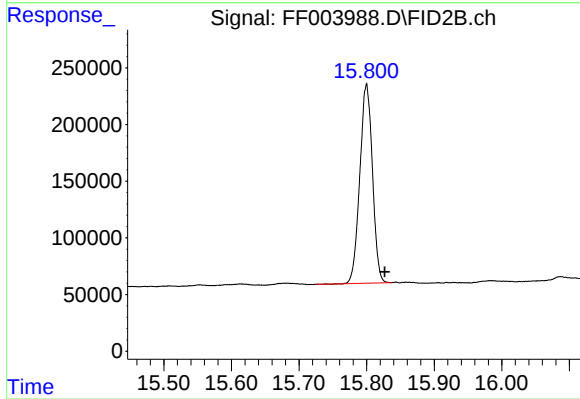

#11 N-HEXACOSANE

R.T.: 15.800 min
Delta R.T.: -0.027 min
Response: 2276061
Conc: 14.75 ug/ml

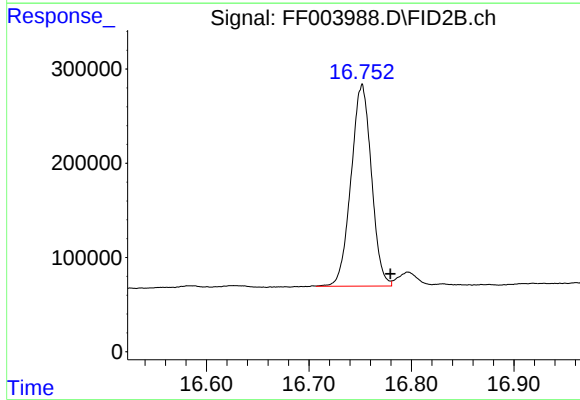

#12 N-OCTACOSANE

R.T.: 16.752 min
Delta R.T.: -0.028 min
Response: 2955222
Conc: 19.56 ug/ml m