

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032620\  
Data File : FF006665.D  
Signal(s) : FID2B.ch  
Acq On : 26 Mar 2020 13:58  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Mar 27 01:09:26 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031020.M  
Quant Title :  
QLast Update : Tue Mar 10 14:59:43 2020  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

| Compound                    | R.T.   | Response | Conc Units   |
|-----------------------------|--------|----------|--------------|
| -----                       |        |          |              |
| System Monitoring Compounds |        |          |              |
| Target Compounds            |        |          |              |
| 3) N-DODECANE               | 6.366  | 5021193  | 35.601 ug/ml |
| 11) N-HEXACOSANE            | 15.805 | 102585   | 0.708 ug/ml  |
| 12) N-OCTACOSANE            | 16.754 | 4960954  | 34.637 ug/ml |
| 13) N-TRIACONTANE           | 17.633 | 790166   | 5.583 ug/ml  |
| 14) N-DOTRIACONTANE         | 18.461 | 795660   | 5.903 ug/ml  |
| 15) N-TETRATRIACONTANE      | 19.242 | 536115   | 4.748 ug/ml  |
| 16) N-HEXATRIACONTANE       | 19.979 | 370698   | 4.036 ug/ml  |
| 17) N-OCTATRIACONTANE       | 20.698 | 251915   | 3.648 ug/ml  |
| 18) N-TETRACONTANE          | 21.569 | 165700   | 2.394 ug/ml  |
| -----                       |        |          |              |


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID\_F\Data\FF032620\  
Data File : FF006665.D  
Signal(s) : FID2B.ch  
Acq On : 26 Mar 2020 13:58  
Operator : DD\AJ  
Sample : RT MARKER  
Misc :  
ALS Vial : 54 Sample Multiplier: 1

Integration File: autoint1.e  
Quant Time: Mar 27 01:09:26 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID\_F\Method\FF031020.M  
Quant Title :  
QLast Update : Tue Mar 10 14:59:43 2020  
Response via : Initial Calibration  
Integrator: ChemStation


Volume Inj. : 1uL  
Signal Phase : Rxi-1ms  
Signal Info : 20mx0.18mmx0.18um

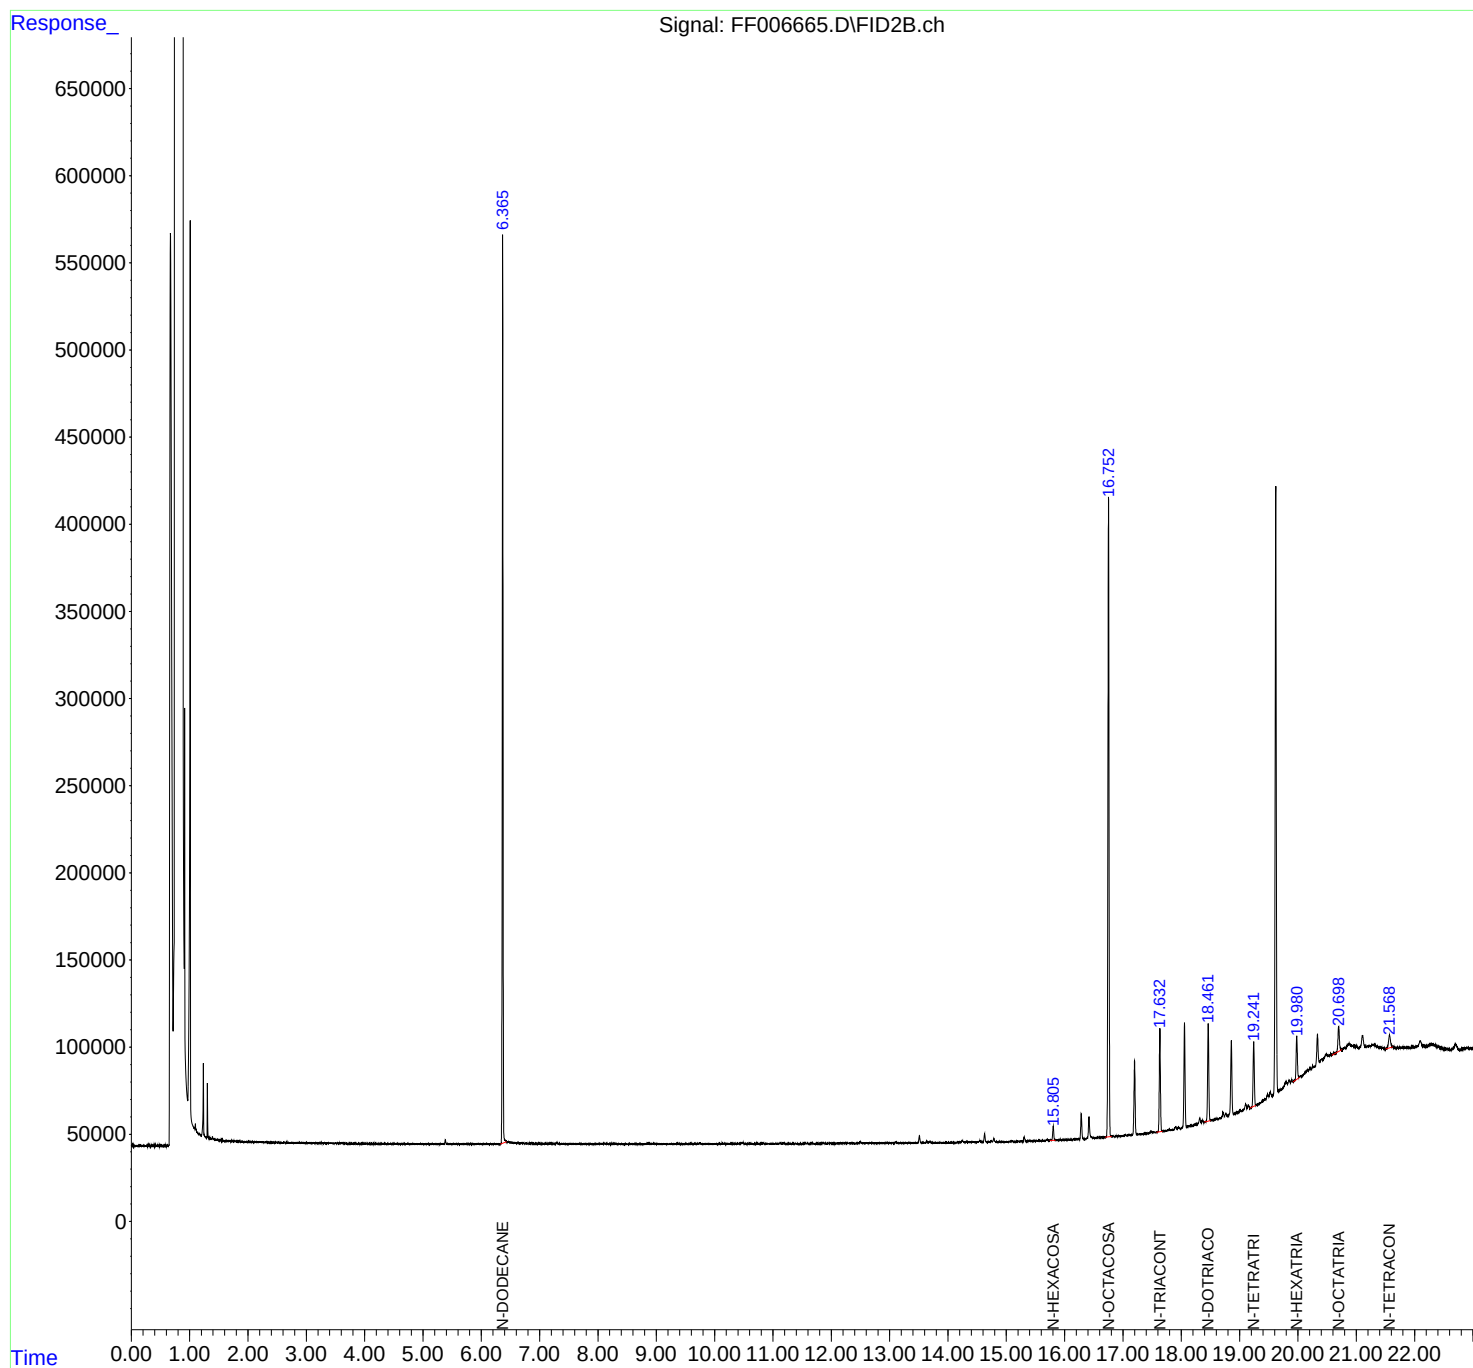

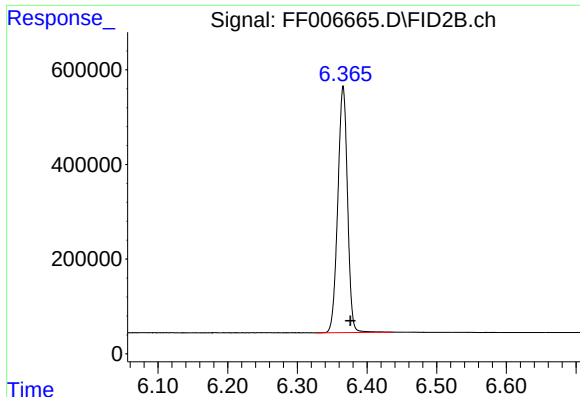


#3 N-DODECANE

R.T.: 6.366 min  
Delta R.T.: -0.010 min  
Response: 5021193  
Conc: 35.60 ug/ml

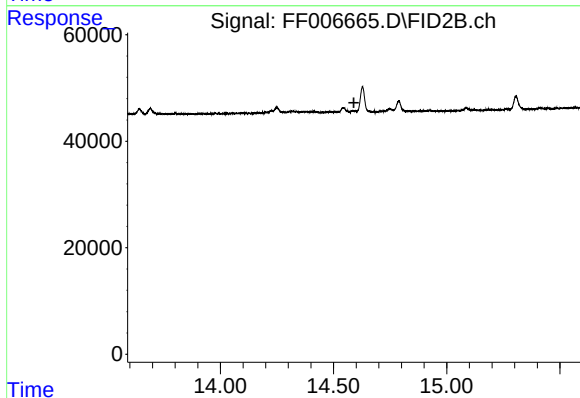


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min  
Exp R.T.: 14.590 min  
Response: 0  
Conc: N.D.

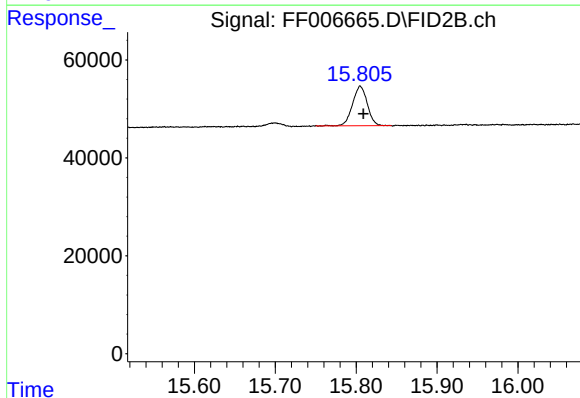


#11 N-HEXACOSANE

R.T.: 15.805 min  
Delta R.T.: -0.004 min  
Response: 102585  
Conc: 0.71 ug/ml

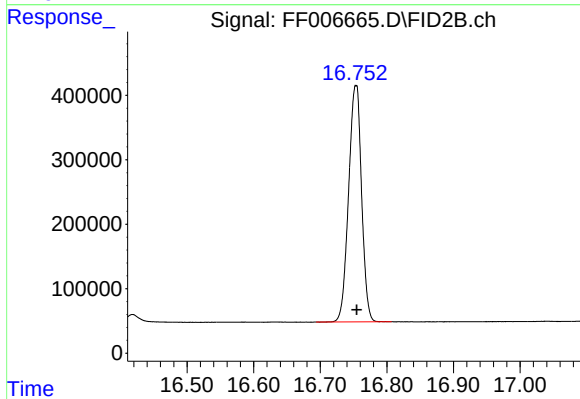


#12 N-OCTACOSANE

R.T.: 16.754 min  
Delta R.T.: 0.000 min  
Response: 4960954  
Conc: 34.64 ug/ml

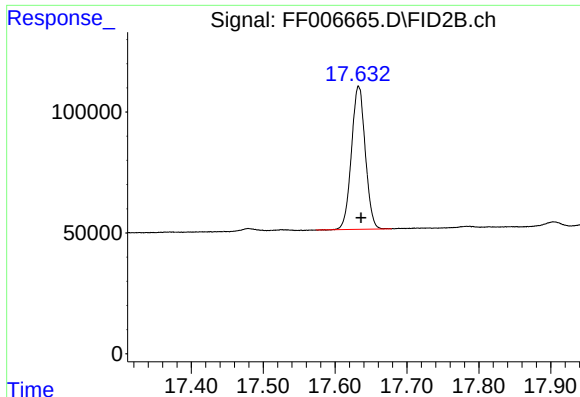


#13 N-TRIACONTANE

R.T.: 17.633 min  
Delta R.T.: -0.003 min  
Response: 790166  
Conc: 5.58 ug/ml

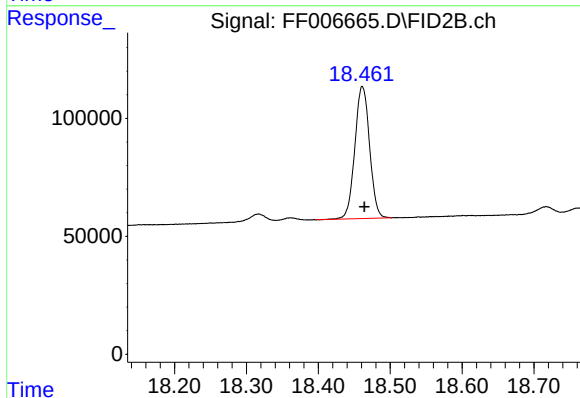


#14 N-DOTRIACONTANE

R.T.: 18.461 min  
Delta R.T.: -0.003 min  
Response: 795660  
Conc: 5.90 ug/ml

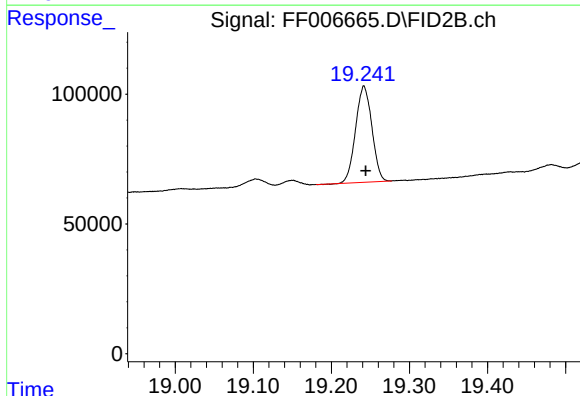


#15 N-TETRATRIACONTANE

R.T.: 19.242 min  
Delta R.T.: -0.002 min  
Response: 536115  
Conc: 4.75 ug/ml

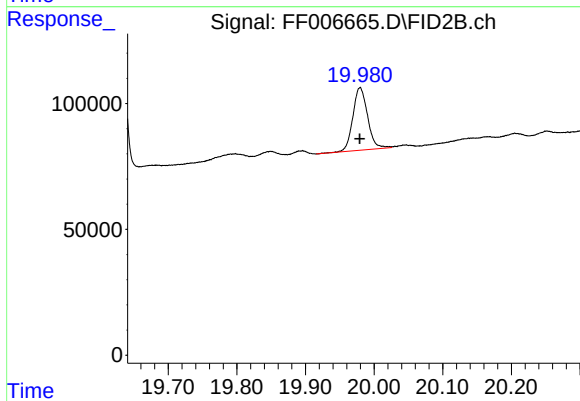


#16 N-HEXATRIACONTANE

R.T.: 19.979 min  
Delta R.T.: 0.000 min  
Response: 370698  
Conc: 4.04 ug/ml

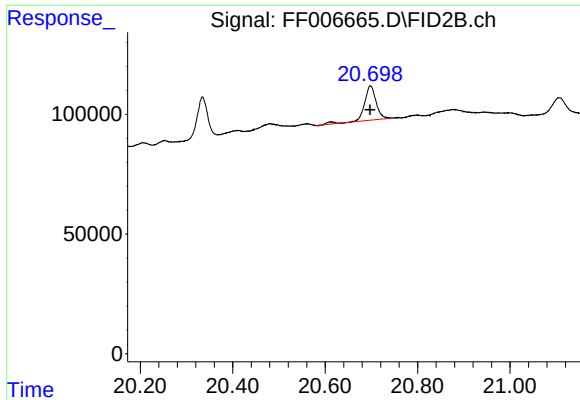

#17 N-OCTATRIACONTANE

R.T.: 20.698 min  
Delta R.T.: 0.000 min  
Response: 251915  
Conc: 3.65 ug/ml

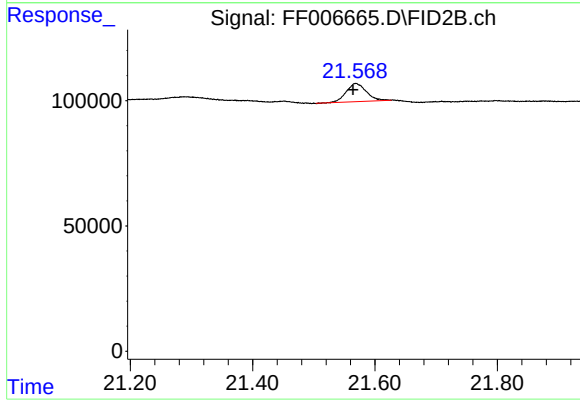

#18 N-TETRACONTANE

R.T.: 21.569 min  
Delta R.T.: 0.004 min  
Response: 165700  
Conc: 2.39 ug/ml