

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032620\
 Data File : FF006674.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2020 18:31
 Operator : DD\AJ
 Sample : L2043-06
 Misc :
 ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
 Quant Time: Mar 27 01:11:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
 Quant Title :
 QLast Update : Tue Mar 10 14:59:43 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.587	1676693	13.028 ug/ml
Target Compounds			
4) N-TETRADECANE	8.220f	335358	2.345 ug/ml
5) N-HEXADECANE	9.789	204626	1.396 ug/ml
11) N-HEXACOSANE	15.805	110981	0.766 ug/ml
12) N-OCTACOSANE	16.752	349489	2.440 ug/ml
13) N-TRIACONTANE	17.636	427001	3.017 ug/ml
14) N-DOTRIACONTANE	18.459	376707	2.795 ug/ml
15) N-TETRATRIACONTANE	19.242	84	0.001 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032620\
Data File : FF006674.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2020 18:31
Operator : DD\AJ
Sample : L2043-06
Misc :
ALS Vial : 63 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 01:11:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

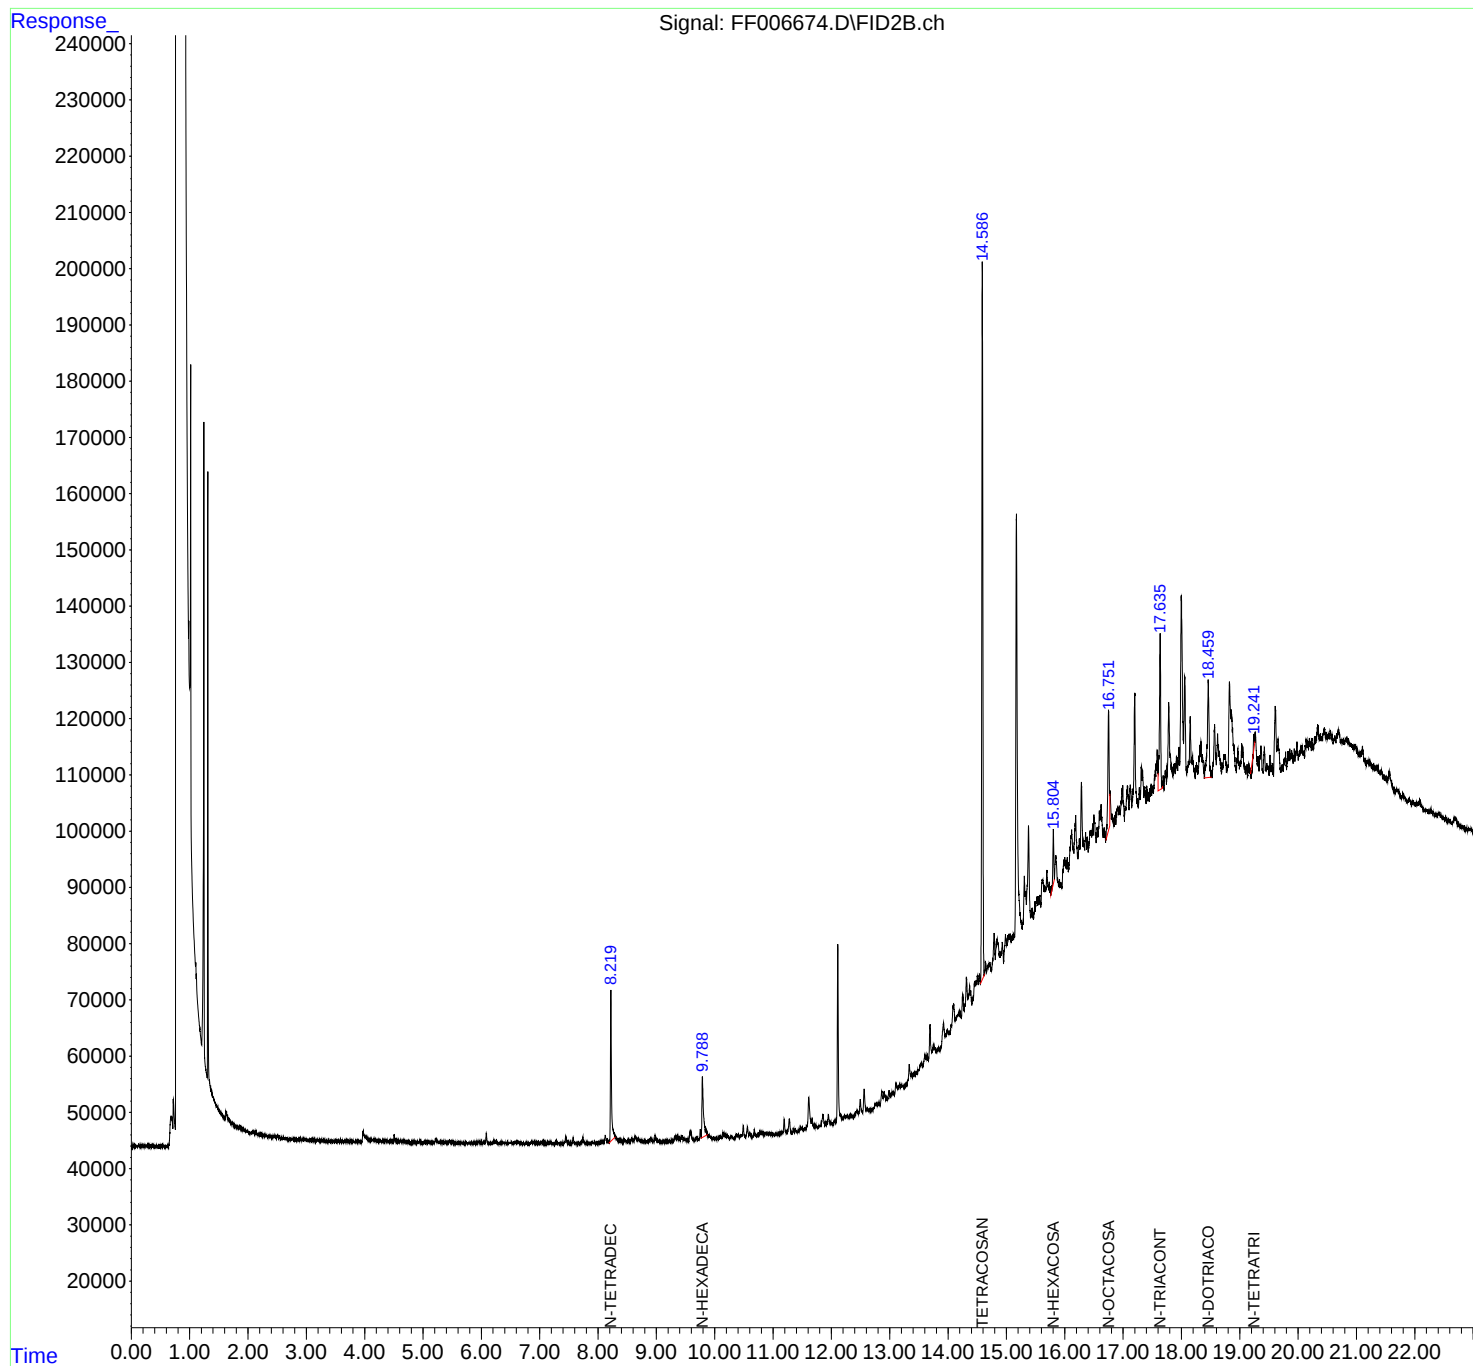

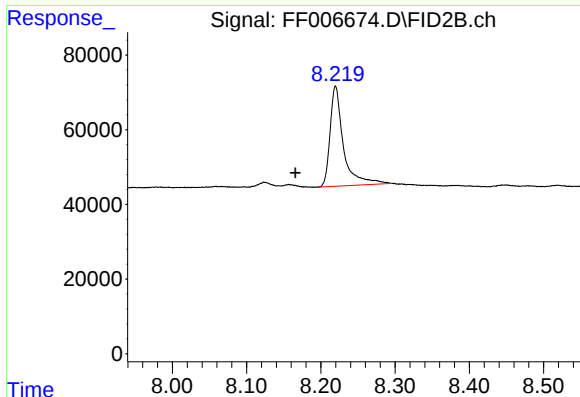


#4 N-TETRADECANE

R.T.: 8.220 min
Delta R.T.: 0.054 min
Response: 335358
Conc: 2.34 ug/ml

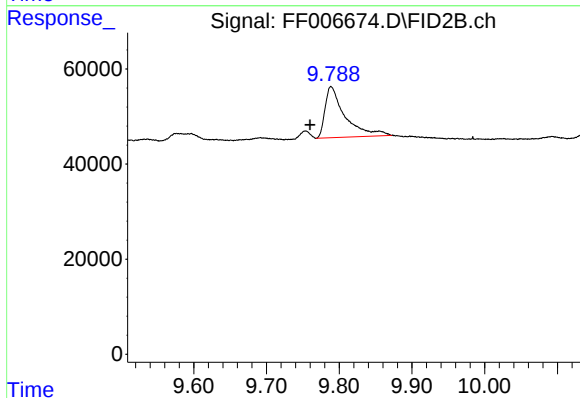


#5 N-HEXADECANE

R.T.: 9.789 min
Delta R.T.: 0.029 min
Response: 204626
Conc: 1.40 ug/ml

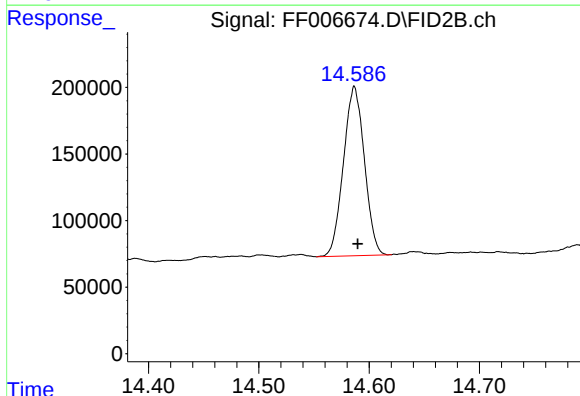


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.587 min
Delta R.T.: -0.003 min
Response: 1676693
Conc: 13.03 ug/ml

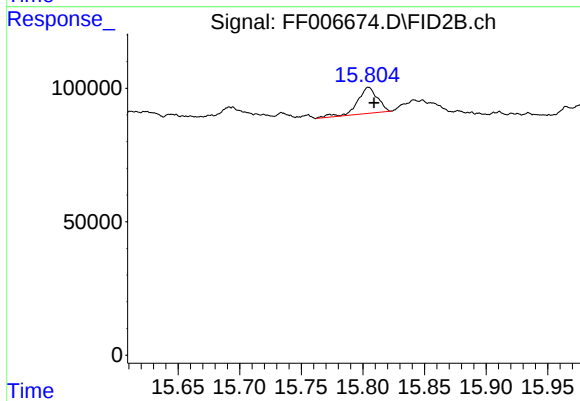


#11 N-HEXACOSANE

R.T.: 15.805 min
Delta R.T.: -0.004 min
Response: 110981
Conc: 0.77 ug/ml

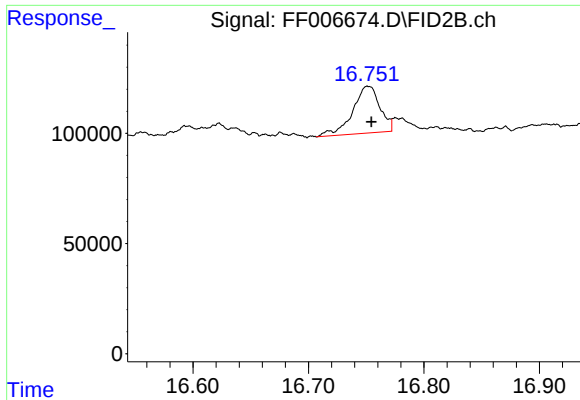


#12 N-OCTACOSANE

R.T.: 16.752 min
Delta R.T.: -0.003 min
Response: 349489
Conc: 2.44 ug/ml

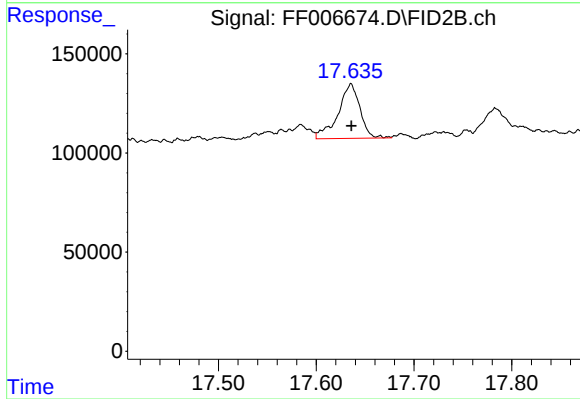


#13 N-TRIACONTANE

R.T.: 17.636 min
Delta R.T.: 0.000 min
Response: 427001
Conc: 3.02 ug/ml

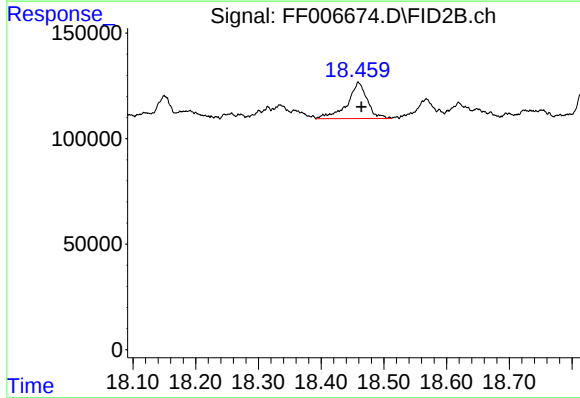

#14 N-DOTRIACONTANE

R.T.: 18.459 min
Delta R.T.: -0.005 min
Response: 376707
Conc: 2.79 ug/ml

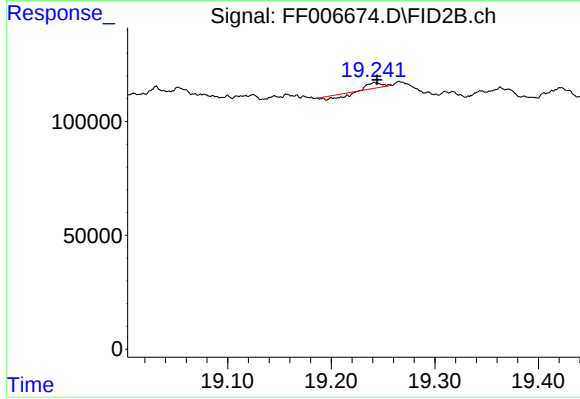

#15 N-TETRATRIACONTANE

R.T.: 19.242 min
Delta R.T.: -0.002 min
Response: 84
Conc: 0.00 ug/ml