

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032620\
Data File : FF006680.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2020 21:34
Operator : DD\AJ
Sample : L2042-11
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 01:12:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.583	2338369	18.169 ug/ml
Target Compounds			
4) N-TETRADECANE	8.218f	279991	1.958 ug/ml
12) N-OCTACOSANE	16.747	156091	1.090 ug/ml
13) N-TRIACONTANE	17.630	150596	1.064 ug/ml
14) N-DOTRIACONTANE	18.458	128314	0.952 ug/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032620\
Data File : FF006680.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2020 21:34
Operator : DD\AJ
Sample : L2042-11
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File: autoint1.e
Quant Time: Mar 27 01:12:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF031020.M
Quant Title :
QLast Update : Tue Mar 10 14:59:43 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

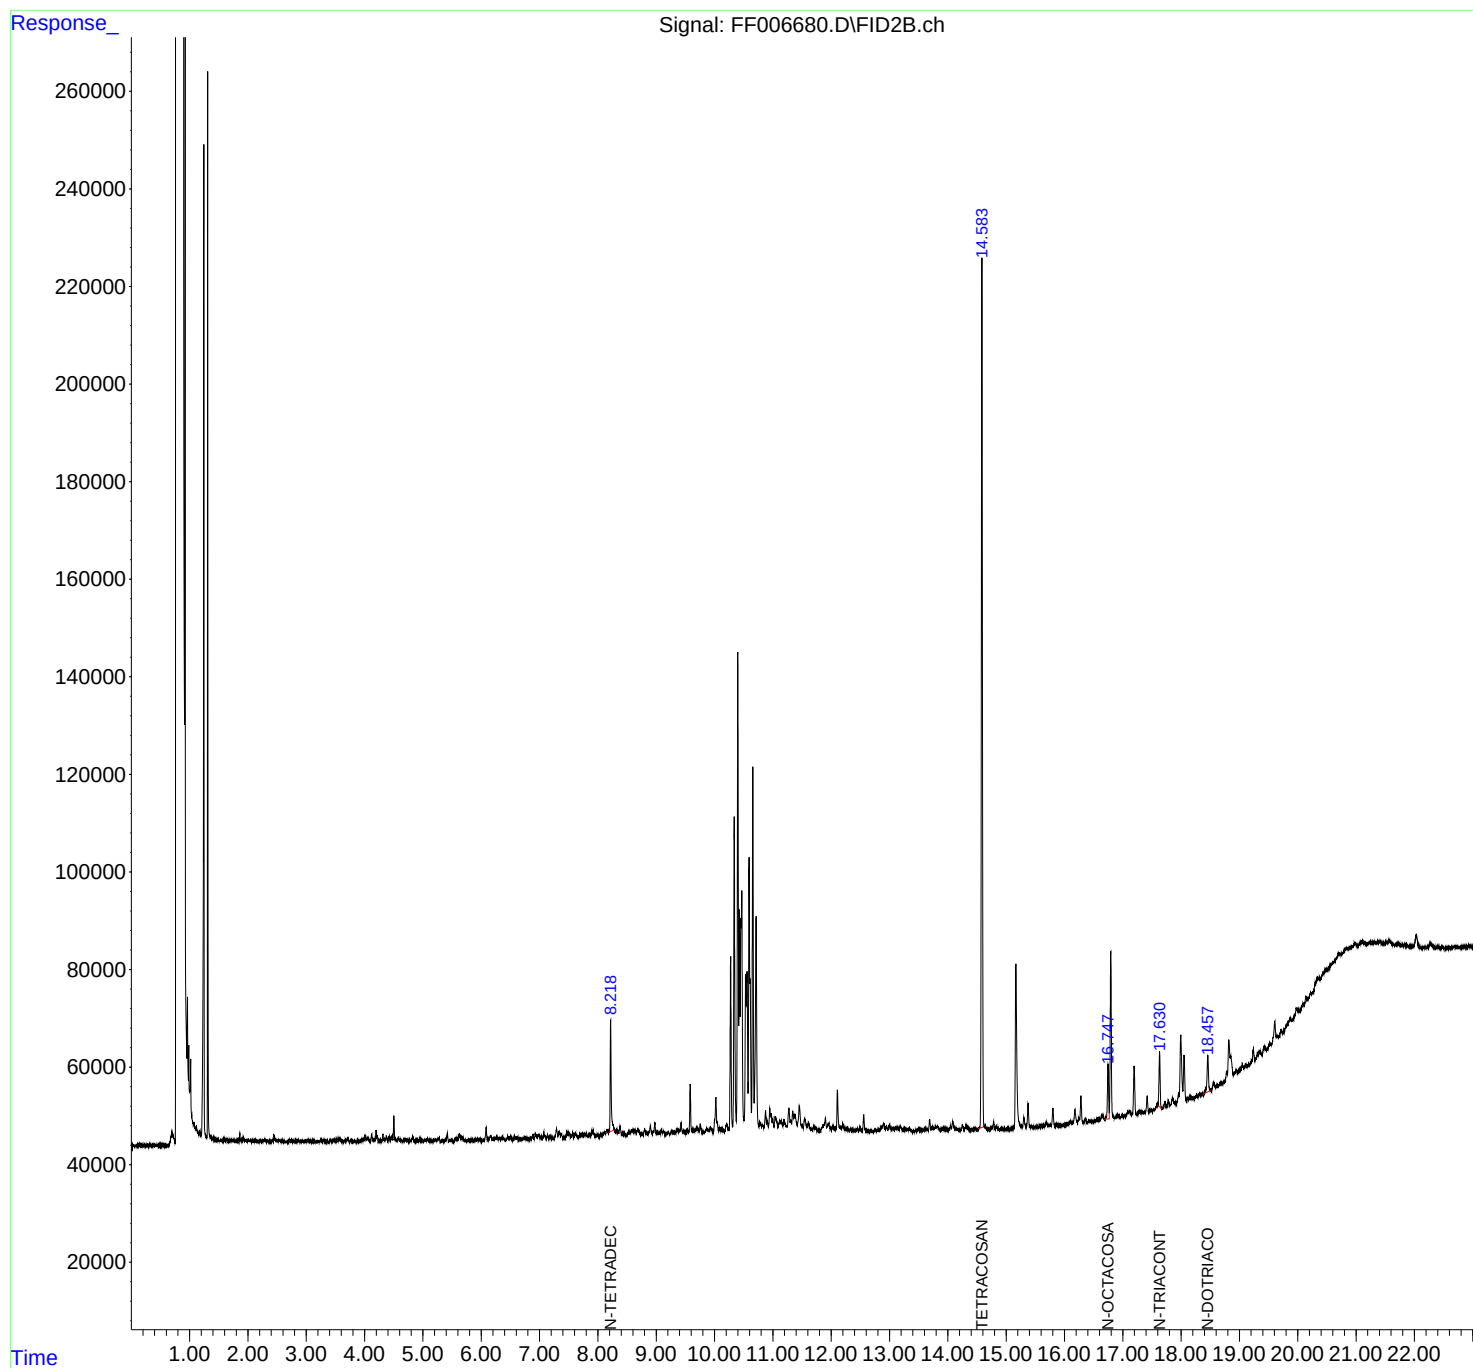

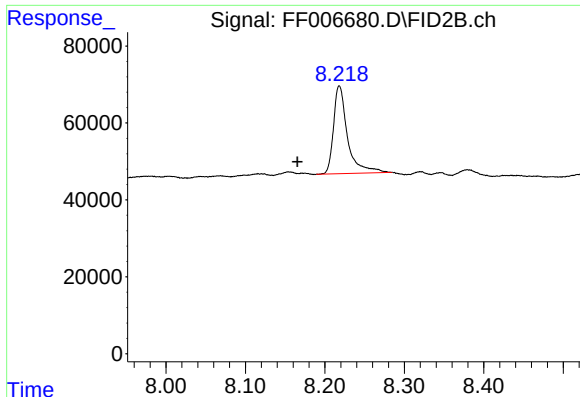


#4 N-TETRADECANE

R.T.: 8.218 min
Delta R.T.: 0.053 min
Response: 279991
Conc: 1.96 ug/ml

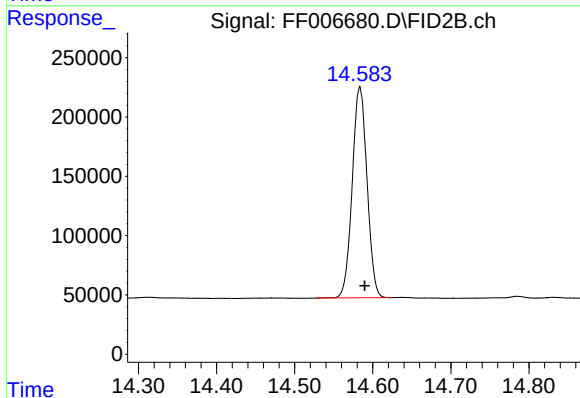


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.583 min
Delta R.T.: -0.006 min
Response: 2338369
Conc: 18.17 ug/ml

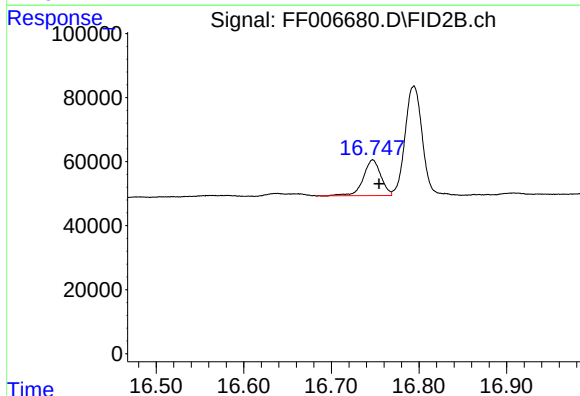


#12 N-OCTACOSANE

R.T.: 16.747 min
Delta R.T.: -0.007 min
Response: 156091
Conc: 1.09 ug/ml

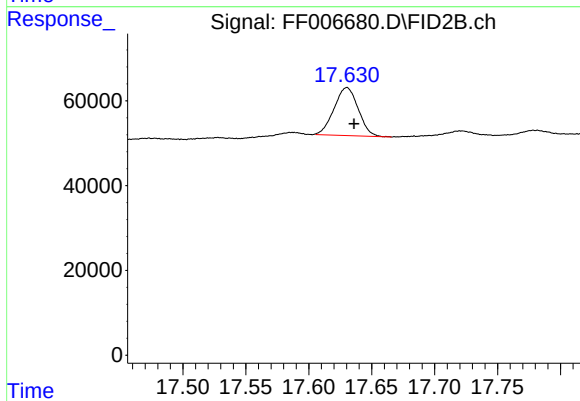

#13 N-TRIACONTANE

R.T.: 17.630 min
Delta R.T.: -0.006 min
Response: 150596
Conc: 1.06 ug/ml

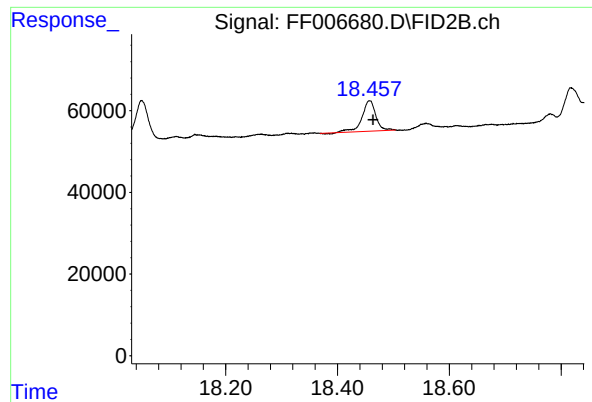

#14 N-DOTRIACONTANE

R.T.: 18.458 min
Delta R.T.: -0.006 min
Response: 128314
Conc: 0.95 ug/ml