

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010158.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 17:06
Operator : AJ\MA
Sample : N1972-05 20X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:25:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units
----------	------	----------	------------

System Monitoring Compounds

Target Compounds

12)	N-OCTACOSANE	16.813	9213	0.070 ug/ml
13)	N-TRIACONTANE	17.706	137992	1.077 ug/ml
14)	N-DOTRIACONTANE	18.539	64259	0.514 ug/ml
15)	N-TETRATRIACONTANE	19.358	347795	3.220 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010158.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 17:06
Operator : AJ\MA
Sample : N1972-05 20X
Misc :
ALS Vial : 69 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:25:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

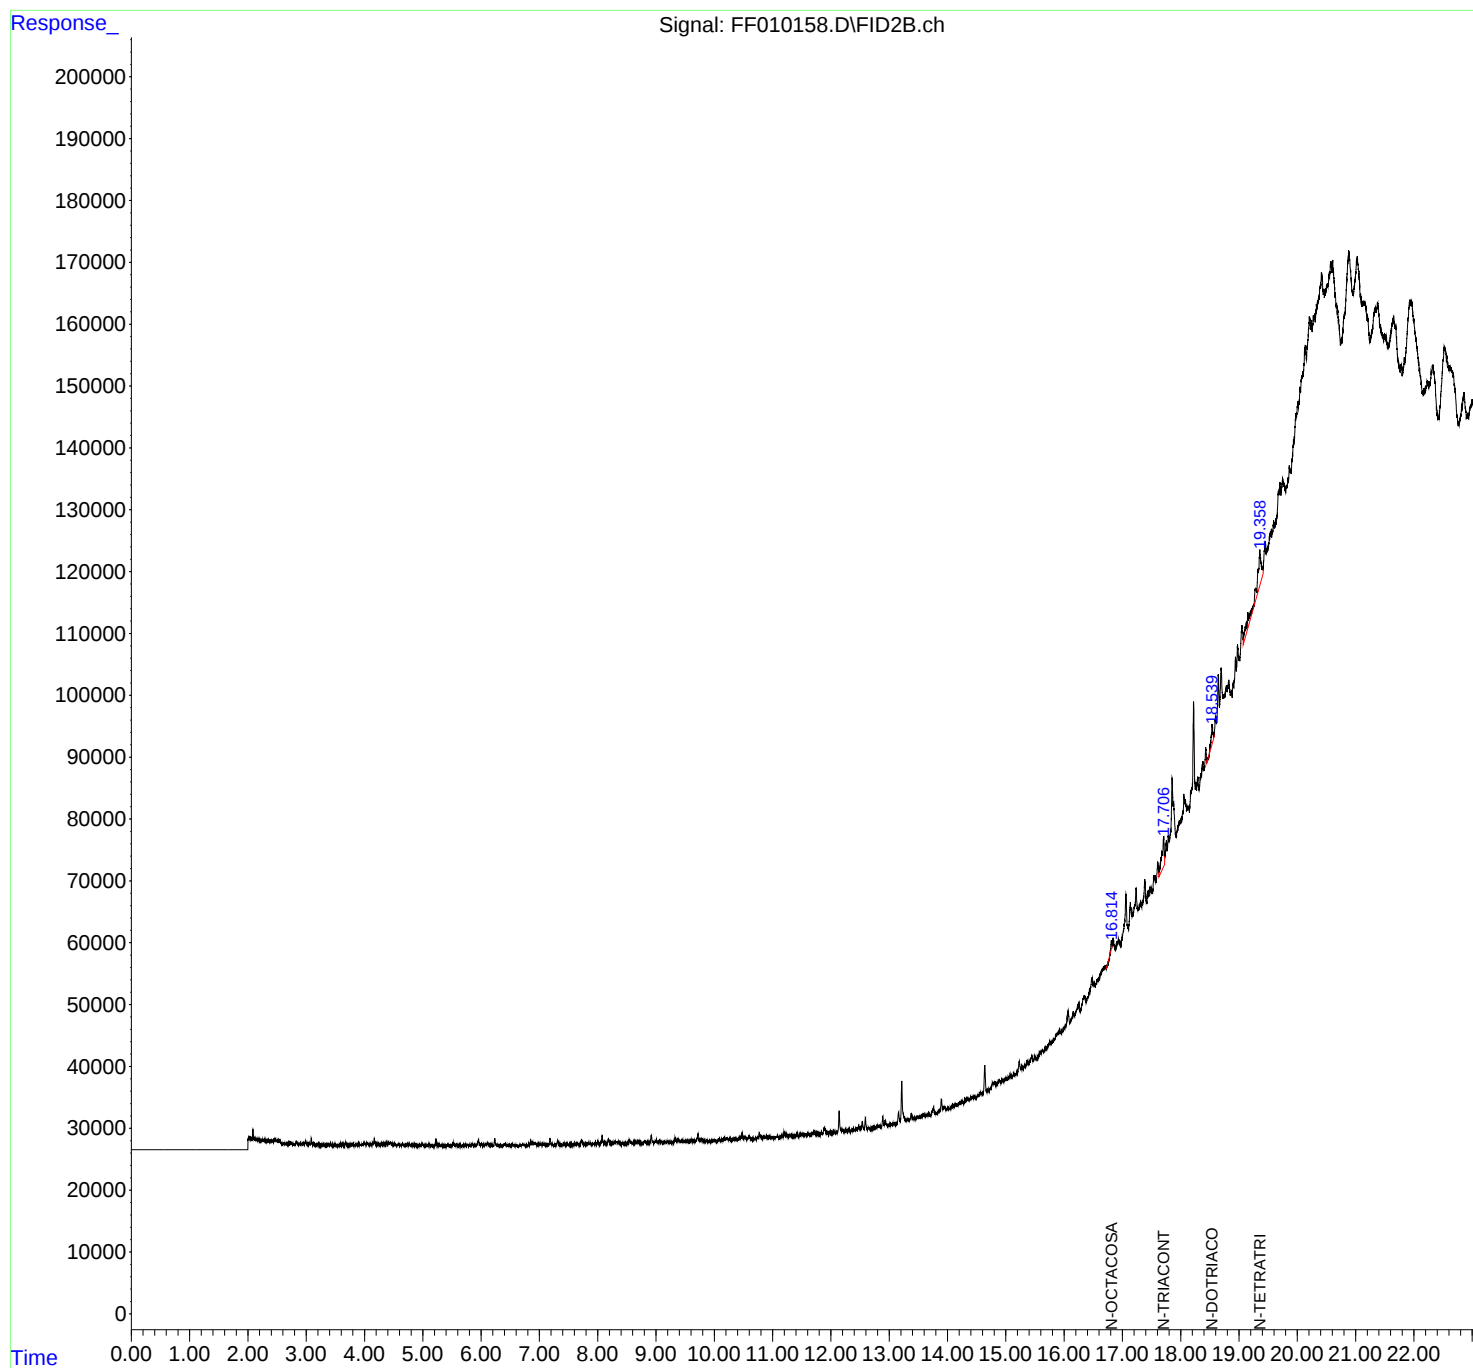


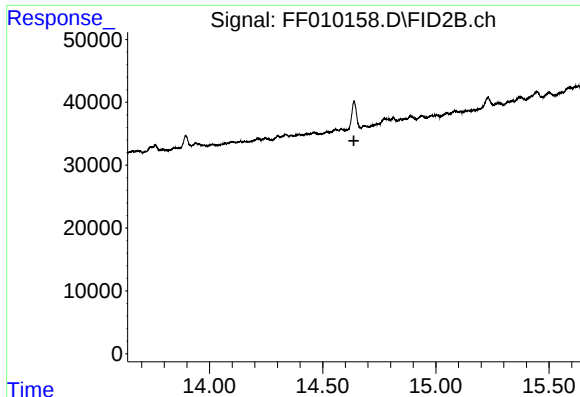

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.638 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

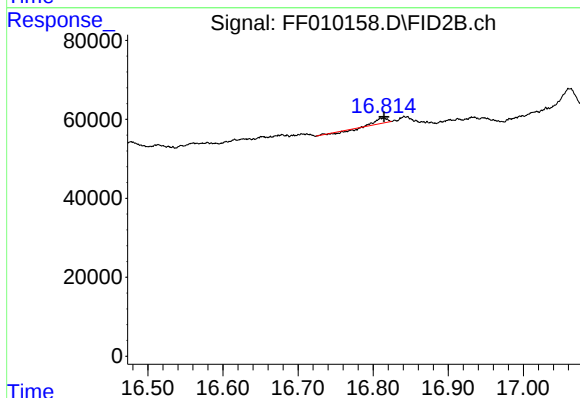


#12 N-OCTACOSANE

R.T.: 16.813 min
Delta R.T.: -0.001 min
Response: 9213
Conc: 0.07 ug/ml

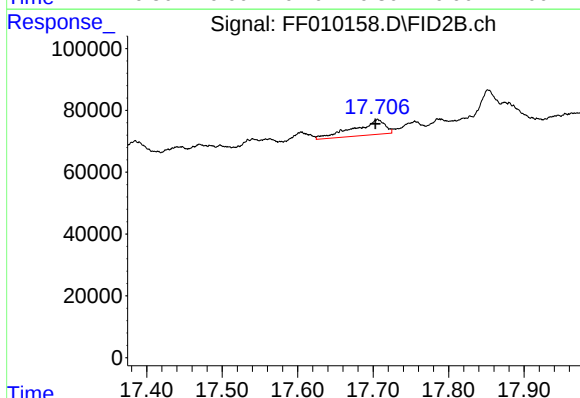


#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: 0.003 min
Response: 137992
Conc: 1.08 ug/ml

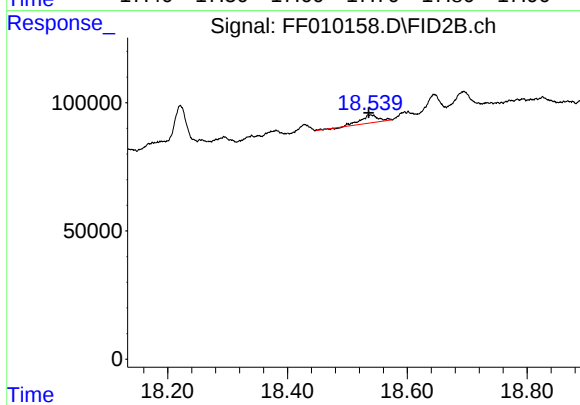

#14 N-DOTRIACONTANE

R.T.: 18.539 min
Delta R.T.: 0.003 min
Response: 64259
Conc: 0.51 ug/ml

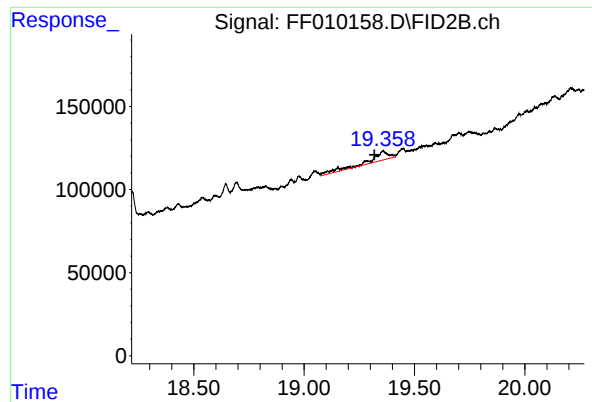

#15 N-TETRATRIACONTANE

R.T.: 19.358 min
Delta R.T.: 0.039 min
Response: 347795
Conc: 3.22 ug/ml

Instrument :

FID_F

ClientSampleId :