

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010159.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 17:36
Operator : AJ\MA
Sample : N1972-06 20X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:25:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
12) N-OCTACOSANE	16.813	75563	0.574 ug/ml
13) N-TRIACONTANE	17.706	99218	0.774 ug/ml
14) N-DOTRIACONTANE	18.540	113793	0.910 ug/ml
15) N-TETRATRIACONTANE	19.360	250658	2.321 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010159.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 17:36
Operator : AJ\MA
Sample : N1972-06 20X
Misc :
ALS Vial : 70 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:25:51 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

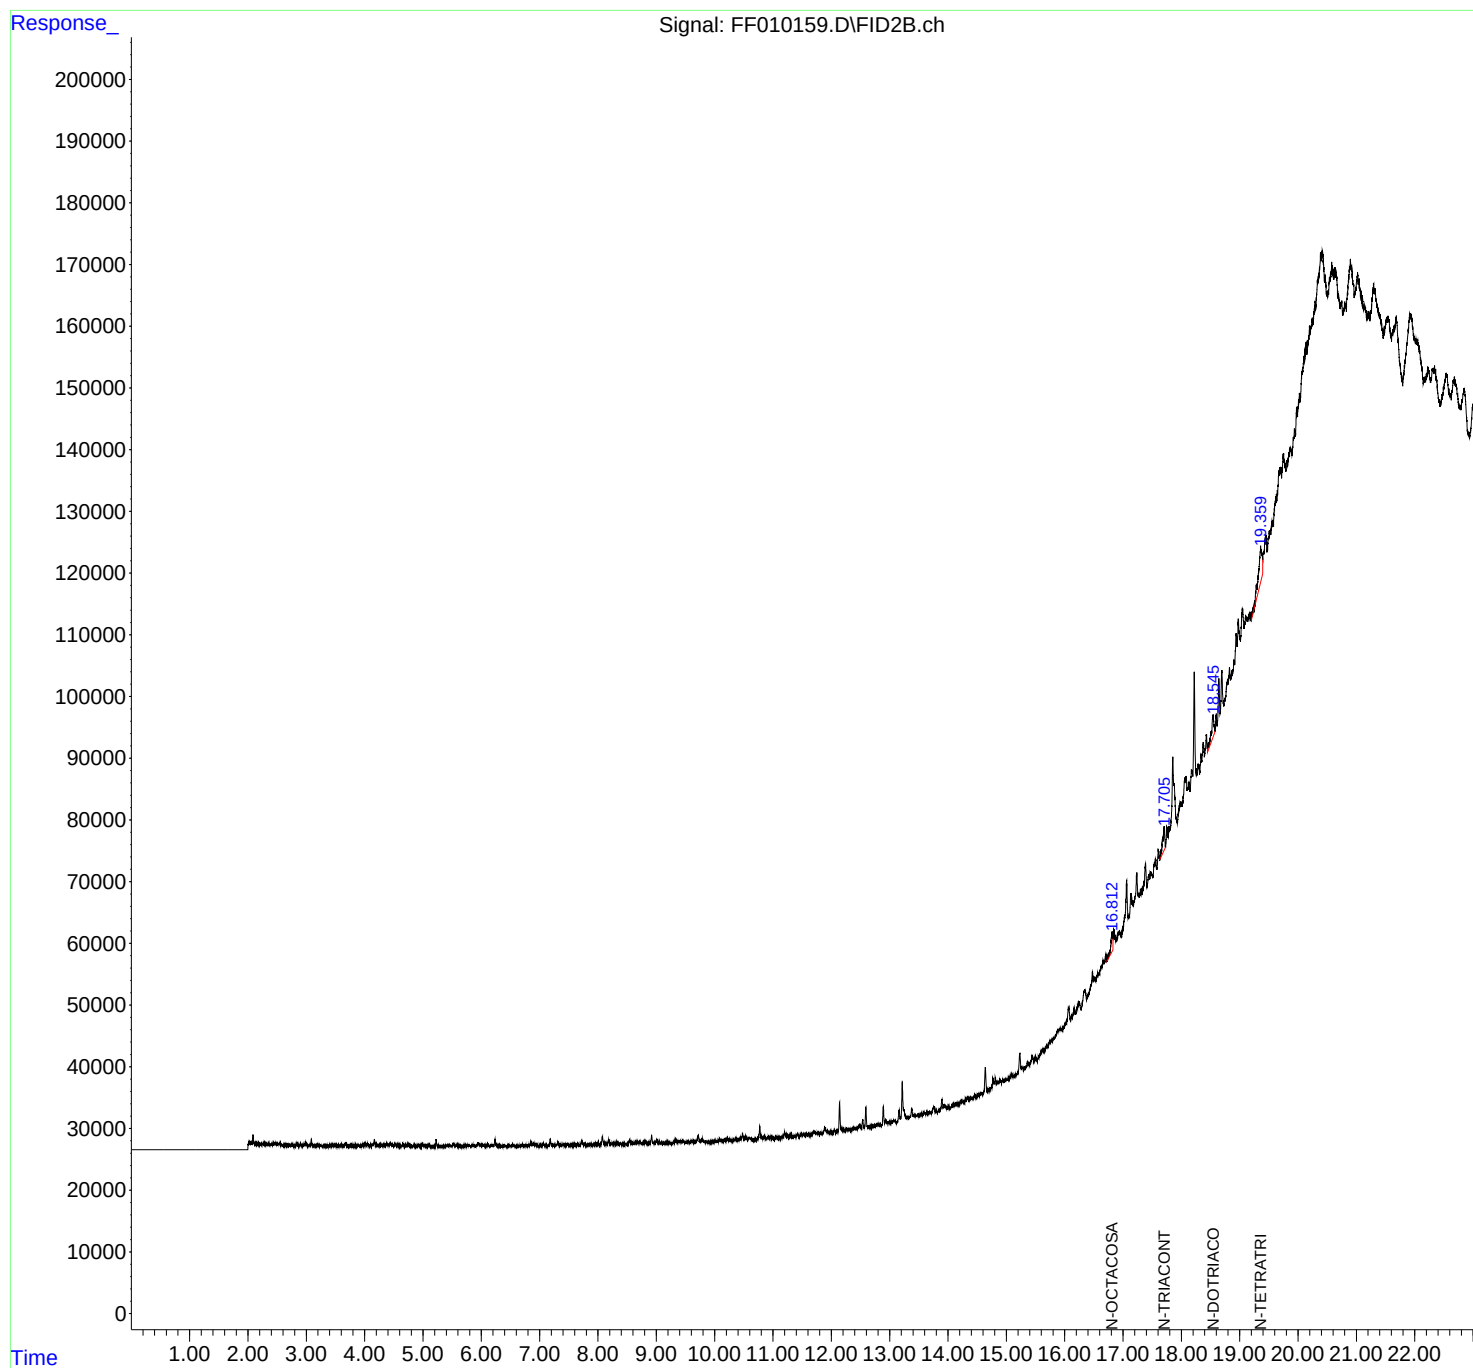


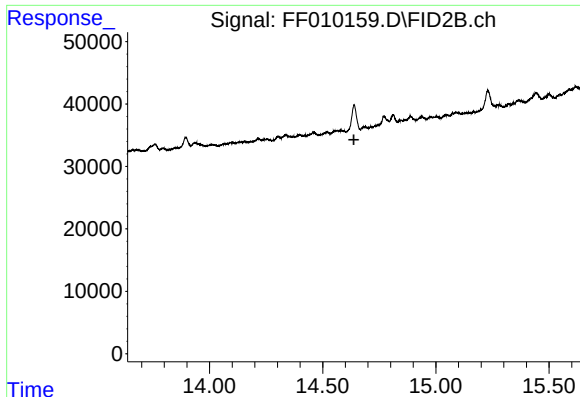

#9 TETRACOSANE-d50 (SURROGATE)


R.T.: 0.000 min
Exp R.T.: 14.638 min
Response: 0
Conc: N.D.

Instrument :
FID_F
ClientSampleId :

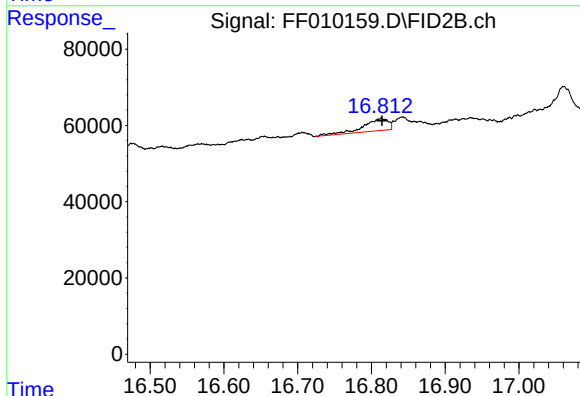


#12 N-OCTACOSANE

R.T.: 16.813 min
Delta R.T.: -0.001 min
Response: 75563
Conc: 0.57 ug/ml

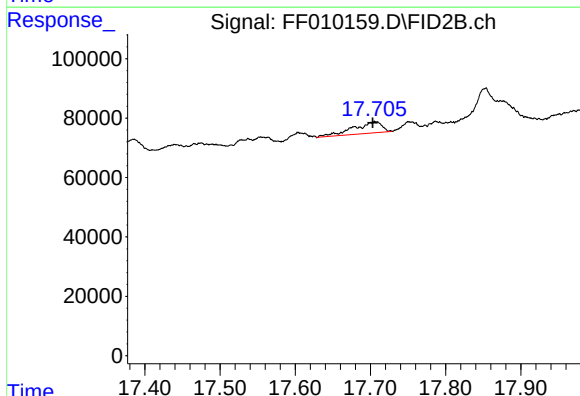


#13 N-TRIACONTANE

R.T.: 17.706 min
Delta R.T.: 0.003 min
Response: 99218
Conc: 0.77 ug/ml

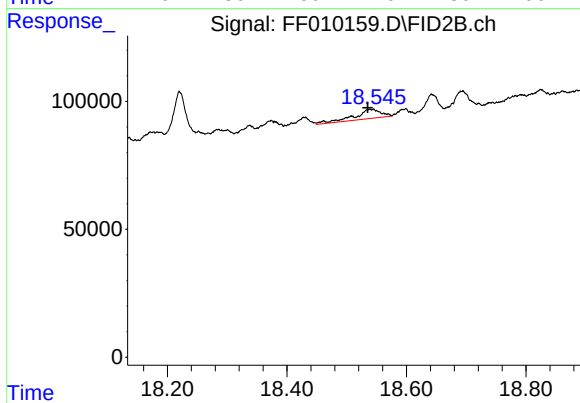

#14 N-DOTRIACONTANE

R.T.: 18.540 min
Delta R.T.: 0.005 min
Response: 113793
Conc: 0.91 ug/ml

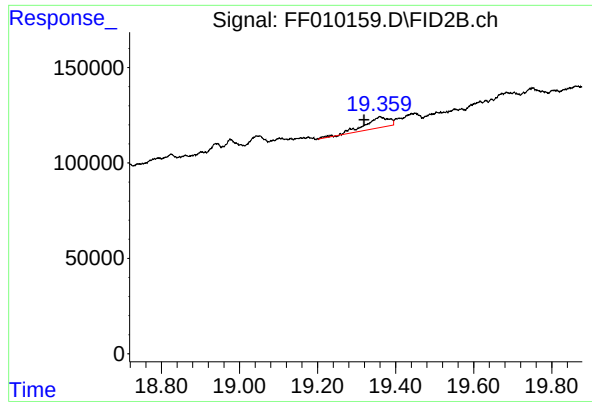

#15 N-TETRATRIACONTANE

R.T.: 19.360 min
Delta R.T.: 0.041 min
Response: 250658
Conc: 2.32 ug/ml

Instrument :

FID_F

ClientSampleId :