

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010166.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 21:37
Operator : AJ\MA
Sample : N1958-03 20X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:26:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
Target Compounds			
7) N-EICOSANE	12.588	205257	1.468 ug/ml
10) N-TETRACOSANE	14.807	106866	0.781 ug/ml
15) N-TETRATRIACONTANE	19.351	164712	1.525 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010166.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 21:37
Operator : AJ\MA
Sample : N1958-03 20X
Misc :
ALS Vial : 75 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 26 22:26:58 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

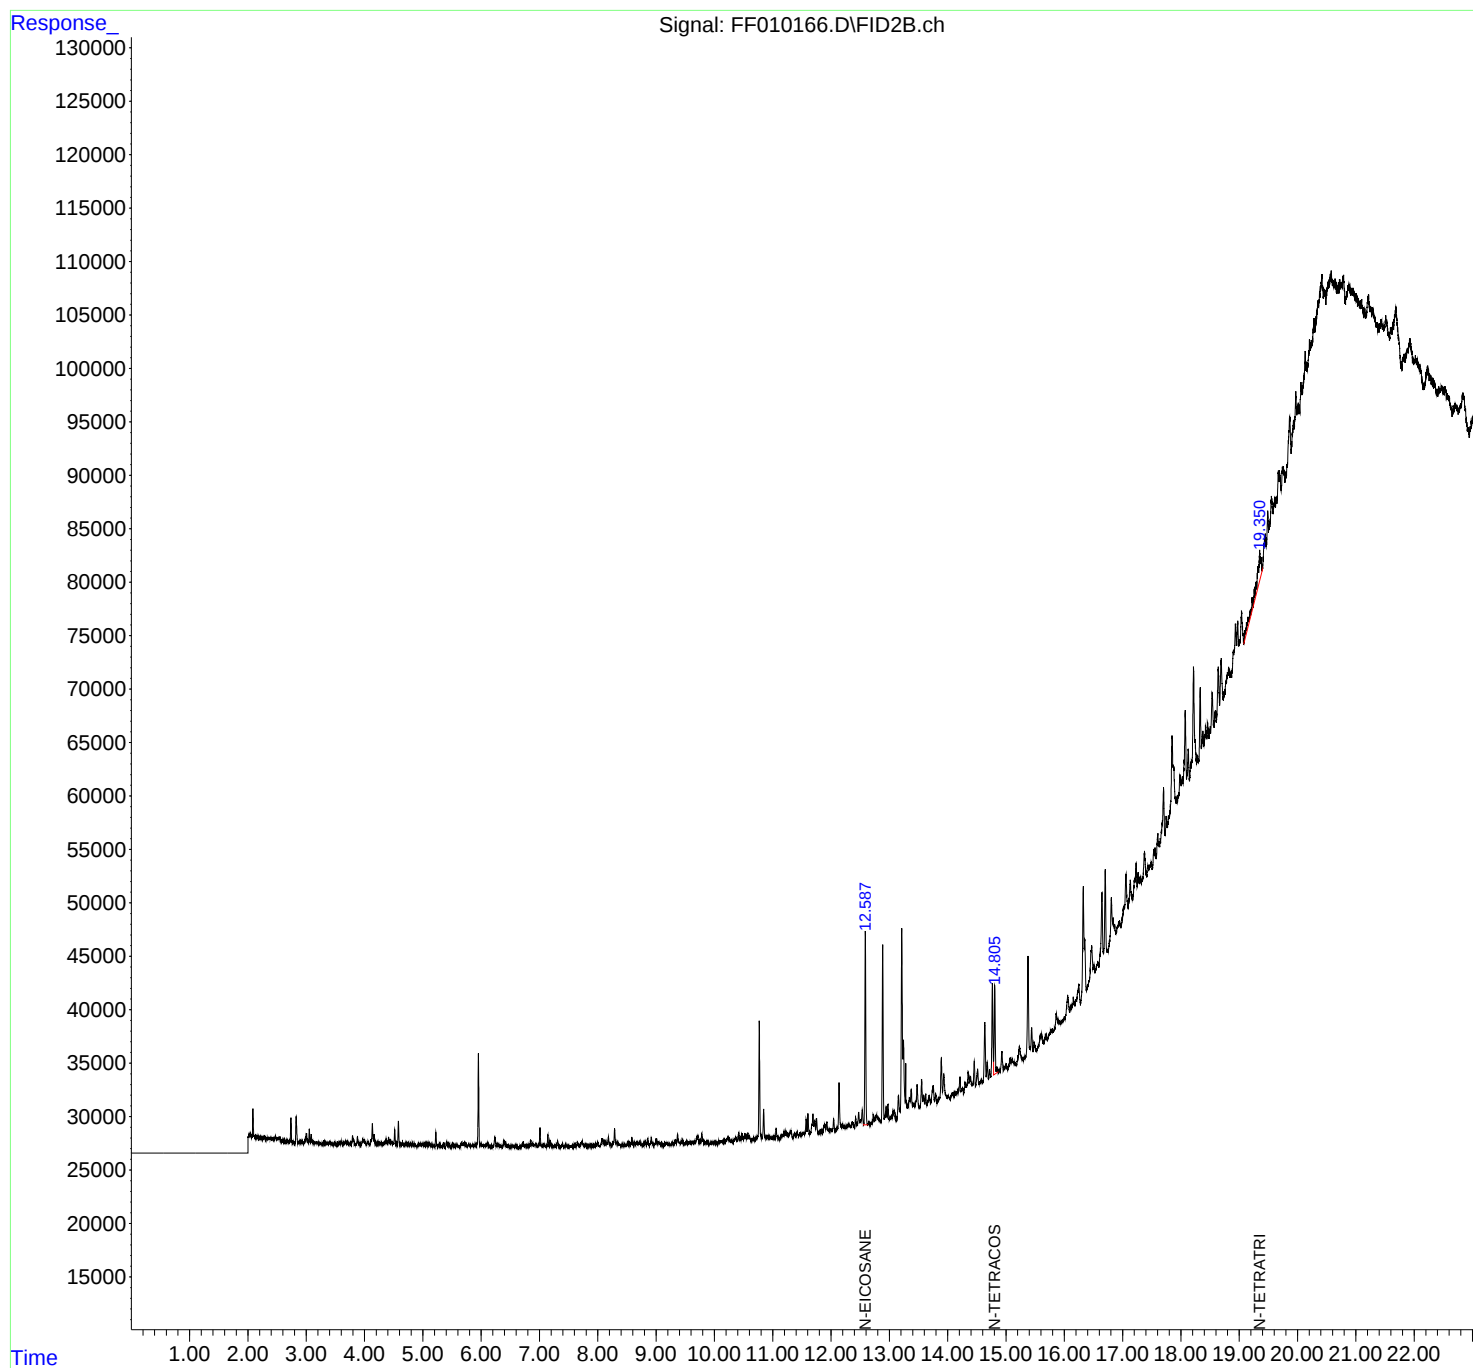


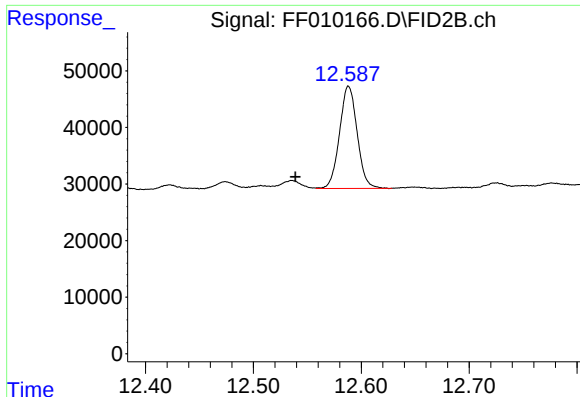

#7 N-EICOSANE


R.T.: 12.588 min
Delta R.T.: 0.050 min
Response: 205257
Conc: 1.47 ug/ml

Instrument :
FID_F
ClientSampleId :

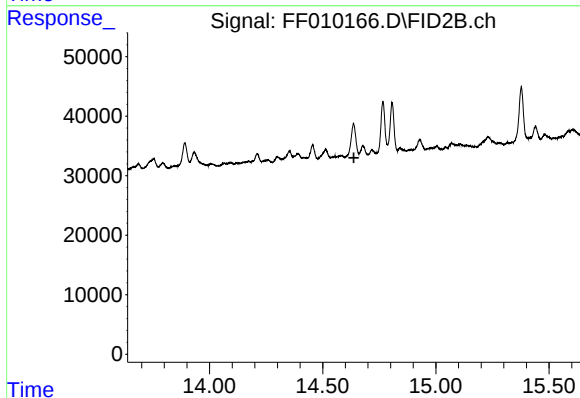


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 0.000 min
Exp R.T. : 14.638 min
Response: 0
Conc: N.D.

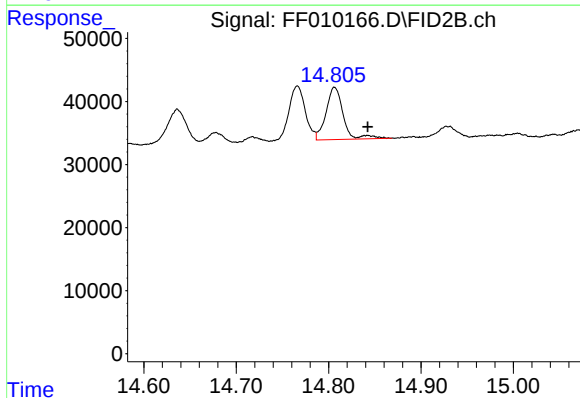

#10 N-TETRACOSANE

R.T.: 14.807 min
Delta R.T.: -0.036 min
Response: 106866
Conc: 0.78 ug/ml

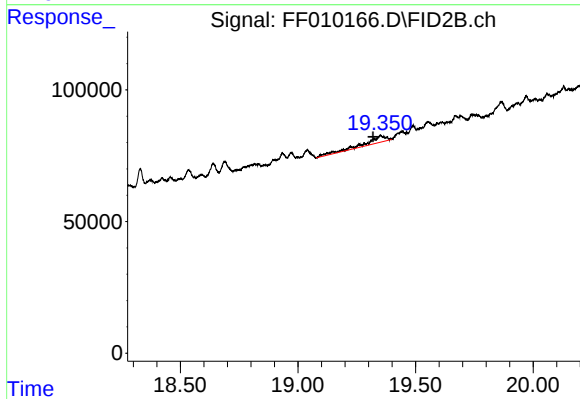

#15 N-TETRATRIACONTANE

R.T.: 19.351 min
Delta R.T.: 0.032 min
Response: 164712
Conc: 1.52 ug/ml