

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
 Data File : FF010168.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2022 22:38
 Operator : AJ\MA
 Sample : N1958-05 20X
 Misc :
 ALS Vial : 77 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 01:04:10 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
 Quant Title :
 QLast Update : Sat Mar 26 09:58:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	99934	0.818 ug/ml
Target Compounds			
7) N-EICOSANE	12.589f	360272	2.577 ug/ml
10) N-TETRACOSANE	14.807	173665	1.270 ug/ml
12) N-OCTACOSANE	16.809	49533	0.377 ug/ml
15) N-TETRATRIACONTANE	19.354	124326	1.151 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010168.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 22:38
Operator : AJ\MA
Sample : N1958-05 20X
Misc :
ALS Vial : 77 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 27 01:04:10 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

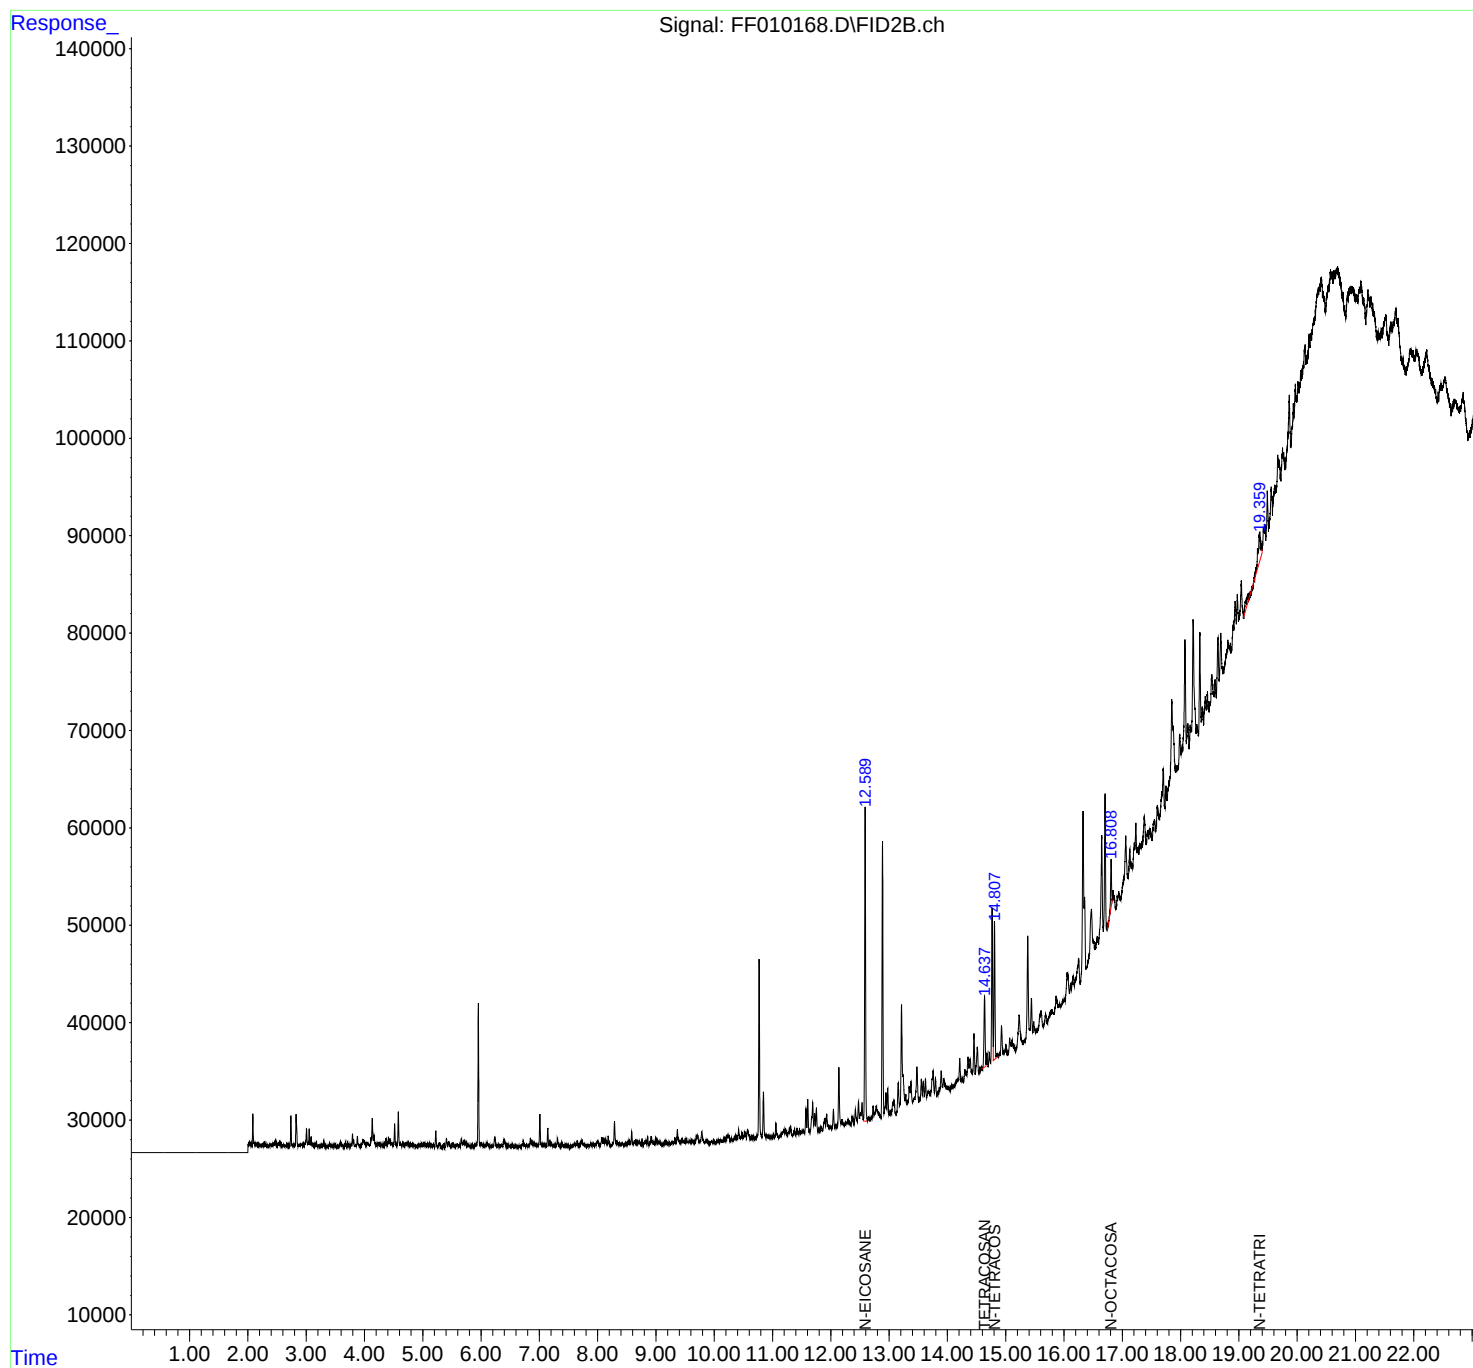


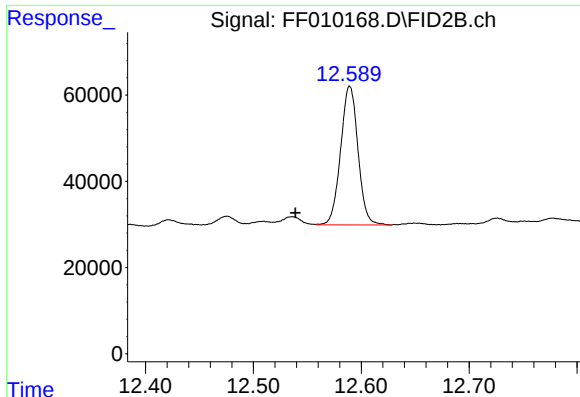

#7 N-EICOSANE


R.T.: 12.589 min
Delta R.T.: 0.051 min
Response: 360272
Conc: 2.58 ug/ml

Instrument :
FID_F
ClientSampleId :

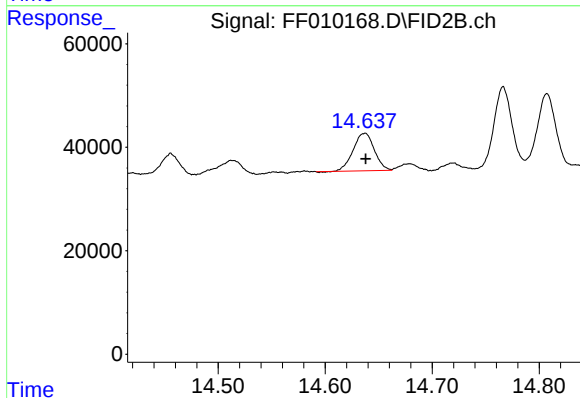


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: -0.001 min
Response: 99934
Conc: 0.82 ug/ml

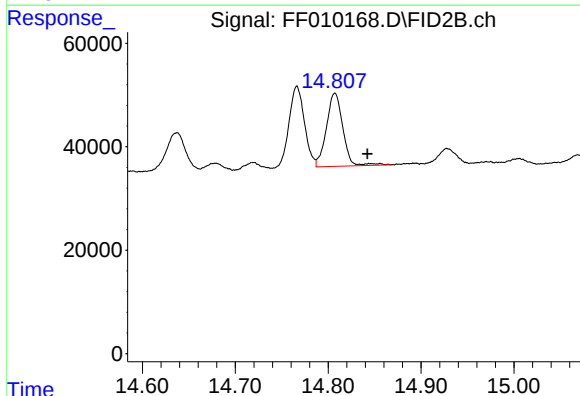


#10 N-TETRACOSANE

R.T.: 14.807 min
Delta R.T.: -0.035 min
Response: 173665
Conc: 1.27 ug/ml

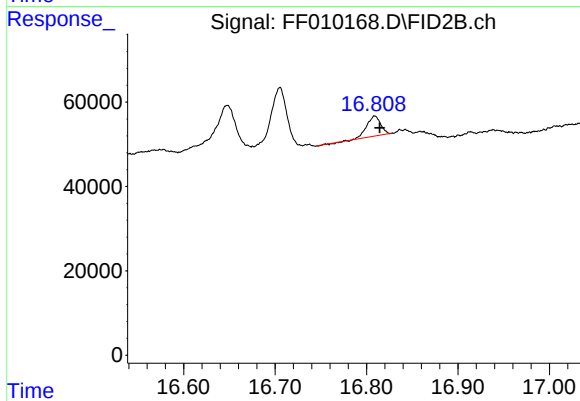

#12 N-OCTACOSANE

R.T.: 16.809 min
Delta R.T.: -0.005 min
Response: 49533
Conc: 0.38 ug/ml

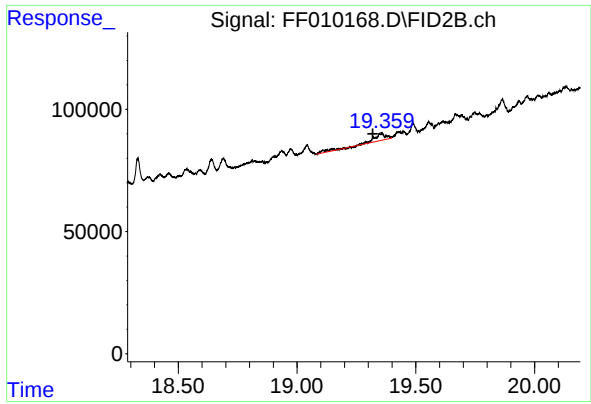

#15 N-TETRATRIACONTANE

R.T.: 19.354 min
Delta R.T.: 0.035 min
Response: 124326
Conc: 1.15 ug/ml

Instrument :
FID_F
ClientSampleId :