

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
 Data File : FF010169.D
 Signal(s) : FID2B.ch
 Acq On : 26 Mar 2022 23:08
 Operator : AJ\MA
 Sample : N1958-06 20X
 Misc :
 ALS Vial : 78 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 01:04:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
 Quant Title :
 QLast Update : Sat Mar 26 09:58:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.637	136558	1.118 ug/ml
Target Compounds			
7) N-EICOSANE	12.589f	687613	4.918 ug/ml
10) N-TETRACOSANE	14.808	292115	2.136 ug/ml
12) N-OCTACOSANE	16.809	205823	1.565 ug/ml
13) N-TRIACONTANE	17.703	115651	0.903 ug/ml
15) N-TETRATRIACONTANE	19.323	137819	1.276 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010169.D
Signal(s) : FID2B.ch
Acq On : 26 Mar 2022 23:08
Operator : AJ\MA
Sample : N1958-06 20X
Misc :
ALS Vial : 78 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 27 01:04:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

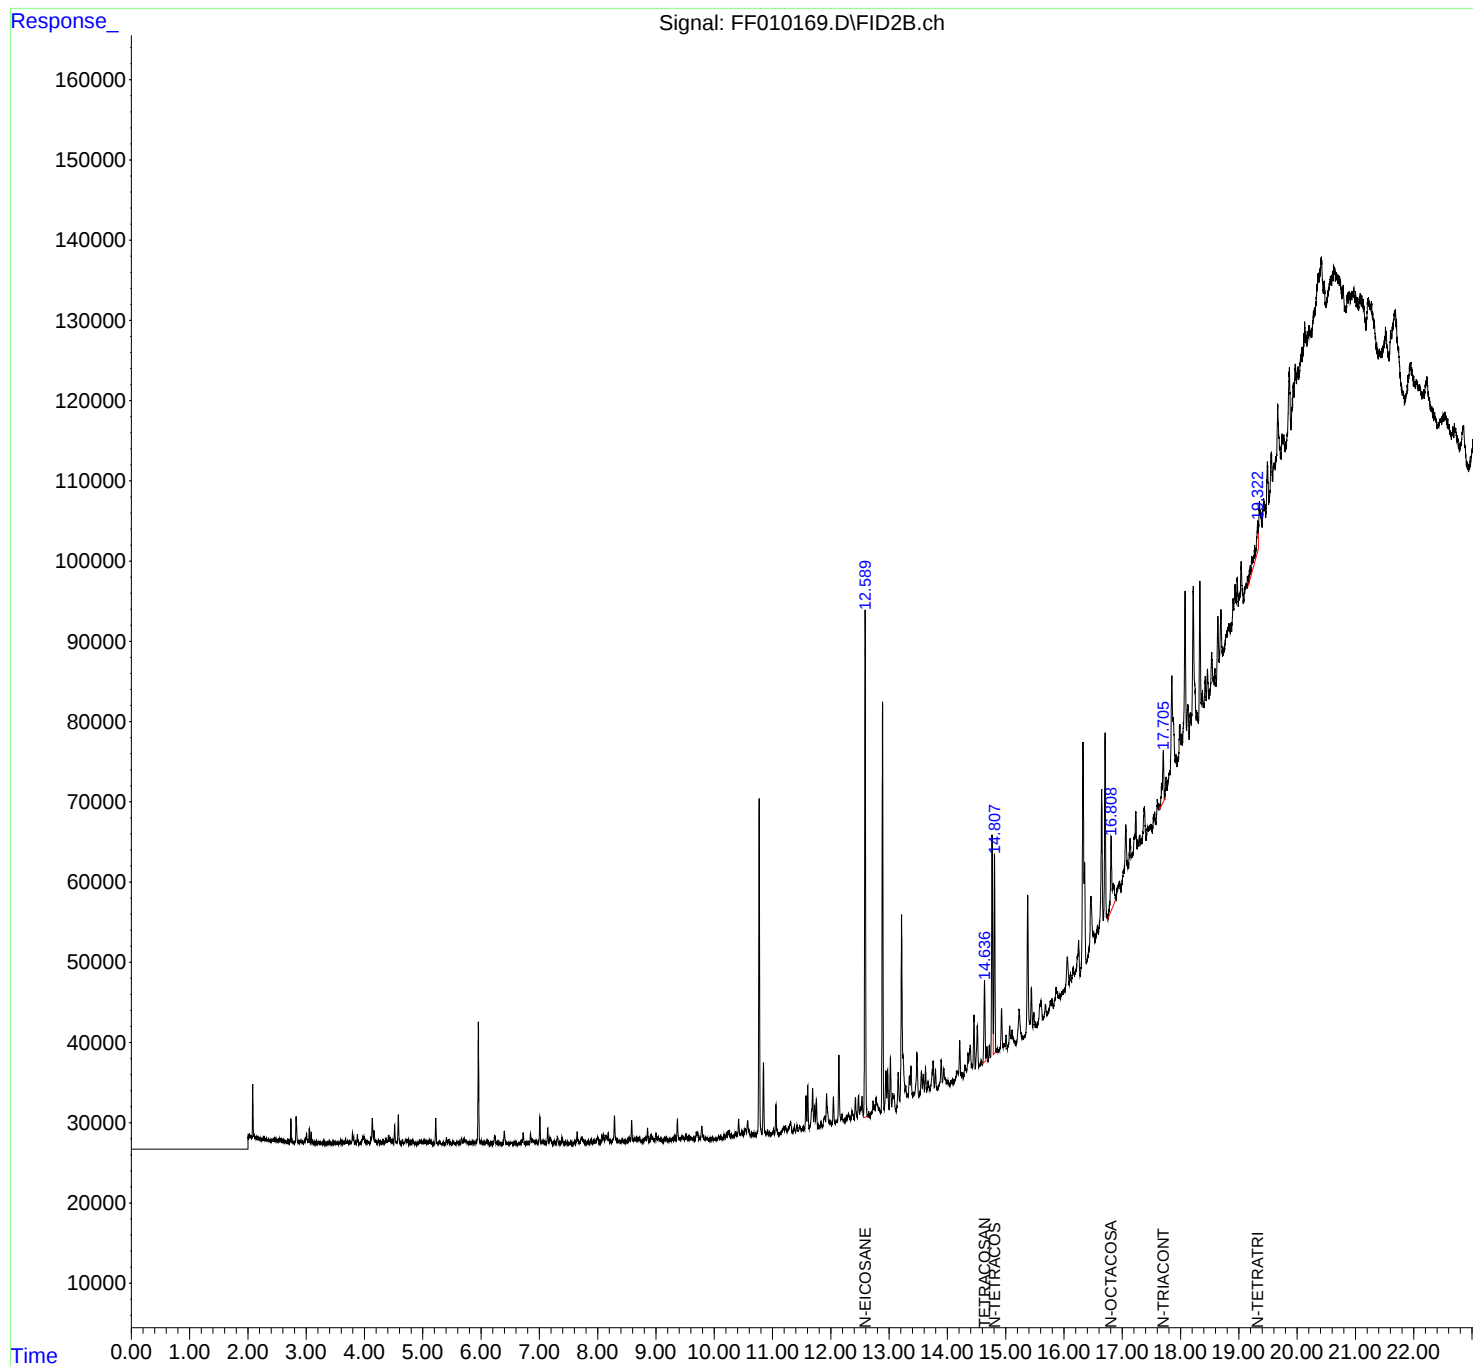


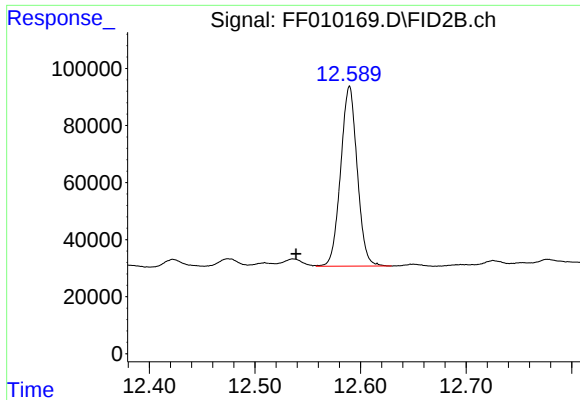

#7 N-EICOSANE


R.T.: 12.589 min
Delta R.T.: 0.051 min
Response: 687613
Conc: 4.92 ug/ml

Instrument :
FID_F
ClientSampleId :

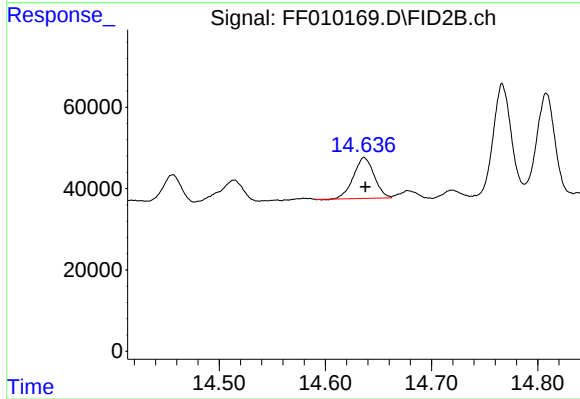


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.637 min
Delta R.T.: -0.001 min
Response: 136558
Conc: 1.12 ug/ml

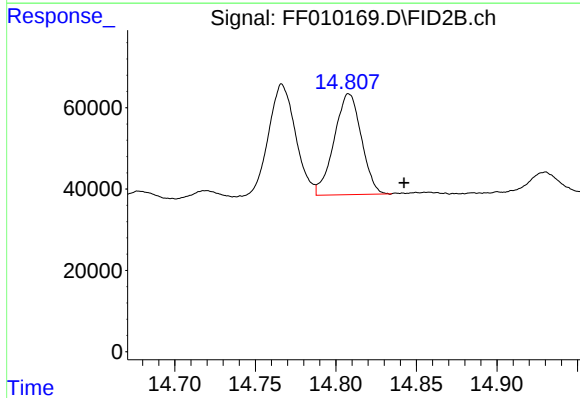


#10 N-TETRACOSANE

R.T.: 14.808 min
Delta R.T.: -0.034 min
Response: 292115
Conc: 2.14 ug/ml

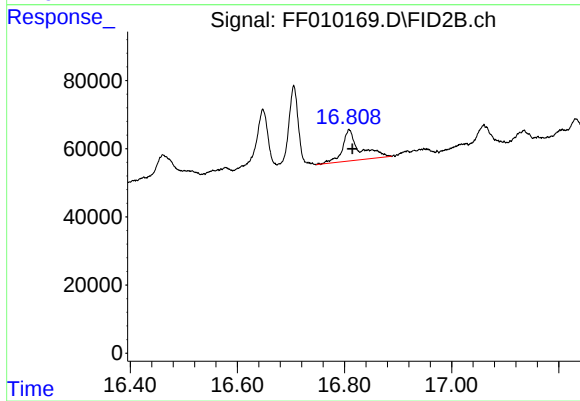

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.006 min
Response: 205823
Conc: 1.56 ug/ml

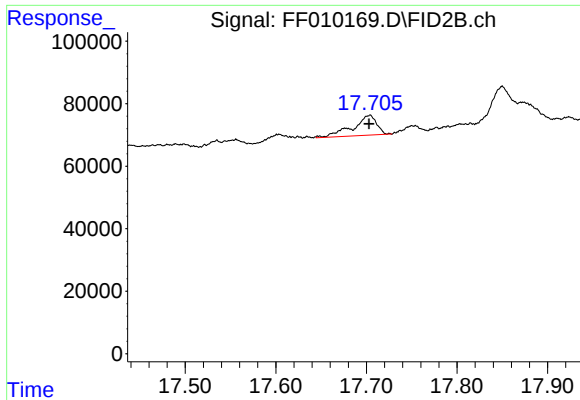

#13 N-TRIACONTANE

R.T.: 17.703 min
Delta R.T.: 0.000 min
Response: 115651
Conc: 0.90 ug/ml

Instrument :
FID_F
ClientSampleId :

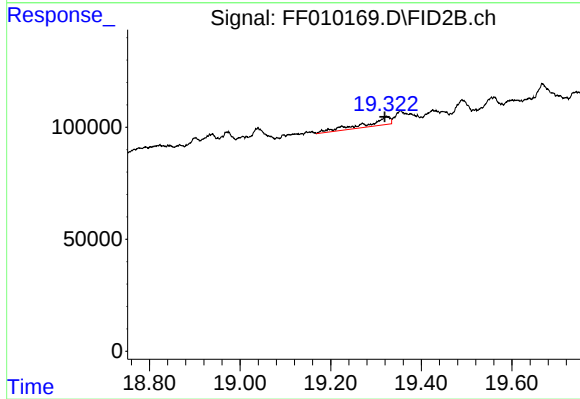

#15 N-TETRATRIACONTANE

R.T.: 19.323 min
Delta R.T.: 0.004 min
Response: 137819
Conc: 1.28 ug/ml