

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
 Data File : FF010171.D
 Signal(s) : FID2B.ch
 Acq On : 27 Mar 2022 00:09
 Operator : AJ\MA
 Sample : N1958-08 20X
 Misc :
 ALS Vial : 80 Sample Multiplier: 1

Instrument :
 FID_F
 ClientSampleId :

Integration File: autoint1.e
 Quant Time: Mar 27 01:04:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
 Quant Title :
 QLast Update : Sat Mar 26 09:58:43 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1uL
 Signal Phase : Rxi-1ms
 Signal Info : 20mx0.18mmx0.18um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
9) S TETRACOSANE-d50 (SURR...	14.638	178536	1.462 ug/ml
Target Compounds			
7) N-EICOSANE	12.593f	2658885	19.016 ug/ml
8) N-DOCOSANE	13.755	266173	1.932 ug/ml
10) N-TETRACOSANE	14.811	981135	7.173 ug/ml
12) N-OCTACOSANE	16.809	367058	2.790 ug/ml
13) N-TRIACONTANE	17.704	278978	2.177 ug/ml
15) N-TETRATRIACONTANE	19.354	100647	0.932 ug/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_F\Data\FF032622\
Data File : FF010171.D
Signal(s) : FID2B.ch
Acq On : 27 Mar 2022 00:09
Operator : AJ\MA
Sample : N1958-08 20X
Misc :
ALS Vial : 80 Sample Multiplier: 1

Instrument :
FID_F
ClientSampleId :

Integration File: autoint1.e
Quant Time: Mar 27 01:04:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_F\Method\FF032622.M
Quant Title :
QLast Update : Sat Mar 26 09:58:43 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1uL
Signal Phase : Rxi-1ms
Signal Info : 20mx0.18mmx0.18um

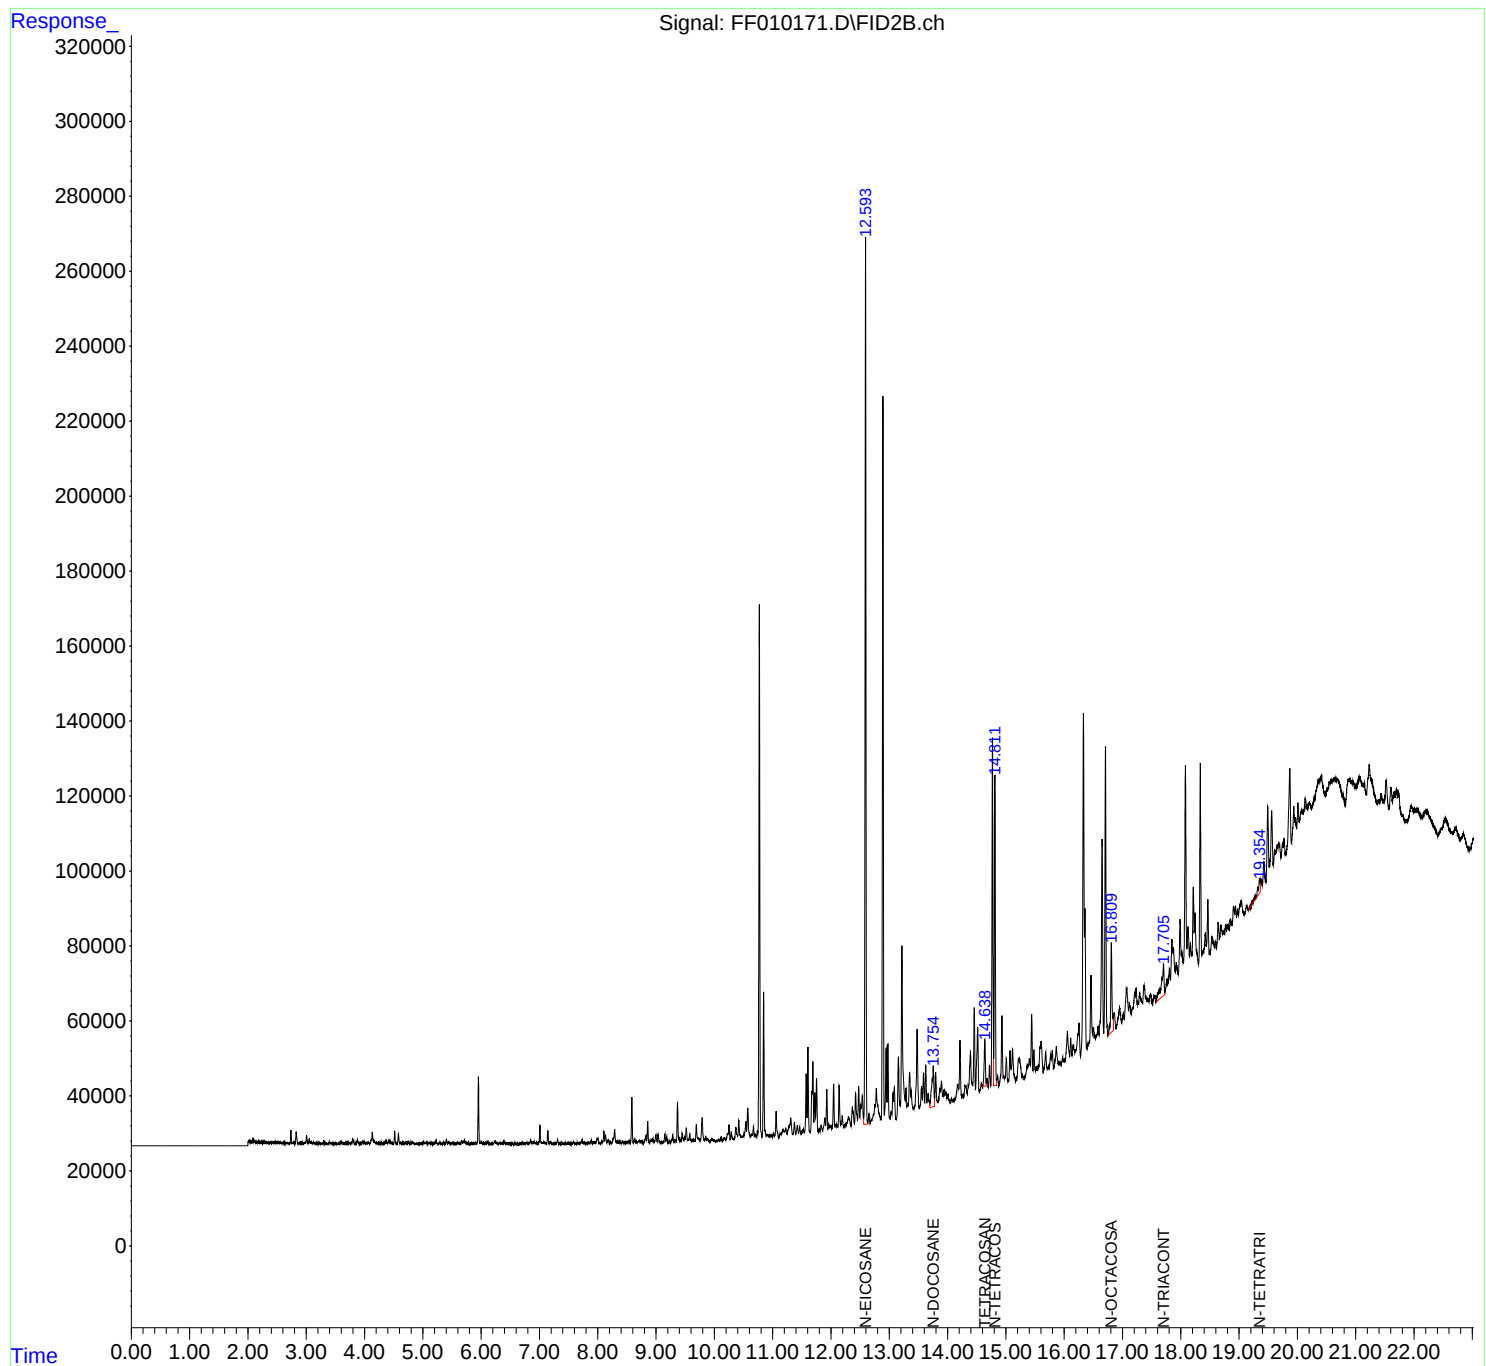


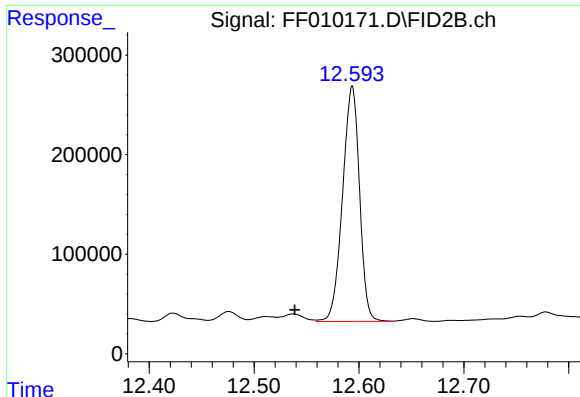

#7 N-EICOSANE


R.T.: 12.593 min
Delta R.T.: 0.055 min
Response: 2658885
Conc: 19.02 ug/ml

Instrument :
FID_F
ClientSampleId :

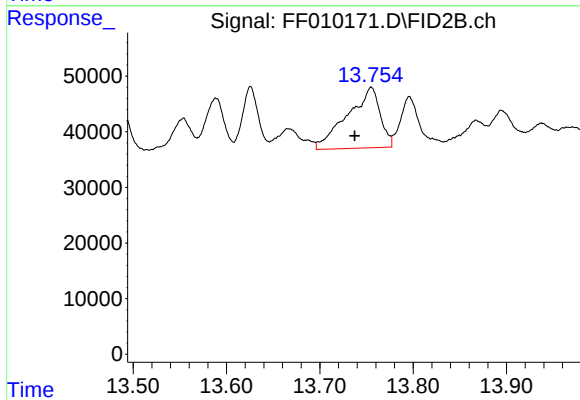


#8 N-DOCOSANE

R.T.: 13.755 min
Delta R.T.: 0.017 min
Response: 266173
Conc: 1.93 ug/ml

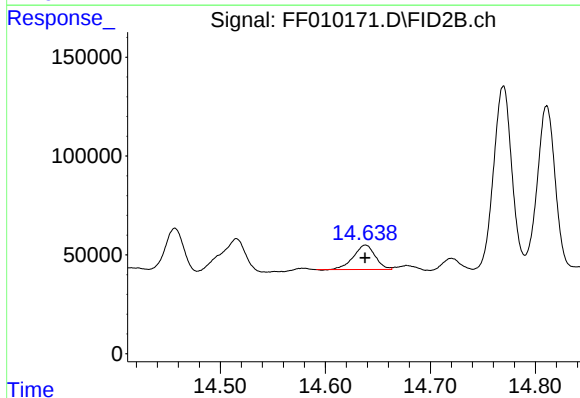


#9 TETRACOSANE-d50 (SURROGATE)

R.T.: 14.638 min
Delta R.T.: 0.000 min
Response: 178536
Conc: 1.46 ug/ml

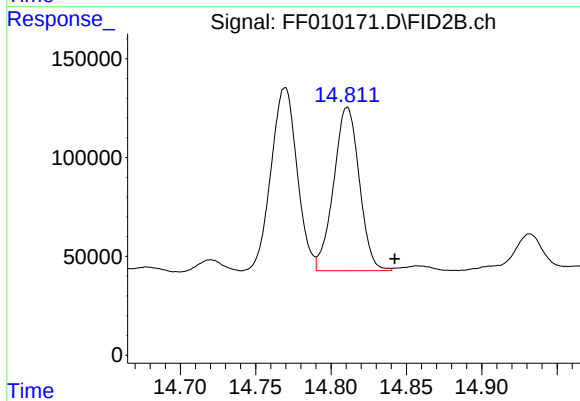

#10 N-TETRACOSANE


R.T.: 14.811 min
Delta R.T.: -0.031 min
Response: 981135
Conc: 7.17 ug/ml

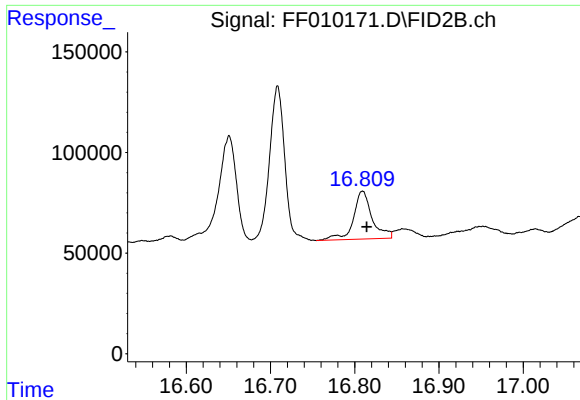

#12 N-OCTACOSANE


R.T.: 16.809 min
Delta R.T.: -0.005 min
Response: 367058
Conc: 2.79 ug/ml

Instrument :
FID_F
ClientSampleId :

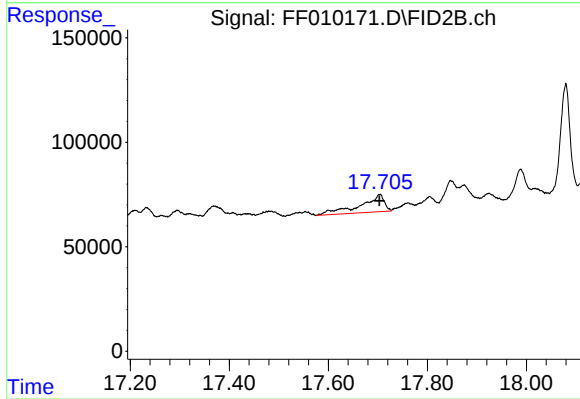

#13 N-TRIACONTANE

R.T.: 17.704 min
Delta R.T.: 0.000 min
Response: 278978
Conc: 2.18 ug/ml

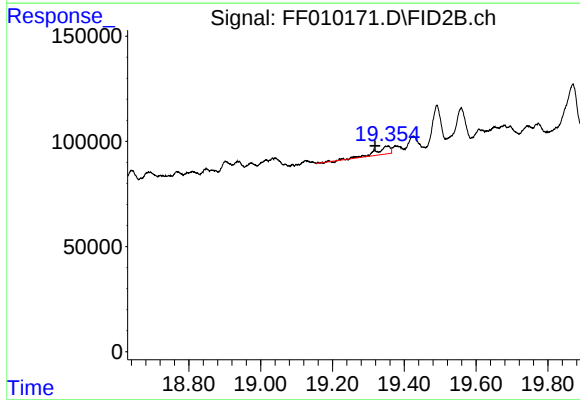

#15 N-TETRATRIACONTANE

R.T.: 19.354 min
Delta R.T.: 0.035 min
Response: 100647
Conc: 0.93 ug/ml